


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122718\
 Data File : BM018416.D
 Acq On : 28 Dec 2018 03:39
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM122718.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 27 14:18:47 2018

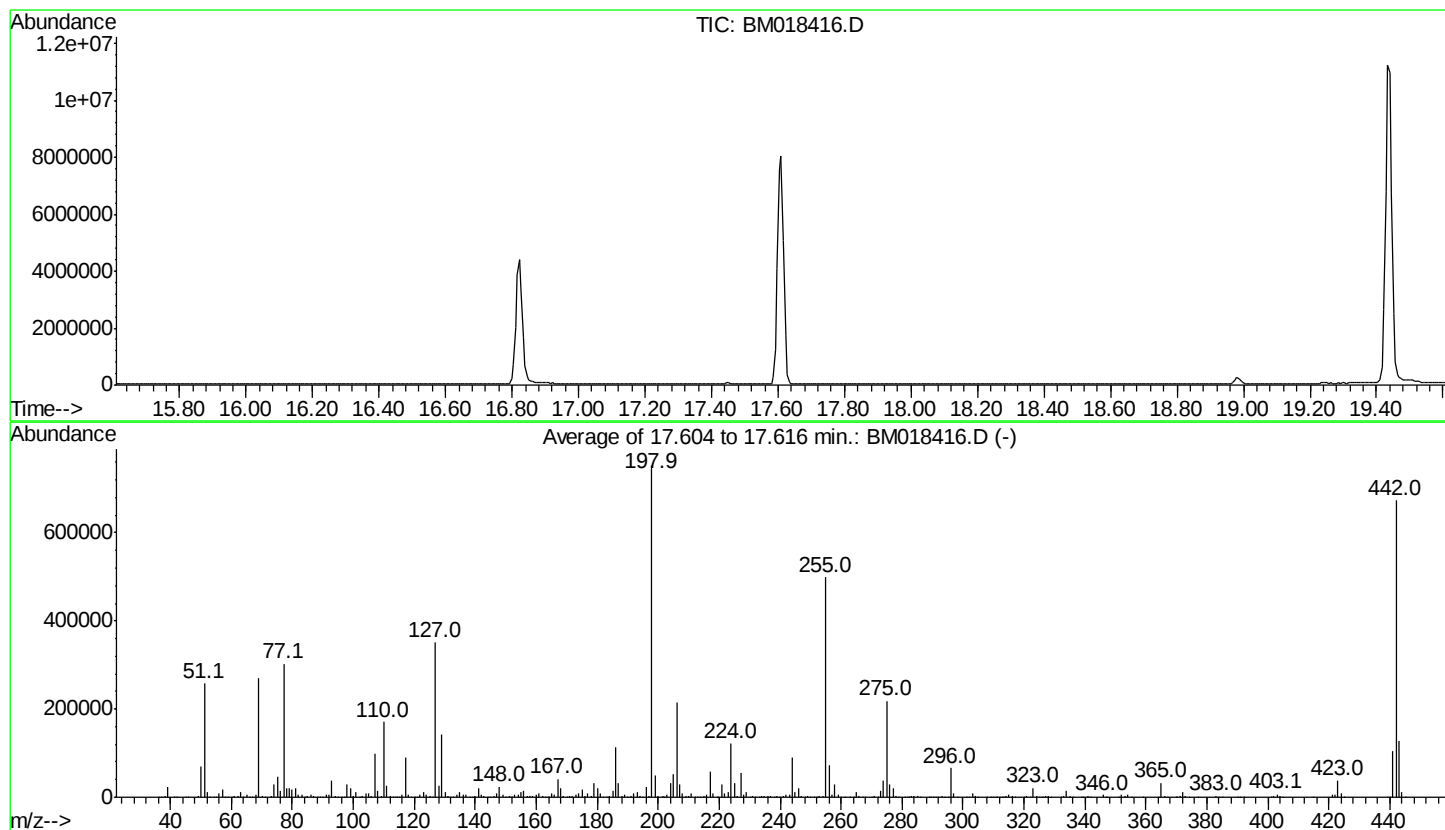

AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	257365	PASS
68	69	0.00	2	1.9	5147	PASS
69	198	0.00	100	36.0	271281	PASS
70	69	0.00	2	0.7	1896	PASS
127	198	10	80	46.6	350954	PASS
197	198	0.00	2	0.6	4238	PASS
198	198	100	100	100.0	752554	PASS
199	198	5	9	6.6	49384	PASS
275	198	10	60	29.1	218730	PASS
365	198	1	100	4.4	33274	PASS
441	198	0.01	100	14.1	106112	PASS
442	198	50	100	89.4	673109	PASS
443	442	15	24	19.0	127746	PASS