

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122819\
 Data File : BM024347.D
 Acq On : 28 Dec 2019 13:48
 Operator : JU
 Sample : K6278--07
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Dec 29 00:52:44 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 29 00:45:10 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.41	152	225215	20.00	ng/ul	0.00
18) Naphthalene-d8	10.18	136	977753	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	575291	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.83	188	1163728	20.00	ng/ul	0.00
78) Chrysene-d12	21.05	240	1126702	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	1405978	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.99	96	17363	3.41	ng/uL	0.01
5) Phenol-d5	6.62	99	254085	11.92	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.77	67	196357	15.35	ng/ul	0.00
9) 2-Chlorophenol-d4	6.95	132	207308	13.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.15	113	144175	8.27	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	96302	13.71	ng/ul	0.00
22) 2-Nitrophenol-d4	9.29	143	102786	13.31	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	164193	10.93	ng/ul	0.00
29) 4-Chloroaniline-d4	10.35	131	185983	10.20	ng/ul	0.00
44) Dimethylphthalate-d6	13.50	166	632382	14.87	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	626656	12.29	ng/ul	0.00
52) 4-Nitrophenol-d4	14.36	143	42589	5.58	ng/ul	0.02
58) Fluorene-d10	15.08	176	503551	13.50	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	44629	6.29	ng/ul	0.00
71) Anthracene-d10	16.93	188	715419	13.51	ng/ul	0.00
79) Pyrene-d10	19.24	212	806920	15.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	946363	13.55	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.65	94	32855	1.492	ng/ul# 87
45) Dimethylphthalate	13.55	163	102865	2.327	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122819\
Data File : BM024347.D
Acq On : 28 Dec 2019 13:48
Operator : JU
Sample : K6278--07
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Dec 29 00:52:44 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 29 00:45:10 2019
Response via : Initial Calibration

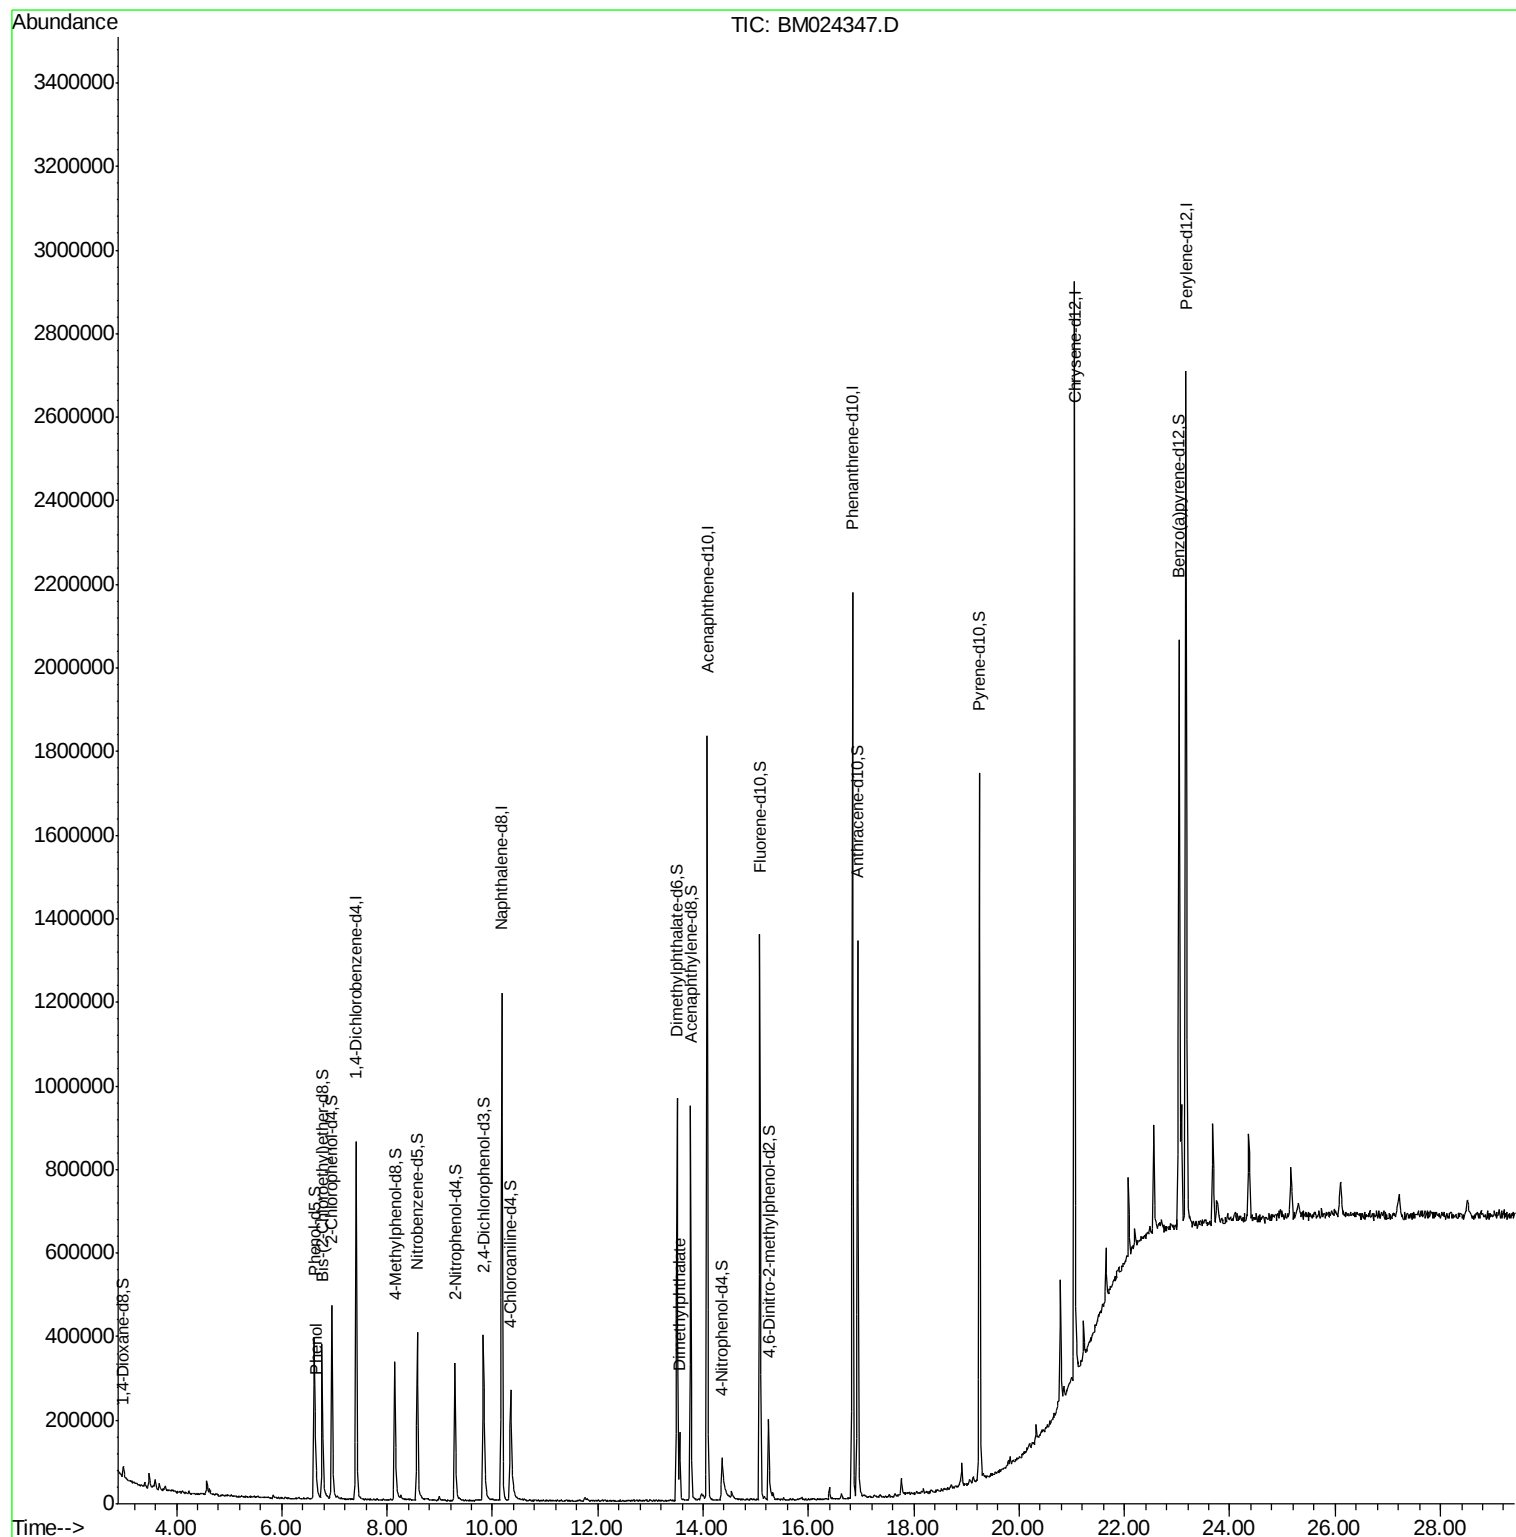

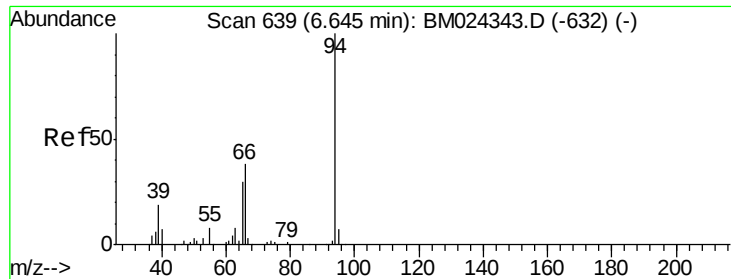

#6

Phenol

Concen: 1.492 ng/ul

RT: 6.65 min Scan# 639

Delta R.T. 0.00 min

Lab File: BM024347.D

Acq: 28 Dec 2019 13:48

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 94 Resp: 32855

Ion Ratio Lower Upper

94 100

65 34.2 22.6 33.8#




66 46.9 30.7 46.1#

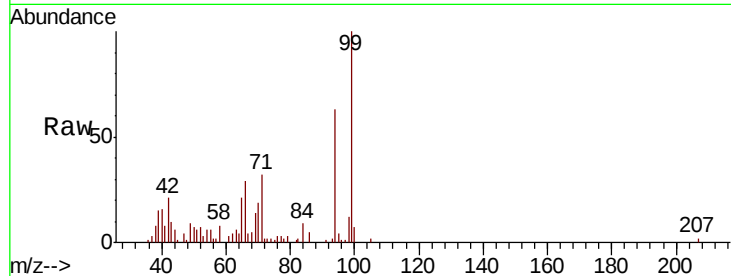

Abundance Ion 94.00 (93.70 to 94.70): BM024347.D (-632) (-)

Ion 65.00 (64.70 to 65.70): BM024347.D (-632) (-)

Ion 66.00 (65.70 to 66.70): BM024347.D (-632) (-)

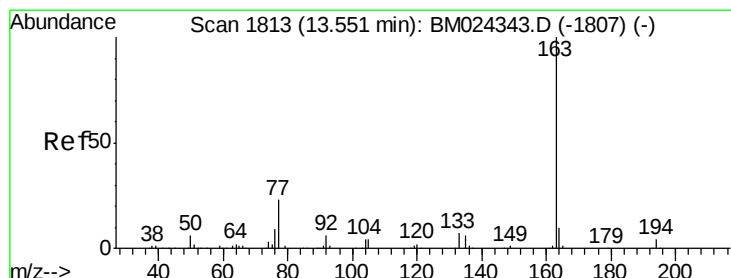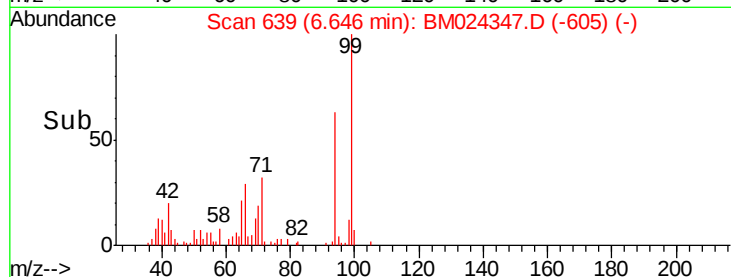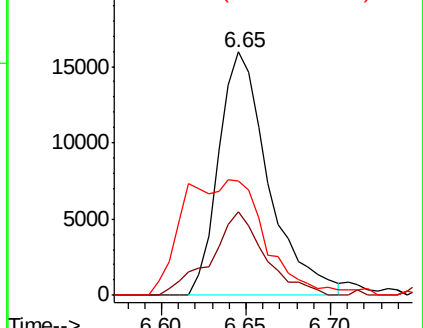

#45

Dimethylphthalate

Concen: 2.327 ng/ul

RT: 13.55 min Scan# 1813

Delta R.T. 0.00 min

Lab File: BM024347.D

Acq: 28 Dec 2019 13:48


Tgt Ion:163 Resp: 102865

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 10.5 7.8 11.6

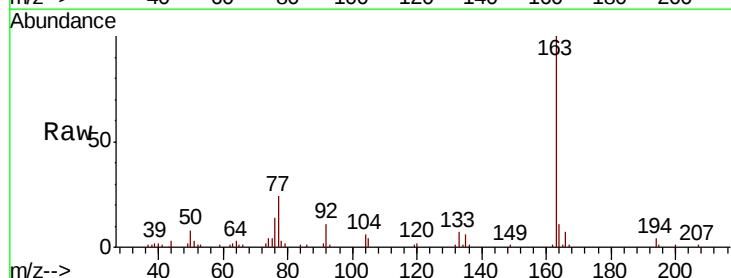

Abundance Ion 163.00 (162.70 to 163.70): BM024347.D (-1807) (-)

Ion 194.00 (193.70 to 194.70): BM024347.D (-1807) (-)

Ion 164.00 (163.70 to 164.70): BM024347.D (-1807) (-)

