

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122819\
 Data File : BM024362.D
 Acq On : 28 Dec 2019 22:47
 Operator : JU
 Sample : K6278-04
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0C46

Manual Integrations
 APPROVED

mohammad
 12/29/2019 5:30:13 PM

Quant Time: Dec 29 02:04:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sun Dec 29 01:30:05 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.41	152	241923	20.00	ng/ul	0.00
18) Naphthalene-d8	10.17	136	993016	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.07	164	574699	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.83	188	1171263	20.00	ng/ul	0.00
78) Chrysene-d12	21.05	240	1149093	20.00	ng/ul	0.00
86) Perylene-d12	23.17	264	1389338	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	2.99	96	23545	4.30	ng/uL	0.01
5) Phenol-d5	6.62	99	329003	14.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.77	67	256306	18.66	ng/ul	0.00
9) 2-Chlorophenol-d4	6.95	132	273342	16.73	ng/ul	0.00
13) 4-Methylphenol-d8	8.14	113	202225	10.80	ng/ul	0.00
19) Nitrobenzene-d5	8.57	128	135989	19.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.28	143	149926	19.11	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.83	165	246101	16.14	ng/ul	0.00
29) 4-Chloroaniline-d4	10.34	131	217081	11.72	ng/ul	0.00
44) Dimethylphthalate-d6	13.50	166	840195	19.77	ng/ul	0.00
47) Acenaphthylene-d8	13.76	160	909438	17.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	80385	10.54	ng/ul	0.02
58) Fluorene-d10	15.08	176	702218	18.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	62414	8.74	ng/ul	0.00
71) Anthracene-d10	16.93	188	979435	18.38	ng/ul	0.00
79) Pyrene-d10	19.24	212	1061985	19.40	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.04	264	1216646	17.63	ng/ul	0.00

Target Compounds

					Ovalue
6) Phenol	6.65	94	46197	1.953 ng/ul	95
45) Dimethylphthalate	13.55	163	112732	2.552 ng/ul	100
70) Phenanthrene	16.87	178	193954	2.958 ng/ul	99
77) Fluoranthene	18.91	202	503356	7.043 ng/ul	99
80) Pyrene	19.27	202	426836	5.690 ng/ul	98
83) Benzo(a)anthracene	21.03	228	266258	3.637 ng/ul	97
85) Chrysene	21.09	228	257275	3.585 ng/ul	95
88) Benzo(b)fluoranthene	22.55	252	377693	4.543 ng/ul#	92
89) Benzo(k)fluoranthene	22.59	252	137570m	1.687 ng/ul	
91) Benzo(a)pyrene	23.08	252	239391	3.183 ng/ul#	90
92) Indeno(1,2,3-cd)pyrene	25.27	276	175251	1.941 ng/ul#	94
94) Benzo(g,h,i)perylene	25.90	276	132154	1.792 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM122819\
Data File : BM024362.D
Acq On : 28 Dec 2019 22:47
Operator : JU
Sample : K6278-04
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0C46

Manual Integrations
APPROVED

mohammad
12/29/2019 5:30:13 PM

Quant Time: Dec 29 02:04:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sun Dec 29 01:30:05 2019
Response via : Initial Calibration

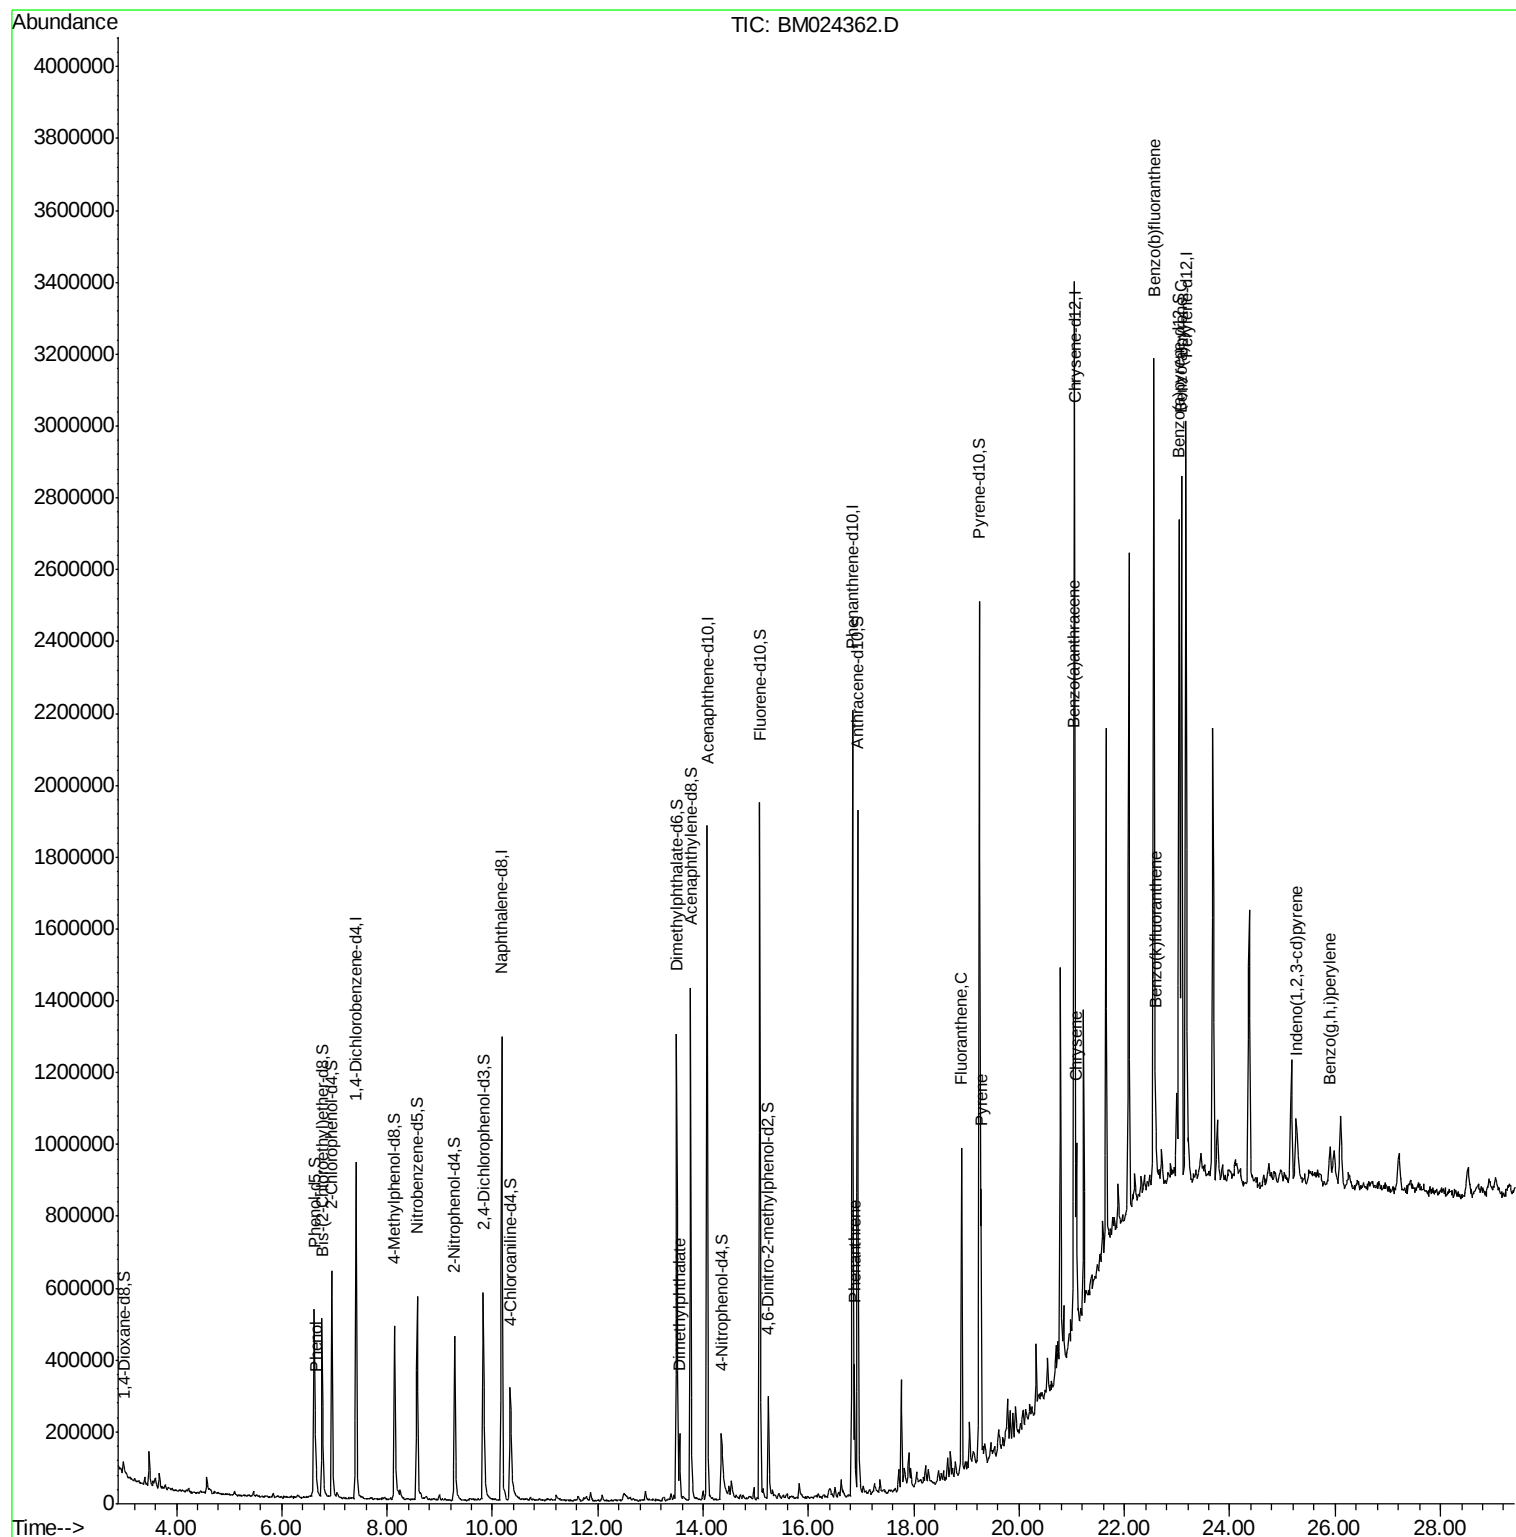

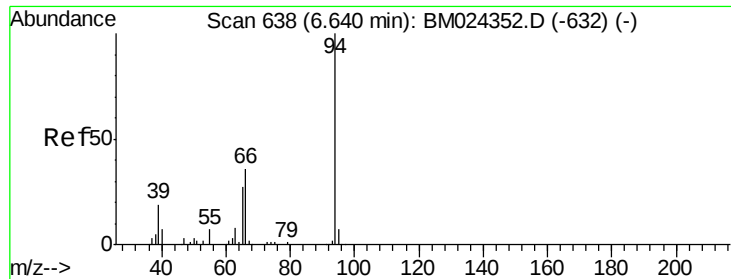

#6

Phenol





Concen: 1.953 ng/ul
 RT: 6.65 min Scan# 639
 Delta R.T. 0.01 min
 Lab File: BM024362.D
 Acq: 28 Dec 2019 22:47

Instrument :
 BNA_M
 ClientSampleId :
 C0C46

Tot Ion	Ratio	Lower	Upper
94	100		
65	27.5	22.6	33.8
66	43.0	30.7	46.1

Manual Integrations
 APPROVED

mohammad
 12/29/2019 5:30:13 PM

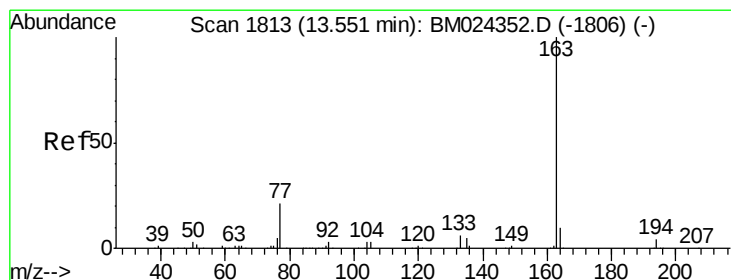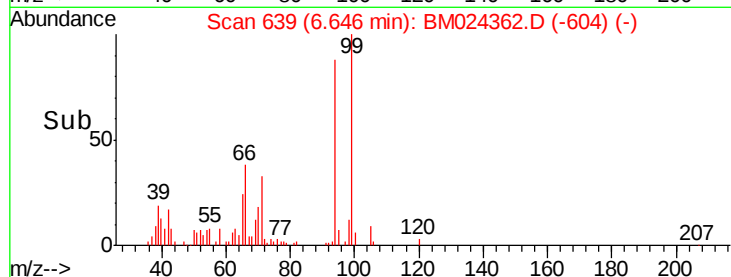
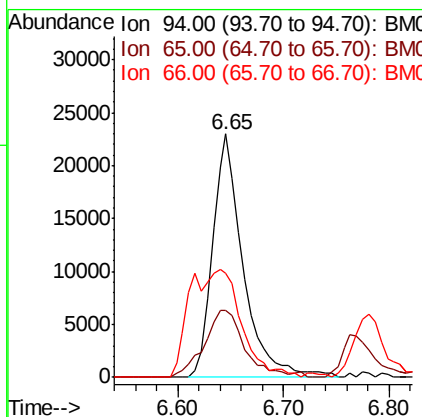
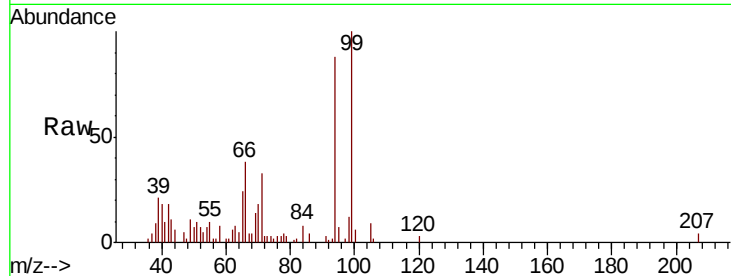



#45

Dimethylphthalate

Concen: 2.552 ng/ul
 RT: 13.55 min Scan# 1813
 Delta R.T. 0.00 min
 Lab File: BM024362.D
 Acq: 28 Dec 2019 22:47

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.2	3.2	4.8
164	9.7	7.8	11.6

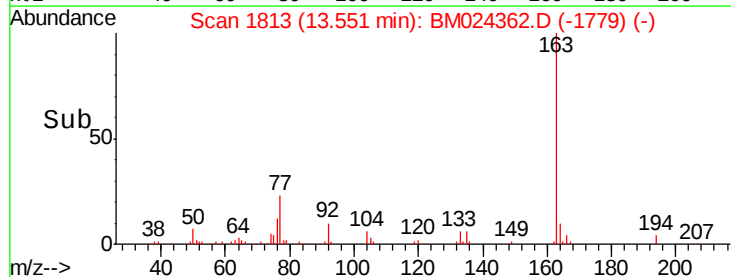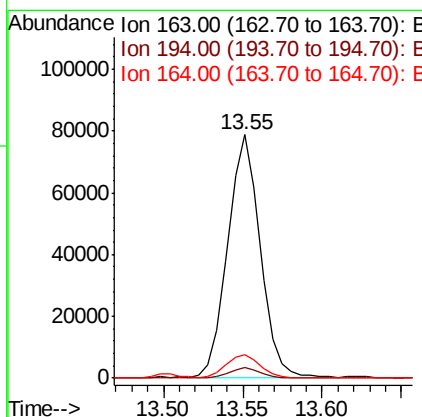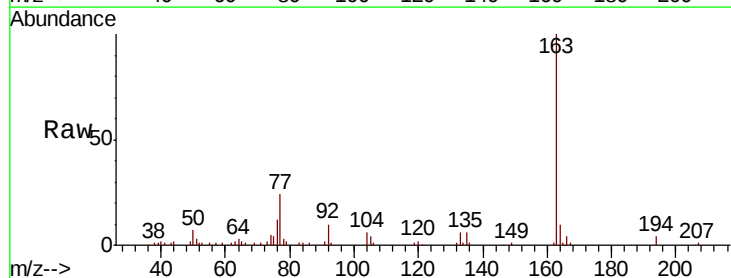

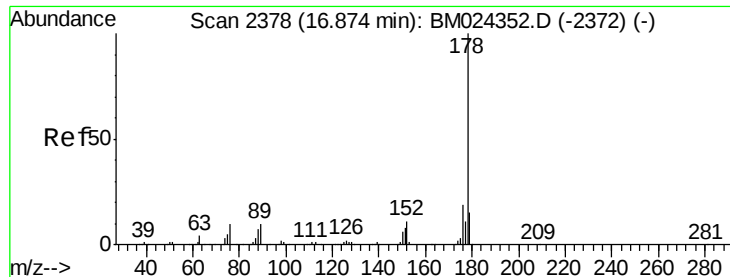


#70
Phenanthrene
Concen: 2.958 ng/ul
RT: 16.87 min Scan# 2378
Delta R.T. 0.00 min
Lab File: BM024362.D
Acq: 28 Dec 2019 22:47

Instrument :
BNA_M
ClientSampleId :
C0C46

Tot Ion	Ratio	Lower	Upper
178	100		
179	15.9	12.6	19.0
176	18.5	15.1	22.7

Manual Integrations
APPROVED

mohammad
12/29/2019 5:30:13 PM



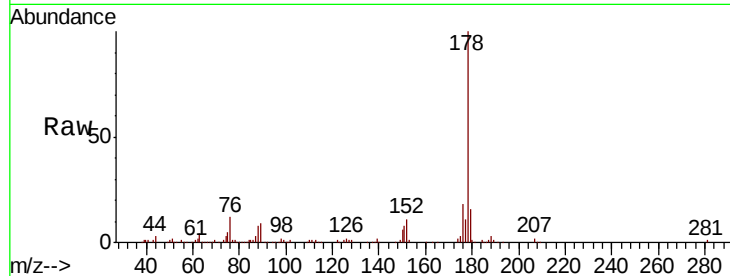


Abundance

Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

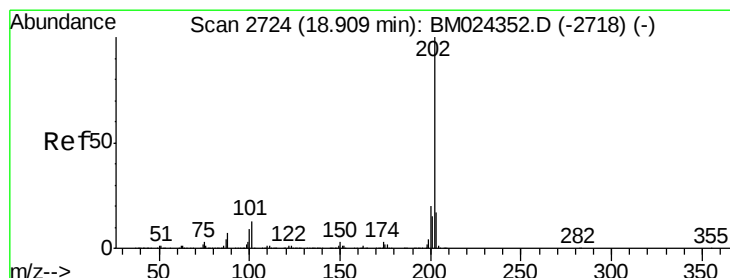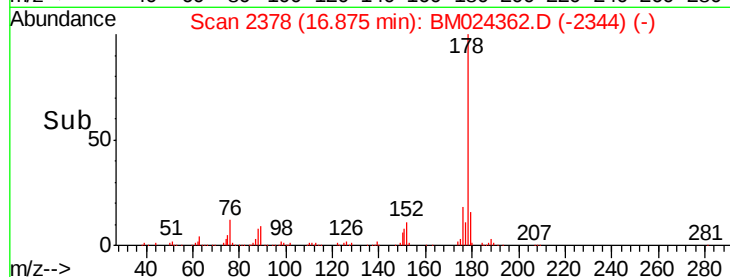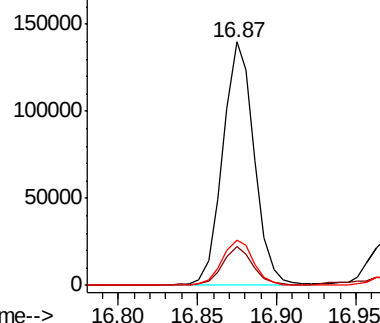

#77
Fluoranthene
Concen: 7.043 ng/ul
RT: 18.91 min Scan# 2724
Delta R.T. 0.00 min
Lab File: BM024362.D
Acq: 28 Dec 2019 22:47




Tgt Ion	Ratio	Lower	Upper
202	100		
101	12.9	10.6	15.8
100	9.5	8.1	12.1


Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

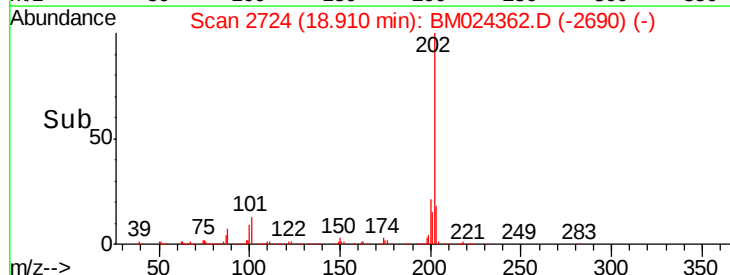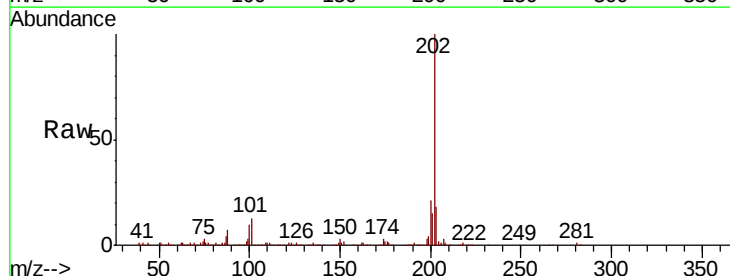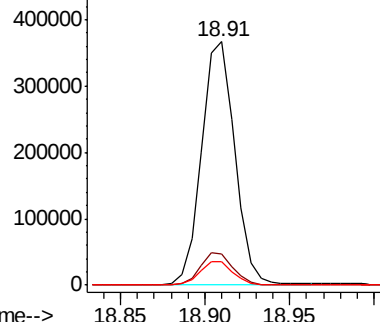

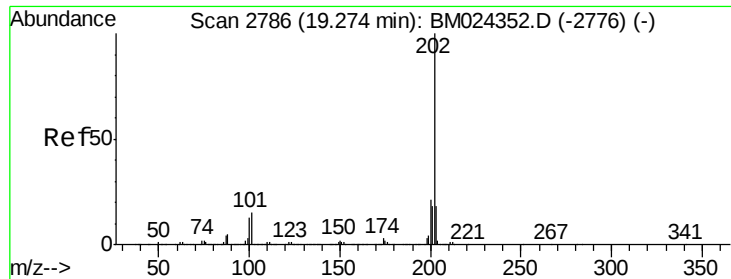





#80
Pvrene
Concen: 5.690 ng/ul
RT: 19.27 min Scan# 2786
Delta R.T. 0.00 min
Lab File: BM024362.D
Acq: 28 Dec 2019 22:47

Instrument :
BNA_M
ClientSampleId :
C0C46

Tot Ion	Ratio	Resp Lower	Upper
202	100		
101	14.0	12.2	18.4
100	12.6	10.0	15.0




Manual Integrations
APPROVED


mohammad
12/29/2019 5:30:13 PM

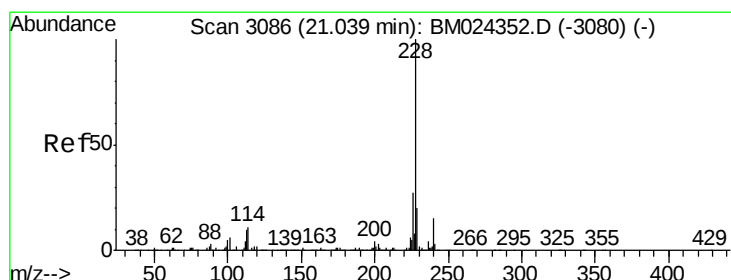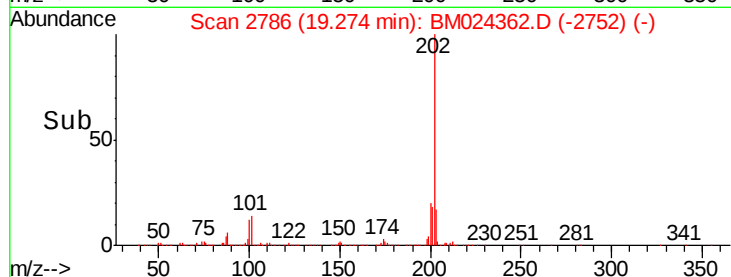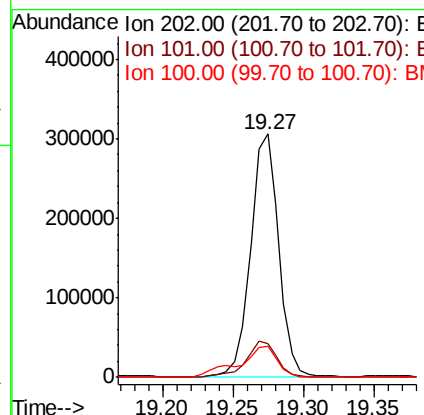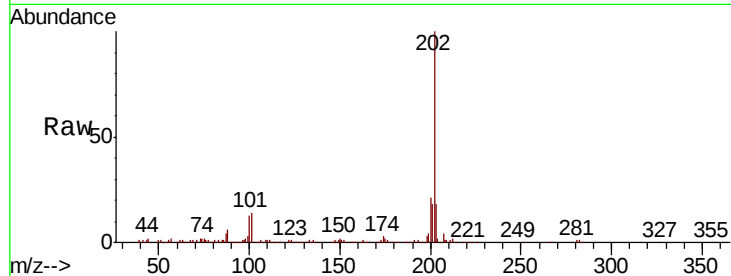

#83
Benzo(a)anthracene
Concen: 3.637 ng/ul
RT: 21.03 min Scan# 3085
Delta R.T. -0.01 min
Lab File: BM024362.D
Acq: 28 Dec 2019 22:47

Tgt Ion	Ratio	Resp Lower	Upper
228	100		
229	20.9	15.8	23.8
226	29.3	22.2	33.2

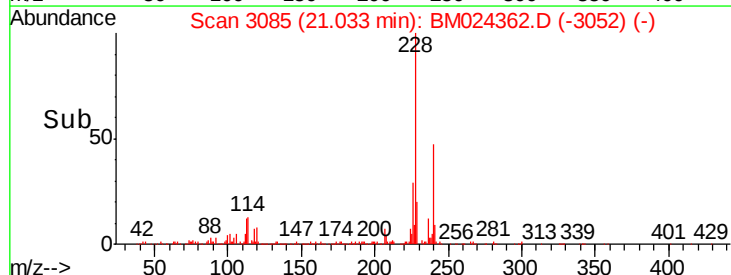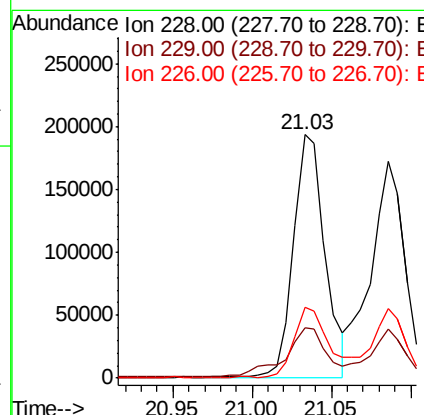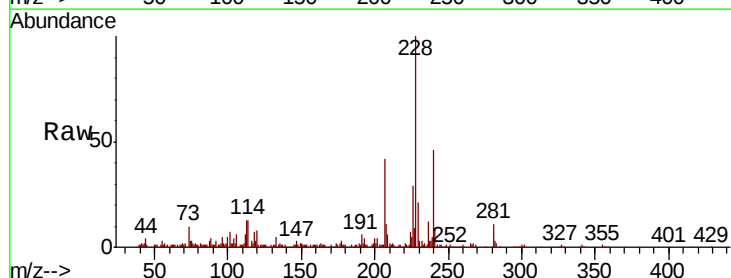

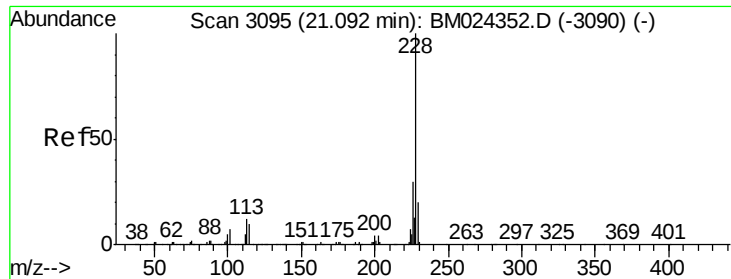

#85

Chrysene

Concen: 3.585 ng/ul

RT: 21.09 min Scan# 3094

Delta R.T. -0.01 min

Lab File: BM024362.D

Acq: 28 Dec 2019 22:47

Instrument :

BNA_M


ClientSampleId :

C0C46

Tot Ion:	228	Resp:	257275
Ion Ratio		Lower	Upper
228	100		
226	31.8	24.0	36.0
229	22.6	15.4	23.2

Manual Integrations
APPROVED

mohammad
12/29/2019 5:30:13 PM



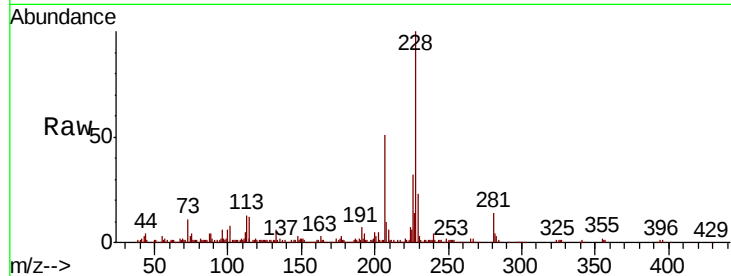


Abundance

Ion 228.00 (227.70 to 228.70): E

Ion 226.00 (225.70 to 226.70): E

Ion 229.00 (228.70 to 229.70): E

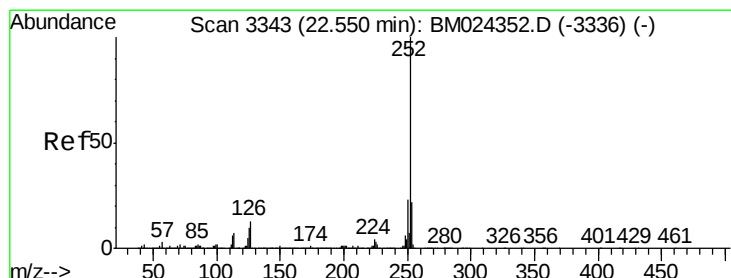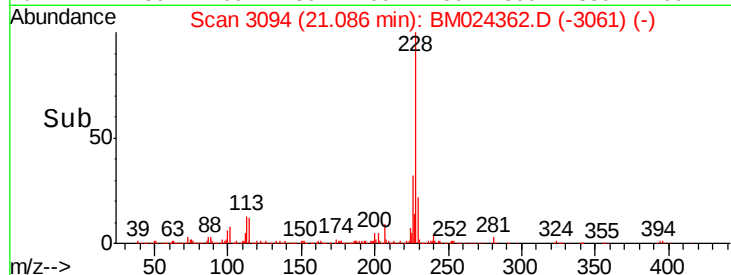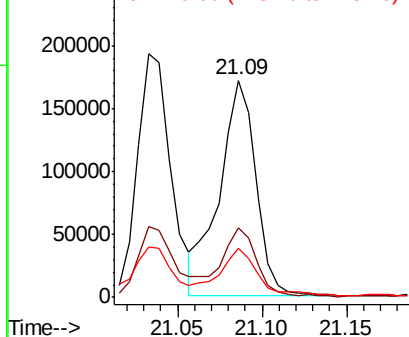

#88

Benzo(b)fluoranthene

Concen: 4.543 ng/ul

RT: 22.55 min Scan# 3343

Delta R.T. 0.00 min

Lab File: BM024362.D

Acq: 28 Dec 2019 22:47




Tgt Ion:	252	Resp:	377693
Ion Ratio		Lower	Upper
252	100		
253	24.0	17.2	25.8
125	14.7	7.8	11.8#


Abundance

Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

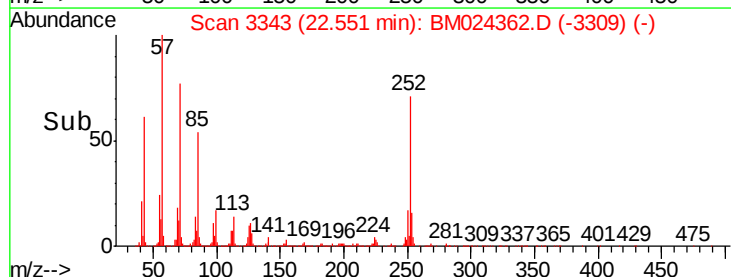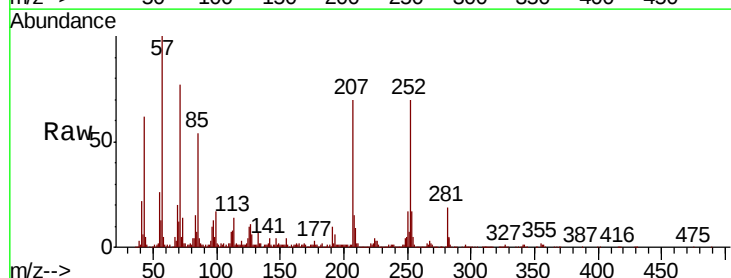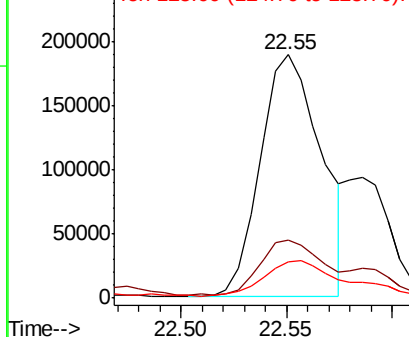

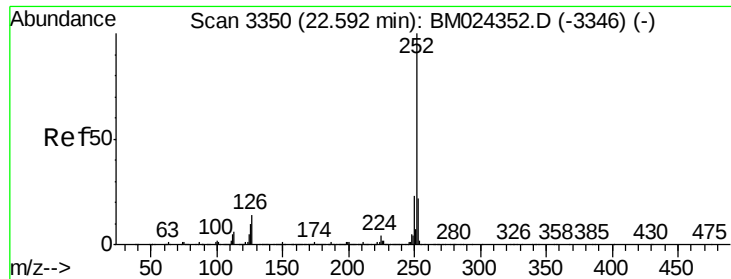





#89
Benzo(k)fluoranthene
Concen: 1.687 ng/ul m
RT: 22.59 min Scan# 3349
Delta R.T. -0.01 min
Lab File: BM024362.D
Acq: 28 Dec 2019 22:47

Instrument :
BNA_M
ClientSampled :
C0C46

Tot Ion	Ratio	Lower	Upper
252	100		
253	24.9	17.8	26.8
125	13.3	7.9	11.9




Manual Integrations
APPROVED


mohammad
12/29/2019 5:30:13 PM

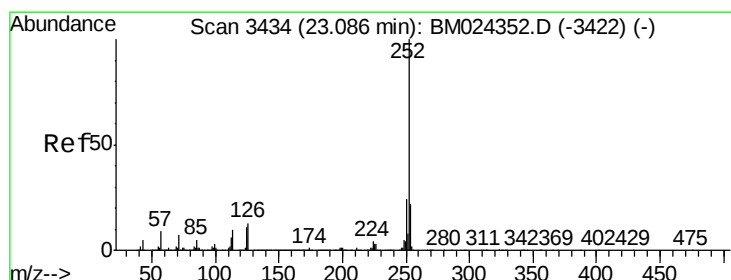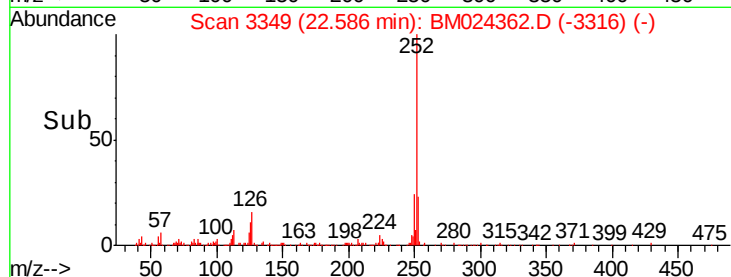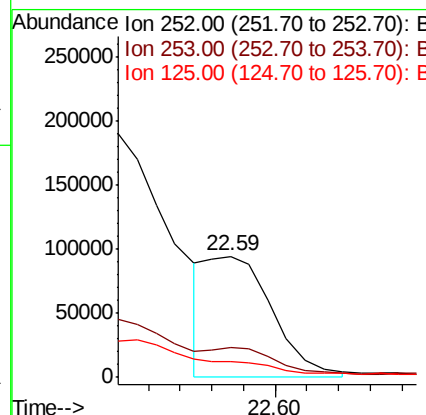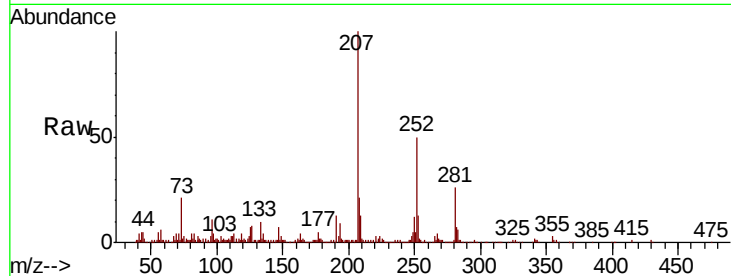

#91
Benzo(a)pyrene
Concen: 3.183 ng/ul
RT: 23.08 min Scan# 3433
Delta R.T. -0.01 min
Lab File: BM024362.D
Acq: 28 Dec 2019 22:47

Tgt Ion	Ratio	Lower	Upper
252	100		
253	25.0	17.5	26.3
125	17.3	8.2	12.4

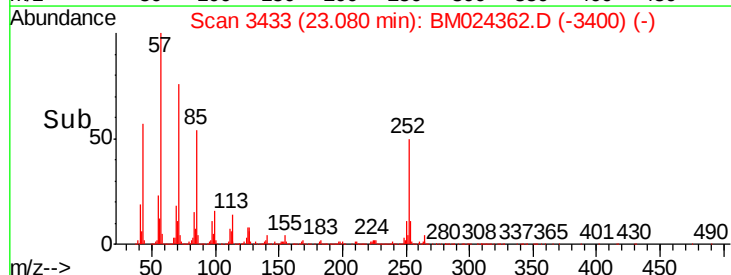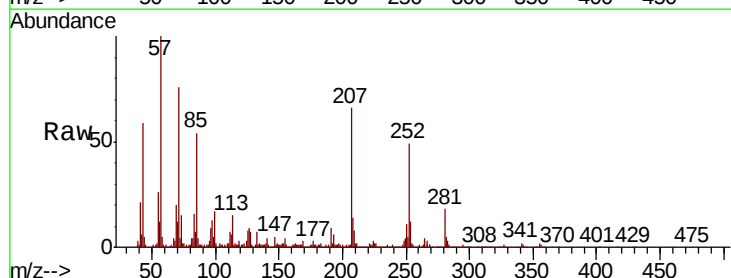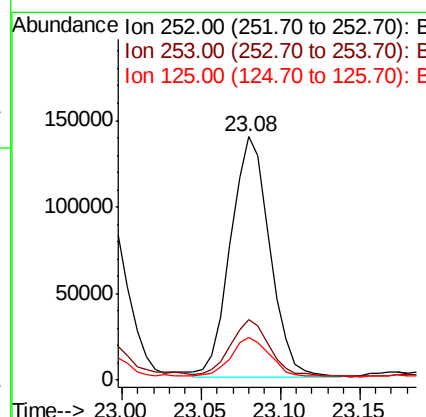

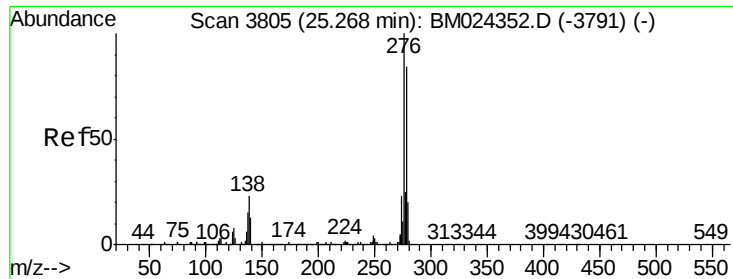





#92
 Indeno(1,2,3-cd)pyrene
 Concen: 1.941 ng/ul
 RT: 25.27 min Scan# 3805
 Delta R.T. 0.00 min
 Lab File: BM024362.D
 Acq: 28 Dec 2019 22:47

Instrument :
 BNA_M
 ClientSampleId :
 C0C46

Tot Ion	Ratio	Lower	Upper
276	100		
138	17.8	18.3	27.5#
277	25.8	20.2	30.2

Manual Integrations
 APPROVED

mohammad
 12/29/2019 5:30:13 PM

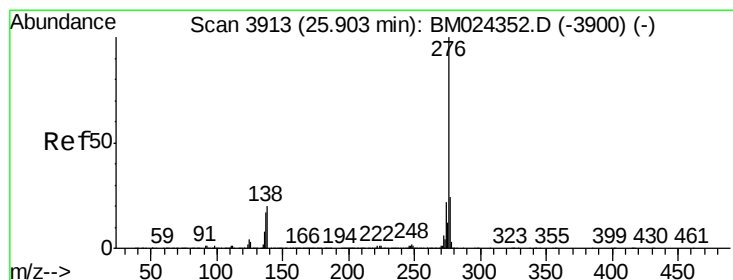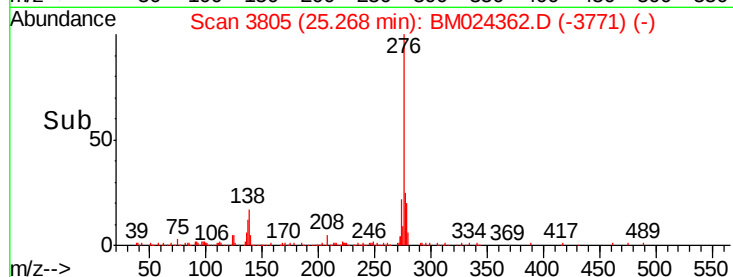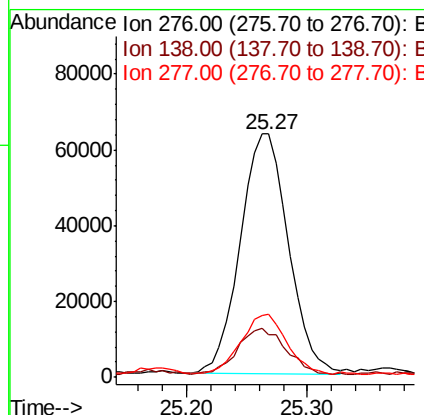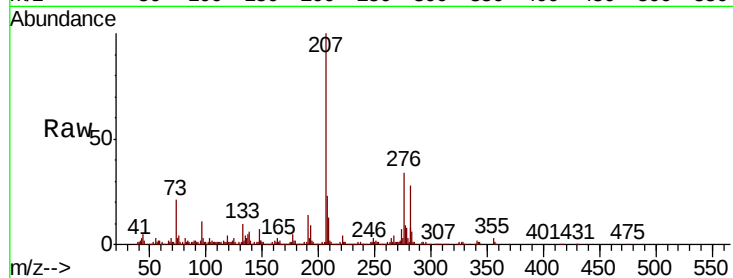

#94
 Benzo(g,h,i)perylene
 Concen: 1.792 ng/ul
 RT: 25.90 min Scan# 3913
 Delta R.T. 0.00 min
 Lab File: BM024362.D
 Acq: 28 Dec 2019 22:47

Tgt Ion	Ratio	Lower	Upper
276	100		
138	18.5	15.3	22.9
277	25.4	19.3	28.9

