
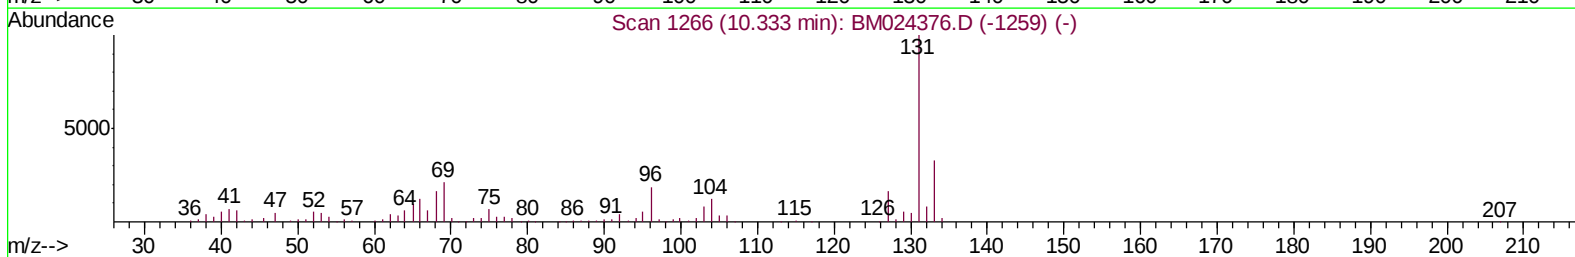
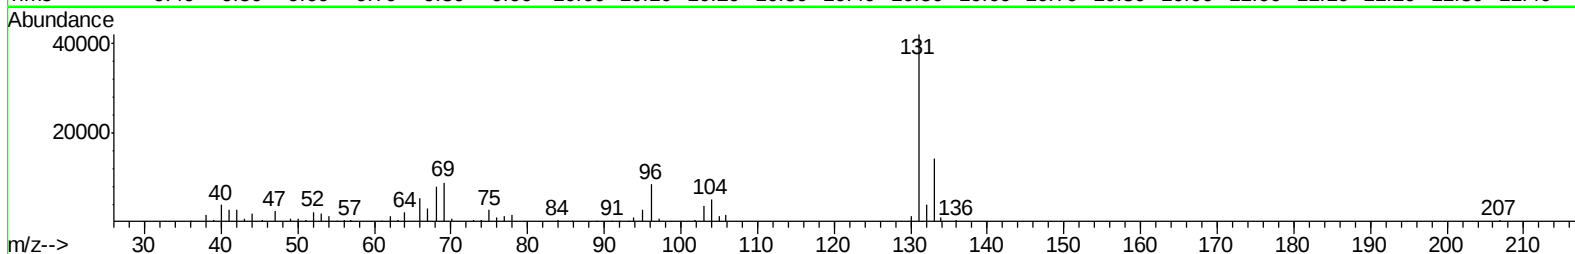


Data File : BM024379.D  
Acq On : 30 Dec 2019 18:45  
Operator : JU  
Sample : K6322-12  
Misc :  
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Dec 31 03:15:27 2019  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_M\METHODS\SOM-EPA-BM121719MA.M  
Quant Title : SVOA CALIBRATION  
QLast Update : Tue Dec 31 03:12:42 2019  
Response via : Initial Calibration

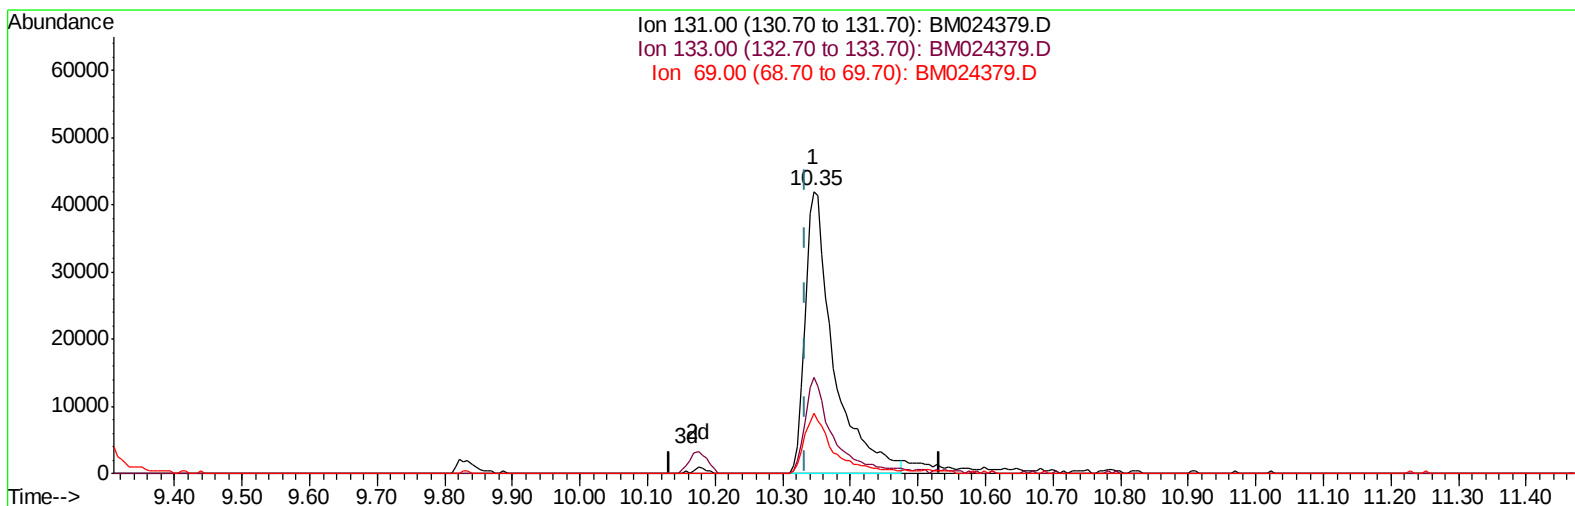

TIC: BM024379.D

(29) 4-Chloroaniline-d4 (S)

10.346min (+0.012) 8.01ng/ul m

response 121882

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 131.00 | 100   | 100   |
| 133.00 | 32.50 | 34.23 |
| 69.00  | 19.00 | 21.40 |
| 0.00   | 0.00  | 0.00  |