
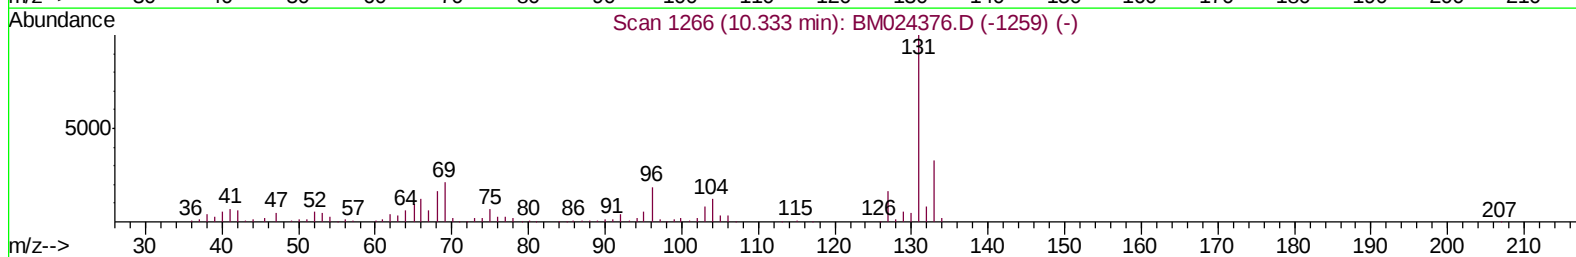
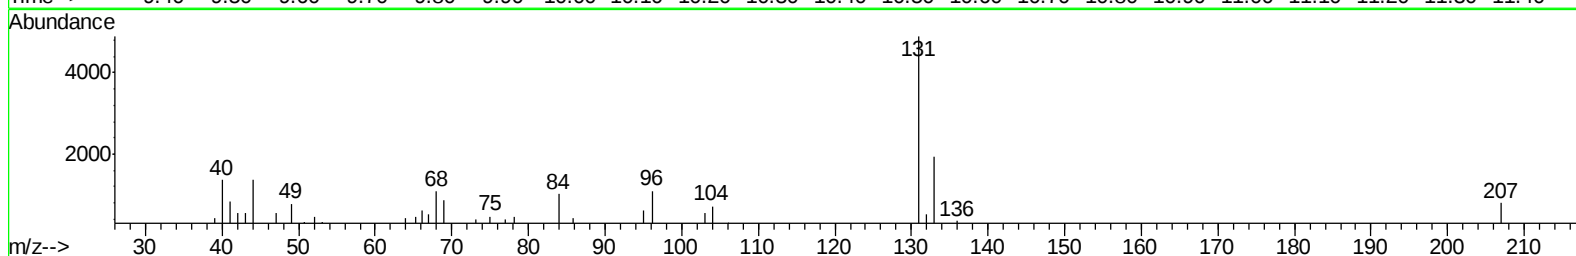


Data File : BM024383.D
Acq On : 30 Dec 2019 21:09
Operator : JU
Sample : K6356-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Dec 31 03:15:57 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Dec 31 03:12:42 2019
Response via : Initial Calibration

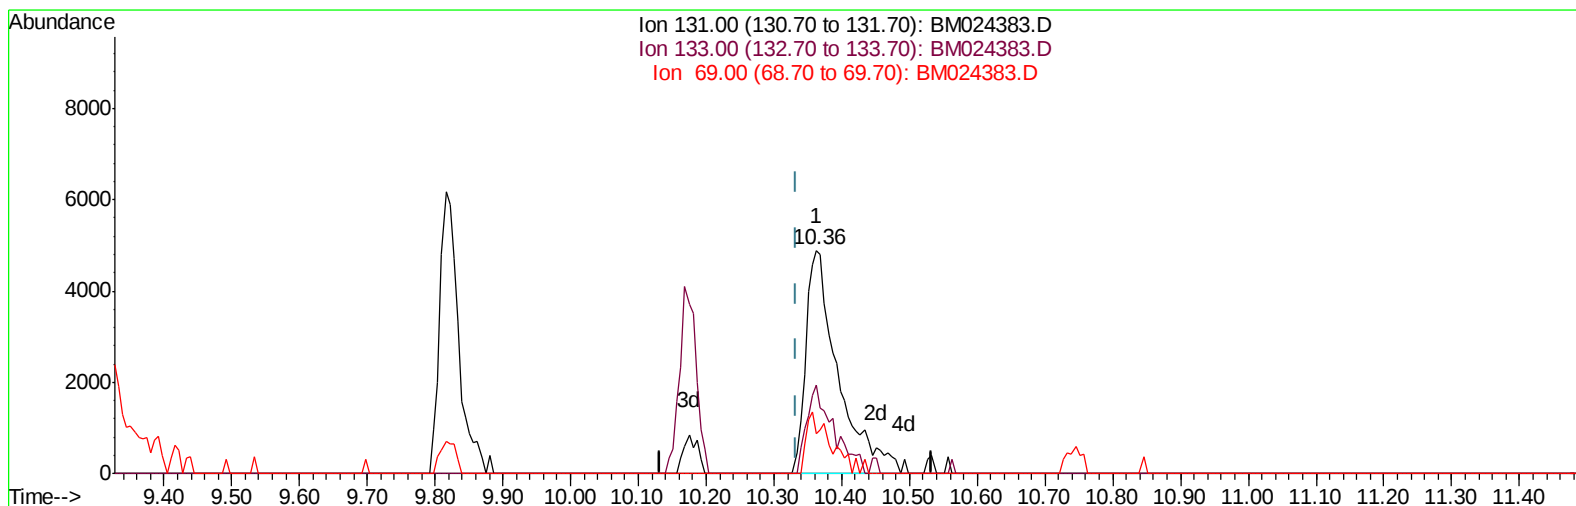

TIC: BM024383.D

(29) 4-Chloroaniline-d4 (S)

10.363min (+0.029) 1.03ng/ul m

response 16235

Ion	Exp%	Act%
131.00	100	100
133.00	32.50	39.74#
69.00	19.00	18.04
0.00	0.00	0.00