

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM123019\
 Data File : BM024379.D
 Acq On : 30 Dec 2019 18:45
 Operator : JU
 Sample : K6322-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Title : SVOA CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.993	16	18	26	rVB2	21410	35285	1.10%	0.115%
2	3.399	84	87	94	rVB6	12010	23725	0.74%	0.077%
3	3.487	98	102	109	rVV	44006	66162	2.06%	0.215%
4	3.681	131	135	141	rVB2	18411	27265	0.85%	0.089%
5	4.228	226	228	234	rVV5	5358	6798	0.21%	0.022%
6	4.293	237	239	243	rBV5	3510	4417	0.14%	0.014%
7	4.581	285	288	294	rBV4	15245	22744	0.71%	0.074%
8	4.628	294	296	302	rBV6	7338	12447	0.39%	0.040%
9	4.822	327	329	333	rVB4	3409	3284	0.10%	0.011%
10	5.093	372	375	376	rBV3	3995	3622	0.11%	0.012%
11	6.569	620	626	628	rBV4	3801	5178	0.16%	0.017%
12	6.616	628	634	651	rVV	240963	539789	16.79%	1.754%
13	6.769	654	660	675	rVV	222793	403494	12.55%	1.311%
14	6.952	684	691	703	rBV	313793	546432	17.00%	1.776%
15	7.405	762	768	781	rBV	753705	1276570	39.71%	4.149%
16	7.622	800	805	808	rBV5	3179	5541	0.17%	0.018%
17	8.146	887	894	910	rBV2	165212	358117	11.14%	1.164%
18	8.269	910	915	920	rVB4	6586	13229	0.41%	0.043%
19	8.569	960	966	983	rBV	247105	482927	15.02%	1.570%
20	8.987	1032	1037	1045	rBV4	9166	16514	0.51%	0.054%
21	9.281	1081	1087	1100	rBV	190052	372473	11.59%	1.211%
22	9.828	1174	1180	1194	rBV	237056	542665	16.88%	1.764%
23	10.175	1231	1239	1257	rBV	1052018	1768206	55.01%	5.747%
24	10.346	1261	1268	1285	rBV	153045	422373	13.14%	1.373%
25	10.787	1338	1343	1347	rBV6	2120	4405	0.14%	0.014%
26	11.222	1409	1417	1420	rBV4	2639	6479	0.20%	0.021%
27	11.634	1486	1487	1494	rVB6	3274	4056	0.13%	0.013%
28	11.798	1511	1515	1517	rBV2	3281	4305	0.13%	0.014%
29	11.875	1522	1528	1534	rVB6	3437	6097	0.19%	0.020%
30	12.540	1636	1641	1645	rBV4	1917	3895	0.12%	0.013%
31	12.910	1698	1704	1708	rBV6	4393	7130	0.22%	0.023%
32	13.387	1780	1785	1790	rBV6	4892	7186	0.22%	0.023%
33	13.498	1798	1804	1809	rBV	618169	884299	27.51%	2.874%
34	13.551	1809	1813	1821	rVB	99316	165944	5.16%	0.539%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM123019\
 Data File : BM024379.D
 Acq On : 30 Dec 2019 18:45
 Operator : JU
 Sample : K6322-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Title : SVOA CALIBRATION

35	13.763	1842	1849	1861	rBV	694531	1067712	33.22%	3.470%
36	13.998	1886	1889	1895	rVB3	4889	6513	0.20%	0.021%
37	14.075	1895	1902	1912	rBV	1425177	2182452	67.90%	7.093%
38	14.145	1912	1914	1916	rVB4	5228	4491	0.14%	0.015%
39	14.375	1947	1953	1959	rBV3	45283	121194	3.77%	0.394%
40	14.551	1978	1983	1990	rVB6	12709	23337	0.73%	0.076%
41	14.698	2007	2008	2014	rVB4	3009	4307	0.13%	0.014%
42	14.904	2041	2043	2046	rVB2	4973	4443	0.14%	0.014%
43	14.963	2046	2053	2056	rBV4	7955	10519	0.33%	0.034%
44	15.081	2067	2073	2080	rBV	899011	1379839	42.93%	4.485%
45	15.133	2080	2082	2084	rVV2	16659	19570	0.61%	0.064%
46	15.157	2084	2086	2091	rVB3	14199	16758	0.52%	0.054%
47	15.245	2096	2101	2108	rBV	108841	193875	6.03%	0.630%
48	15.439	2129	2134	2138	rBV5	6254	8075	0.25%	0.026%
49	15.516	2145	2147	2151	rVB4	3411	3728	0.12%	0.012%
50	15.586	2153	2159	2161	rBV6	7958	10770	0.34%	0.035%
51	15.828	2196	2200	2202	rBV2	10005	12451	0.39%	0.040%
52	15.869	2205	2207	2213	rVB5	3839	4883	0.15%	0.016%
53	15.992	2225	2228	2231	rBV5	3331	4436	0.14%	0.014%
54	16.092	2242	2245	2248	rVB4	2772	3328	0.10%	0.011%
55	16.151	2252	2255	2259	rVV3	4096	6662	0.21%	0.022%
56	16.186	2259	2261	2268	rVB6	4848	8116	0.25%	0.026%
57	16.398	2288	2297	2303	rBV9	17179	38424	1.20%	0.125%
58	16.504	2310	2315	2320	rBV6	13166	23930	0.74%	0.078%
59	16.575	2322	2327	2331	rVV5	7893	13611	0.42%	0.044%
60	16.622	2331	2335	2338	rVV3	16407	23011	0.72%	0.075%
61	16.651	2338	2340	2346	rVV2	11403	18671	0.58%	0.061%
62	16.833	2365	2371	2375	rBV	1710590	2439044	75.88%	7.927%
63	16.875	2375	2378	2382	rVV	291118	383298	11.92%	1.246%
64	16.933	2382	2388	2402	rVB	964189	1469153	45.71%	4.775%
65	17.151	2423	2425	2428	rVB4	3965	3929	0.12%	0.013%
66	17.210	2431	2435	2436	rBV4	3430	3894	0.12%	0.013%
67	17.263	2436	2444	2450	rBV8	14542	39013	1.21%	0.127%
68	17.363	2457	2461	2465	rBV5	13092	20490	0.64%	0.067%
69	17.545	2488	2492	2493	rBV4	4546	5720	0.18%	0.019%
70	17.633	2504	2507	2515	rBV7	6425	12193	0.38%	0.040%
71	17.710	2516	2520	2524	rBV	26969	37735	1.17%	0.123%

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM123019\
 Data File : BM024379.D
 Acq On : 30 Dec 2019 18:45
 Operator : JU
 Sample : K6322-12
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BT7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0.1 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
 Title : SVOA CALIBRATION

72	17.757	2524	2528	2536	rVV3	65061	111077	3.46%	0.361%
73	17.904	2549	2553	2558	rBV2	45538	76025	2.37%	0.247%
74	17.945	2558	2560	2565	rVB4	22418	28298	0.88%	0.092%
75	18.051	2576	2578	2580	rBV2	7563	5776	0.18%	0.019%
76	18.116	2587	2589	2592	rBV3	5369	6193	0.19%	0.020%
77	18.221	2603	2607	2612	rBV	25259	39586	1.23%	0.129%
78	18.280	2612	2617	2621	rVV5	18783	28525	0.89%	0.093%
79	18.369	2630	2632	2636	rVB4	6026	4802	0.15%	0.016%
80	18.469	2647	2649	2653	rVB4	8295	7761	0.24%	0.025%
81	18.645	2674	2679	2684	rBV5	23563	41920	1.30%	0.136%
82	18.698	2684	2688	2691	rBV5	30711	44416	1.38%	0.144%
83	18.792	2700	2704	2711	rVB5	19607	32627	1.02%	0.106%
84	18.904	2718	2723	2732	rVB	562103	769963	23.95%	2.502%
85	19.057	2746	2749	2753	rBV3	30718	40180	1.25%	0.131%
86	19.239	2775	2780	2784	rBV	1367457	2034375	63.29%	6.612%
87	19.268	2784	2785	2795	rVB	491404	511841	15.92%	1.664%
88	19.780	2870	2872	2877	rVB2	45712	51307	1.60%	0.167%
89	19.821	2877	2879	2882	rVB3	23182	24682	0.77%	0.080%
90	19.880	2886	2889	2893	rBV3	43796	53979	1.68%	0.175%
91	20.786	3039	3043	3049	rBV4	197082	296170	9.21%	0.963%
92	21.051	3082	3088	3092	rBV	2198348	3058867	95.16%	9.942%
93	21.086	3092	3094	3100	rVB	241599	266794	8.30%	0.867%
94	22.557	3339	3344	3349	rBV2	363683	667424	20.76%	2.169%
95	23.039	3421	3426	3430	rBV	1024250	1668509	51.91%	5.423%
96	23.168	3442	3448	3464	rVB	1692697	3214388	100.00%	10.447%


Sum of corrected areas: 30768113

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM123019\
Data File : BM024379.D
Acq On : 30 Dec 2019 18:45
Operator : JU
Sample : K6322-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

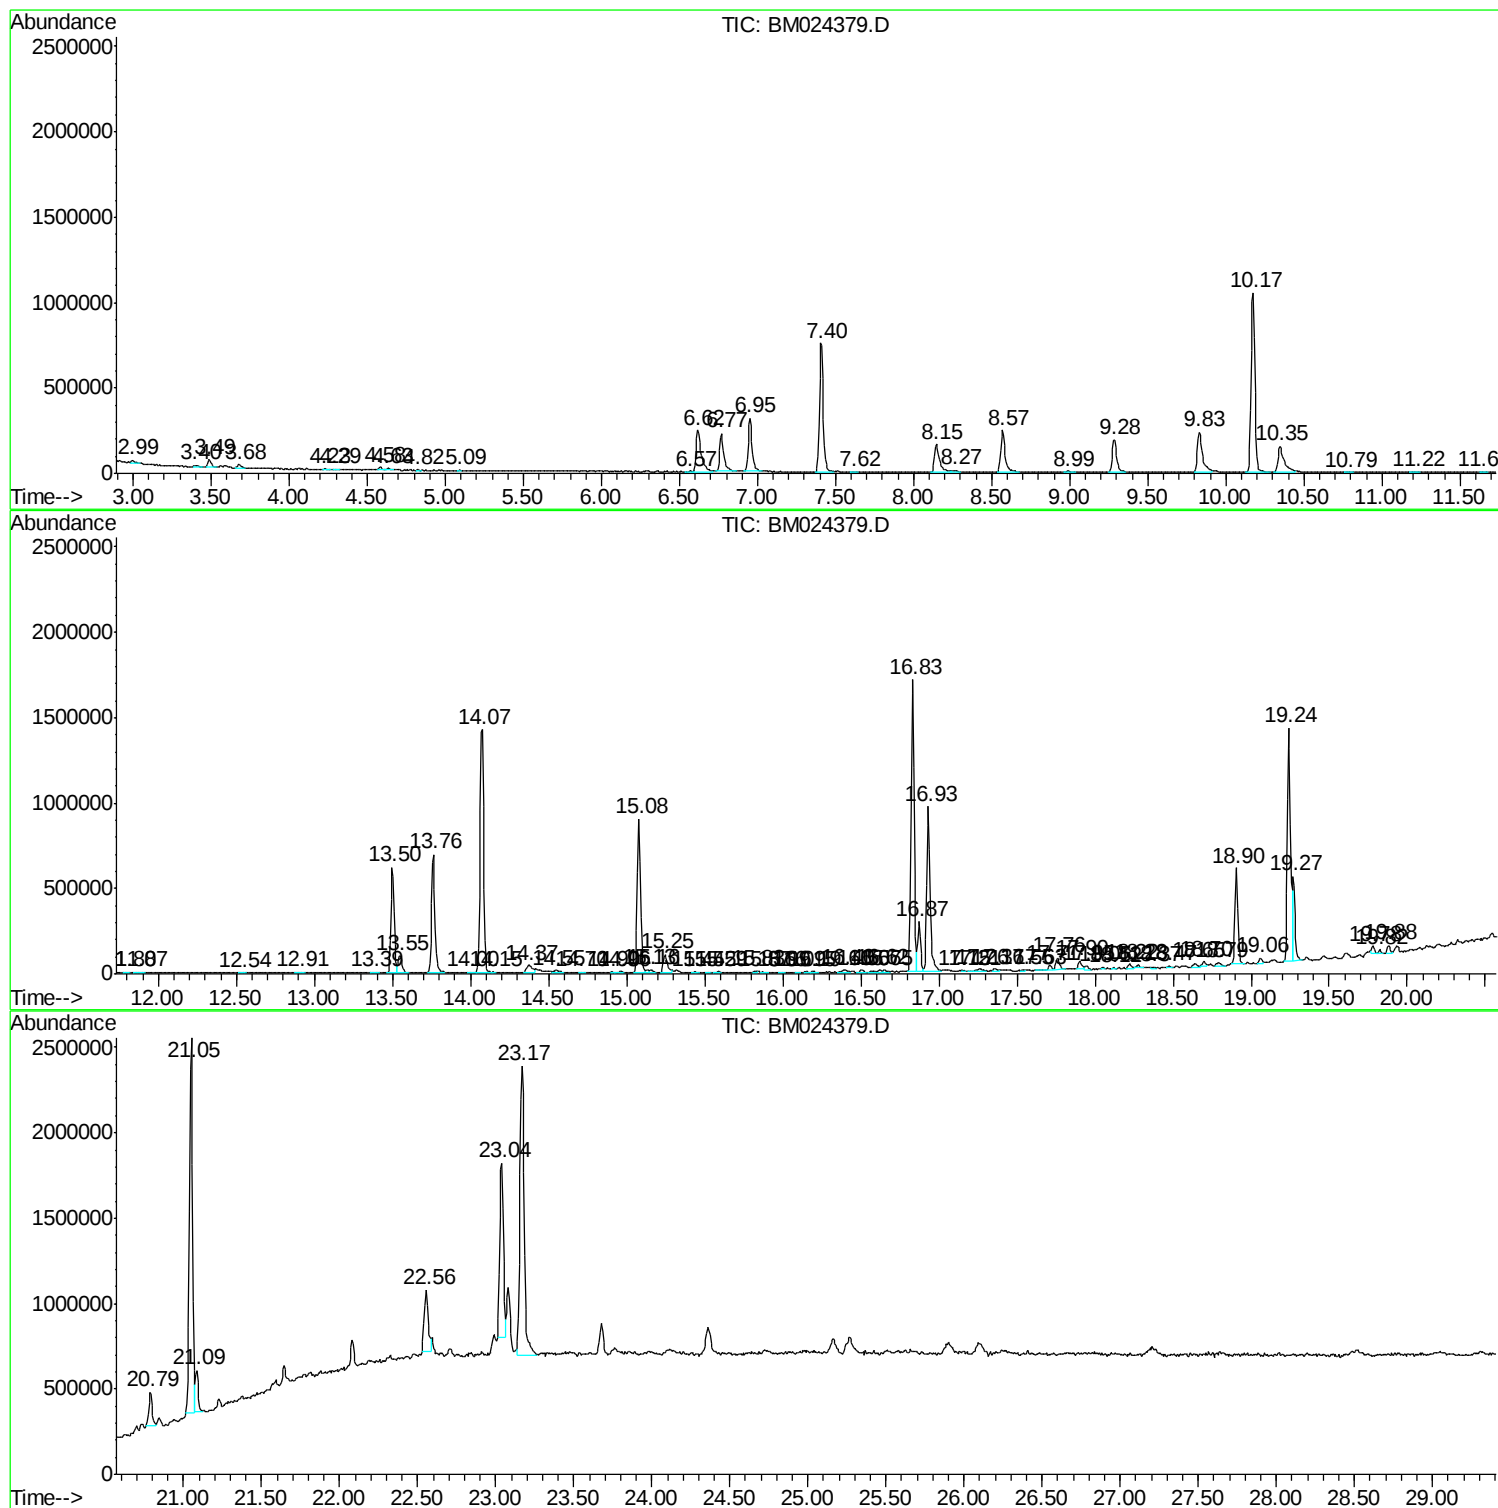

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM123019\
Data File : BM024379.D
Acq On : 30 Dec 2019 18:45
Operator : JU
Sample : K6322-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM123019\
Data File : BM024379.D
Acq On : 30 Dec 2019 18:45
Operator : JU
Sample : K6322-12
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BT7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM121719MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc