

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
 Data File : BM038383.D
 Acq On : 06 Jan 2023 11:23
 Operator : CG/JU
 Sample : PB149980BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK980

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038383.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	27	30	42	rVB2	25807	41295	2.61%	0.254%
2	3.799	100	104	121	rBV	286690	469007	29.68%	2.881%
3	4.122	156	159	165	rVB2	5862	7334	0.46%	0.045%
4	5.475	388	389	391	rBV	1898	1701	0.11%	0.010%
5	5.557	401	403	407	rBV4	1389	2123	0.13%	0.013%
6	6.910	631	633	636	rBV2	1117	1628	0.10%	0.010%
7	7.157	669	675	689	rVV	338319	524354	33.19%	3.221%
8	7.328	698	704	713	rBV	258648	397807	25.18%	2.444%
9	7.522	731	737	752	rVB	330282	532119	33.68%	3.269%
10	7.998	811	818	828	rVV	273488	423365	26.79%	2.601%
11	8.710	932	939	952	rBV	340258	550378	34.83%	3.381%
12	9.169	1009	1017	1032	rBV	279673	467958	29.62%	2.875%
13	9.892	1133	1140	1156	rBV	237272	390248	24.70%	2.398%
14	10.022	1160	1162	1167	rBV4	1233	1682	0.11%	0.010%
15	10.433	1225	1232	1241	rBV	312637	538392	34.07%	3.308%
16	10.810	1290	1296	1306	rBV	340264	537336	34.01%	3.301%
17	10.951	1314	1320	1338	rBV	294321	527404	33.38%	3.240%
18	12.398	1563	1566	1569	rBV4	2236	3592	0.23%	0.022%
19	14.039	1839	1845	1856	rVB	574213	734689	46.50%	4.514%
20	14.327	1888	1894	1908	rVB	579337	809826	51.25%	4.975%
21	14.627	1938	1945	1954	rBV	442807	654101	41.40%	4.019%
22	14.833	1974	1980	1996	rBV	209858	358057	22.66%	2.200%
23	14.957	2000	2001	2006	rVB4	2069	2873	0.18%	0.018%
24	15.621	2107	2114	2126	rBV	721977	1007324	63.75%	6.189%
25	15.745	2129	2135	2150	rVV	284229	395139	25.01%	2.428%
26	15.862	2150	2155	2157	rVB4	1900	2745	0.17%	0.017%
27	16.721	2298	2301	2305	rVB4	1436	1620	0.10%	0.010%
28	16.809	2314	2316	2319	rBV3	1694	1756	0.11%	0.011%
29	17.086	2358	2363	2365	rBV4	1037	1661	0.11%	0.010%
30	17.368	2405	2411	2420	rBV	551576	767650	48.58%	4.716%
31	17.468	2422	2428	2442	rVV	810966	1146428	72.56%	7.043%
32	17.880	2494	2498	2501	rBV3	3132	4769	0.30%	0.029%
33	18.821	2654	2658	2663	rVV6	4034	5806	0.37%	0.036%
34	19.327	2739	2744	2747	rBV5	8278	11194	0.71%	0.069%
35	19.392	2752	2755	2759	rBV3	6070	10386	0.66%	0.064%
36	19.662	2800	2801	2806	rBV5	4901	5688	0.36%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038383.D
Acq On : 06 Jan 2023 11:23
Operator : CG/JU
Sample : PB149980BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK980

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Title : SVOA CALIBRATION

37	19.756	2811	2817	2824	rBV	1075757	1358887	86.00%	8.349%
38	20.733	2979	2983	2988	rBV	93760	106801	6.76%	0.656%
39	21.544	3116	3121	3127	rBV	664377	855153	54.12%	5.254%
40	23.821	3501	3508	3519	rBV	822985	1580021	100.00%	9.707%
41	23.974	3528	3534	3547	rBV2	532040	1036612	65.61%	6.369%




Sum of corrected areas: 16276909

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038383.D
Acq On : 06 Jan 2023 11:23
Operator : CG/JU
Sample : PB149980BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK980

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

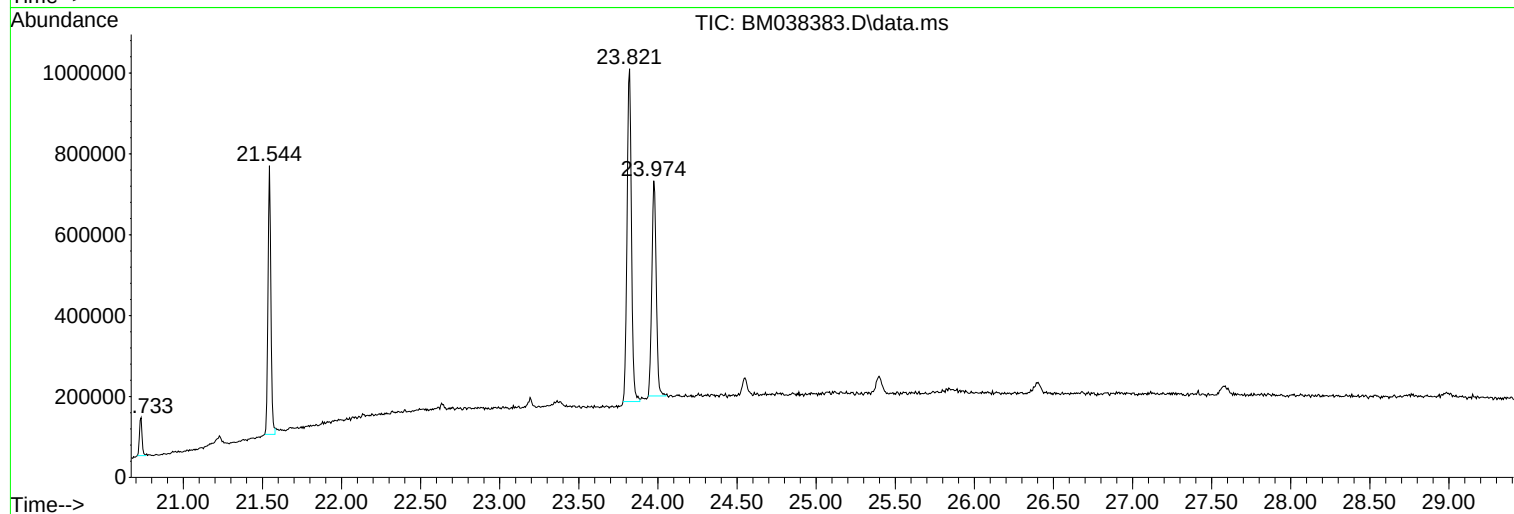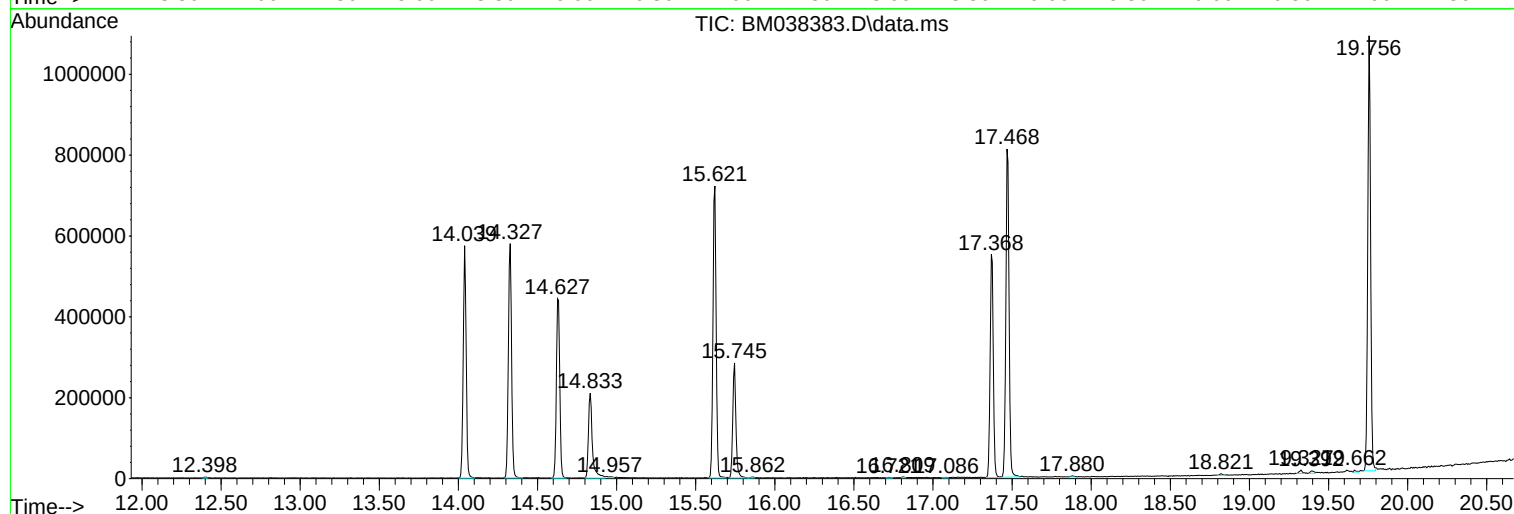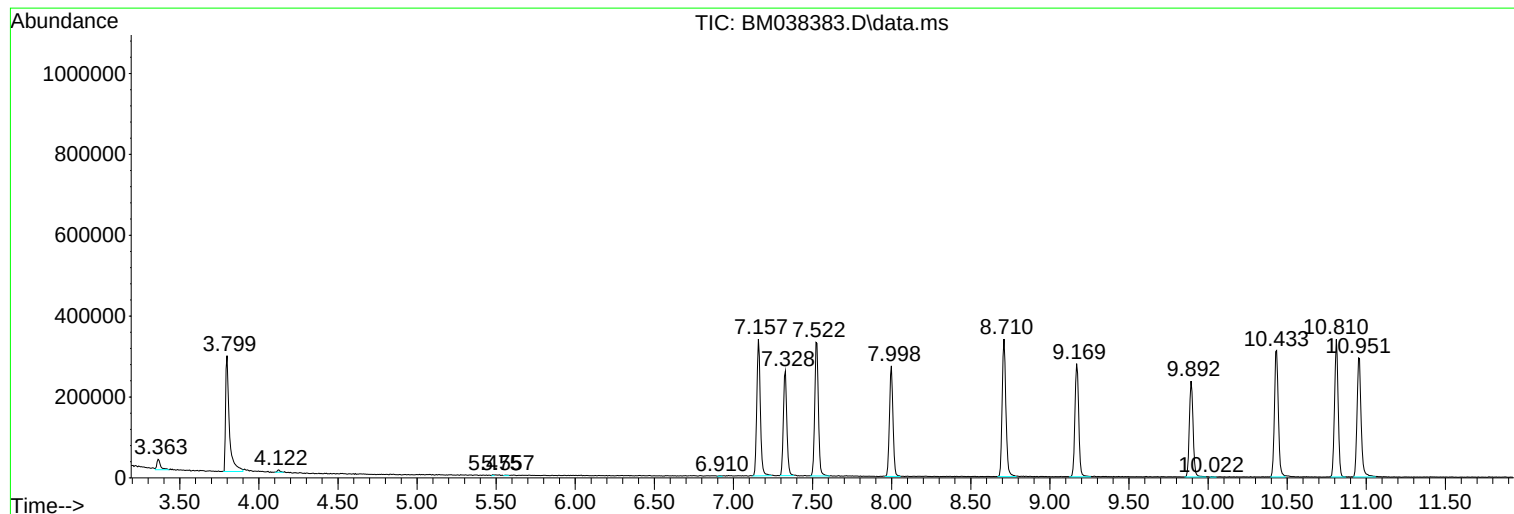

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038383.D
Acq On : 06 Jan 2023 11:23
Operator : CG/JU
Sample : PB149980BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK980










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Adipic acid, 2-ethylhexyl o... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.733	2.50 ng/ul	106801	Chrysene-d12	21.544

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	83
2			Hexanedioic acid, mono(2-ethylhe...	258	C14H26O4	004337-65-9	62
3			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	58
4			Adipic acid, 2-ethylhexyl isobut...	314	C18H34O4	1010324-48-0	50
5			Diisooctyl adipate	370	C22H42O4	001330-86-5	49

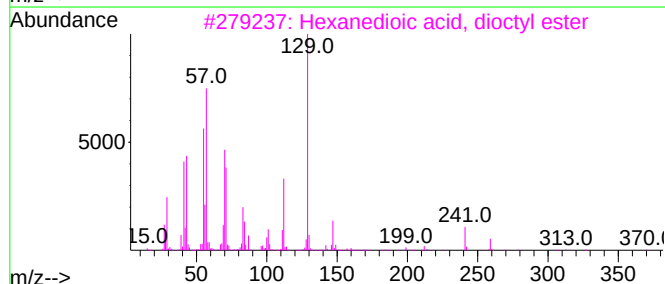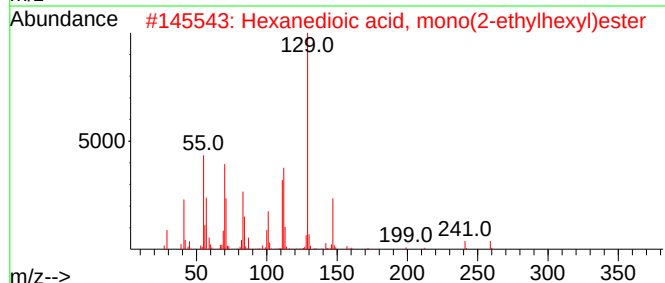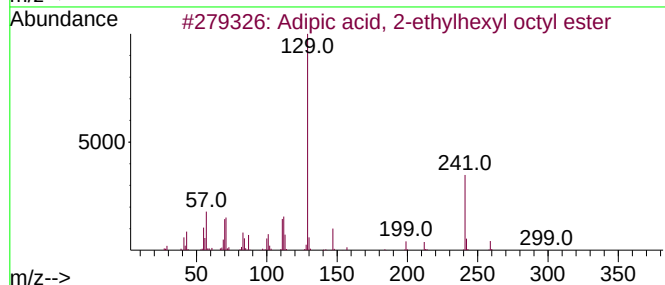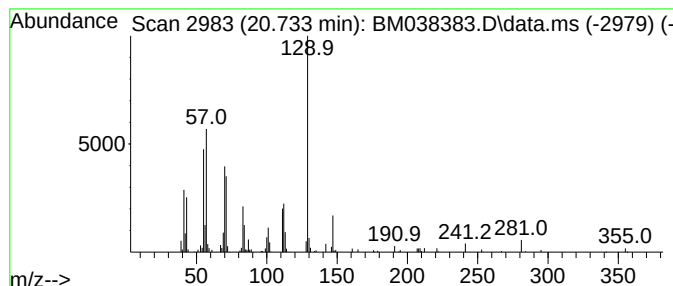

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038383.D
Acq On : 06 Jan 2023 11:23
Operator : CG/JU
Sample : PB149980BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK980

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Adipic acid, 2-...	20.733	2.5	ng/u1	106801	5	21.544	855153	20.0