

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
 Data File : BM038385.D
 Acq On : 06 Jan 2023 12:37
 Operator : CG/JU
 Sample : PB149982BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK982

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038385.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	37	rVB	27413	32316	1.91%	0.192%
2	3.798	100	104	122	rBV	307263	508678	30.02%	3.024%
3	4.128	156	160	165	rVB2	5980	9280	0.55%	0.055%
4	4.234	176	178	181	rBV3	2089	1855	0.11%	0.011%
5	4.345	195	197	199	rBV2	1642	1908	0.11%	0.011%
6	7.163	669	676	689	rVV	337768	544860	32.16%	3.239%
7	7.328	698	704	717	rVB	268317	409968	24.20%	2.437%
8	7.528	731	738	747	rBV	338714	529261	31.24%	3.146%
9	7.998	811	818	828	rVV	296953	453284	26.75%	2.694%
10	8.710	933	939	949	rBV	362664	584848	34.52%	3.477%
11	9.169	1007	1017	1030	rBV	305784	501577	29.60%	2.982%
12	9.892	1134	1140	1152	rBV	248470	413819	24.42%	2.460%
13	10.433	1225	1232	1243	rBV	341219	571323	33.72%	3.396%
14	10.810	1289	1296	1306	rVB	349041	570075	33.65%	3.389%
15	10.957	1314	1321	1337	rBV	325369	566618	33.44%	3.368%
16	12.404	1561	1567	1570	rBV5	1937	3429	0.20%	0.020%
17	14.039	1839	1845	1860	rBV	560341	758314	44.76%	4.508%
18	14.327	1887	1894	1903	rBV	608413	849466	50.14%	5.049%
19	14.633	1940	1946	1957	rVB	475330	685962	40.49%	4.078%
20	14.833	1974	1980	1998	rBV	220658	361532	21.34%	2.149%
21	15.409	2074	2078	2082	rBV4	1142	2013	0.12%	0.012%
22	15.621	2107	2114	2126	rBV	771628	1044302	61.64%	6.208%
23	15.745	2130	2135	2147	rBV	293996	399827	23.60%	2.377%
24	15.862	2152	2155	2157	rVB3	2051	1990	0.12%	0.012%
25	16.974	2340	2344	2346	rBV3	1188	1940	0.11%	0.012%
26	17.156	2372	2375	2381	rBV4	1341	2295	0.14%	0.014%
27	17.368	2406	2411	2419	rBV	554022	763138	45.04%	4.536%
28	17.468	2422	2428	2444	rVV	849156	1161455	68.55%	6.904%
29	18.062	2523	2529	2532	rBV7	1051	2257	0.13%	0.013%
30	18.156	2543	2545	2549	rBV4	1514	2302	0.14%	0.014%
31	18.233	2555	2558	2562	rVV4	1196	1916	0.11%	0.011%
32	18.827	2655	2659	2660	rBV3	1780	2265	0.13%	0.013%
33	18.927	2673	2676	2678	rBV2	2155	1955	0.12%	0.012%
34	19.203	2721	2723	2725	rBV3	2151	2379	0.14%	0.014%
35	19.321	2740	2743	2750	rVB5	7679	10391	0.61%	0.062%
36	19.392	2752	2755	2759	rBV2	6428	8361	0.49%	0.050%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038385.D
Acq On : 06 Jan 2023 12:37
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK982

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Title : SVOA CALIBRATION

37	19.462	2764	2767	2769	rBV4	2385	2640	0.16%	0.016%
38	19.609	2790	2792	2794	rBV3	2716	2221	0.13%	0.013%
39	19.756	2811	2817	2824	rBV	1077966	1351203	79.75%	8.032%
40	20.727	2979	2982	2989	rBV	69357	85469	5.04%	0.508%
41	21.538	3116	3120	3128	rBV	608764	834028	49.23%	4.958%
42	23.191	3398	3401	3405	rVB2	56627	79228	4.68%	0.471%
43	23.815	3500	3507	3516	rBV2	920362	1694264	100.00%	10.071%
44	23.974	3527	3534	3543	rBV	513213	1006630	59.41%	5.984%




Sum of corrected areas: 16822842

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038385.D
Acq On : 06 Jan 2023 12:37
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

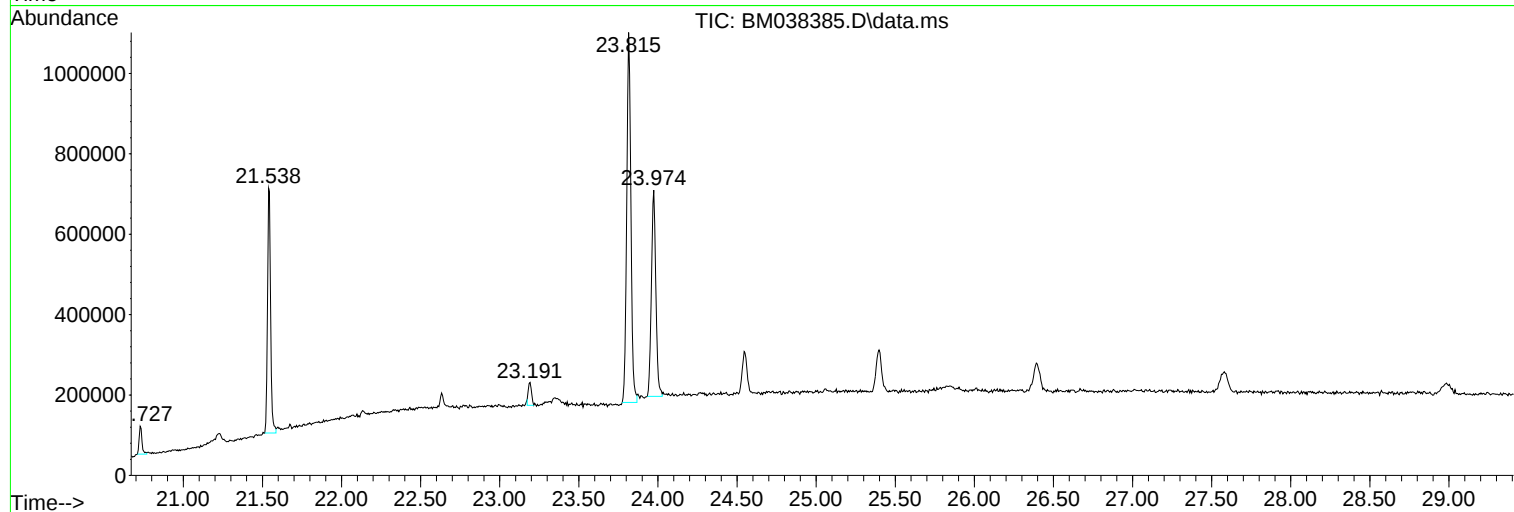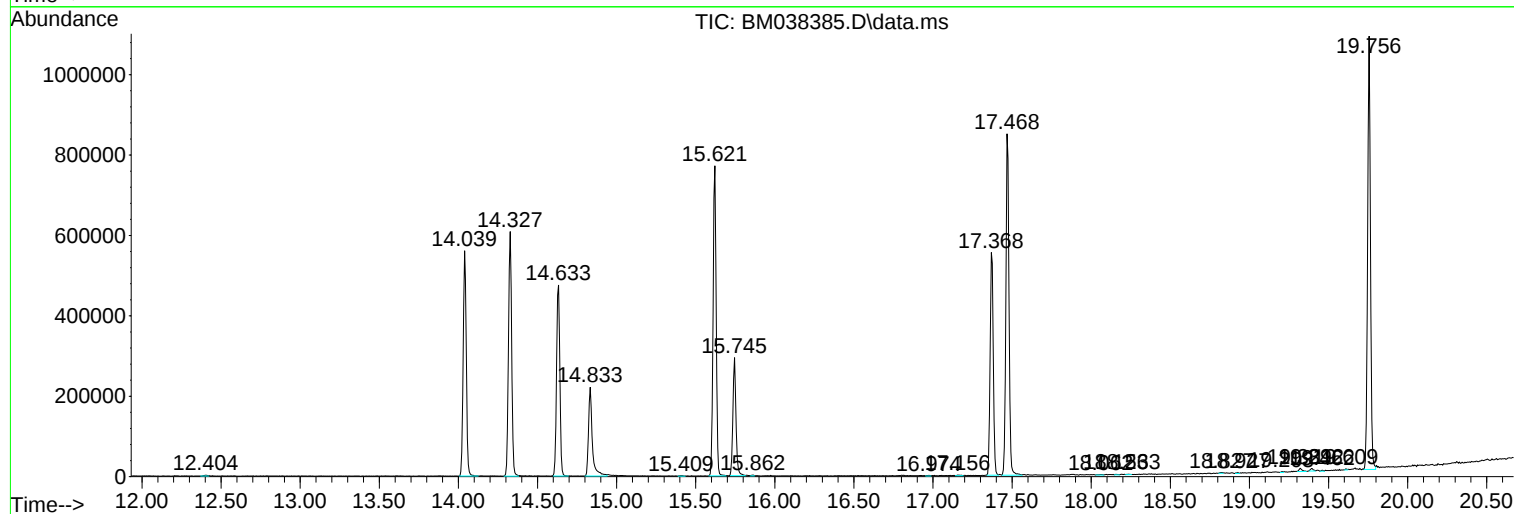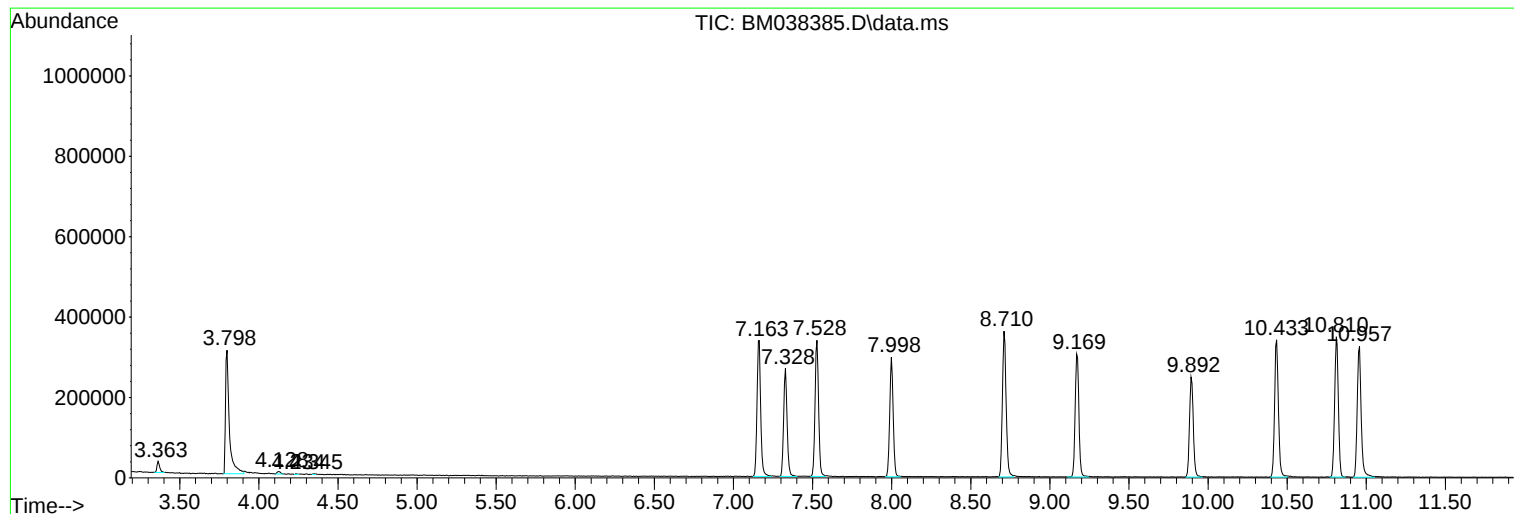

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038385.D
Acq On : 06 Jan 2023 12:37
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038385.D
Acq On : 06 Jan 2023 12:37
Operator : CG/JU
Sample : PB149982BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK982

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library :
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------