

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
 Data File : BM038390.D
 Acq On : 06 Jan 2023 17:30
 Operator : CG/JU
 Sample : PB150076BL
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK076

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038390.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	27	30	38	rVB	25562	35590	2.08%	0.194%
2	3.799	101	104	133	rBV	308731	527067	30.75%	2.871%
3	4.122	156	159	167	rVB2	8616	12360	0.72%	0.067%
4	4.481	218	220	223	rBV3	1743	2059	0.12%	0.011%
5	7.157	668	675	692	rBV	378838	616365	35.96%	3.358%
6	7.328	698	704	712	rBV	292981	446409	26.04%	2.432%
7	7.528	731	738	751	rVB	371512	589369	34.38%	3.211%
8	7.998	811	818	830	rVB	316591	492436	28.73%	2.683%
9	8.710	933	939	954	rBV	391077	627436	36.60%	3.418%
10	9.169	1010	1017	1030	rBV	328212	537307	31.34%	2.927%
11	9.892	1132	1140	1150	rBV	279159	455545	26.58%	2.482%
12	10.434	1224	1232	1246	rBV	365227	621675	36.27%	3.387%
13	10.810	1289	1296	1303	rBV	385713	629866	36.74%	3.432%
14	10.957	1314	1321	1331	rBV	342831	601212	35.07%	3.275%
15	12.398	1562	1566	1571	rVB5	2745	4674	0.27%	0.025%
16	14.039	1839	1845	1855	rBV	629080	826340	48.21%	4.502%
17	14.327	1887	1894	1906	rBV	643646	922495	53.82%	5.026%
18	14.633	1939	1946	1953	rBV	539876	774134	45.16%	4.218%
19	14.833	1974	1980	1992	rBV	240251	395161	23.05%	2.153%
20	15.621	2107	2114	2121	rBV	796667	1144155	66.75%	6.233%
21	15.745	2129	2135	2150	rVB	327274	449067	26.20%	2.447%
22	15.857	2150	2154	2157	rBV5	3278	4712	0.27%	0.026%
23	16.810	2313	2316	2318	rBV3	2195	2222	0.13%	0.012%
24	17.368	2405	2411	2422	rBV	644785	905011	52.80%	4.931%
25	17.468	2422	2428	2440	rBV	928753	1254227	73.17%	6.833%
26	17.815	2484	2487	2489	rBV4	1443	1900	0.11%	0.010%
27	17.880	2494	2498	2504	rVB7	2617	5776	0.34%	0.031%
28	18.104	2533	2536	2539	rVB5	1396	1998	0.12%	0.011%
29	18.410	2586	2588	2590	rBV2	2471	2352	0.14%	0.013%
30	18.662	2629	2631	2635	rBV4	1404	1927	0.11%	0.010%
31	18.821	2655	2658	2661	rBV4	2975	3914	0.23%	0.021%
32	19.027	2691	2693	2695	rBV3	2045	2081	0.12%	0.011%
33	19.321	2739	2743	2747	rVB3	7991	10894	0.64%	0.059%
34	19.392	2752	2755	2760	rVV2	7891	9409	0.55%	0.051%
35	19.756	2811	2817	2828	rBV	1189277	1497342	87.35%	8.158%
36	20.727	2978	2982	2987	rBV	88414	95260	5.56%	0.519%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038390.D
Acq On : 06 Jan 2023 17:30
Operator : CG/JU
Sample : PB150076BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK076

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Title : SVOA CALIBRATION

37	21.539	3115	3120	3131	rBV	777230	1018257	59.40%	5.548%
38	23.815	3500	3507	3518	rBV	884230	1714185	100.00%	9.339%
39	23.968	3527	3533	3541	rBV2	564833	1112964	64.93%	6.063%




Sum of corrected areas: 18355153

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038390.D
Acq On : 06 Jan 2023 17:30
Operator : CG/JU
Sample : PB150076BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

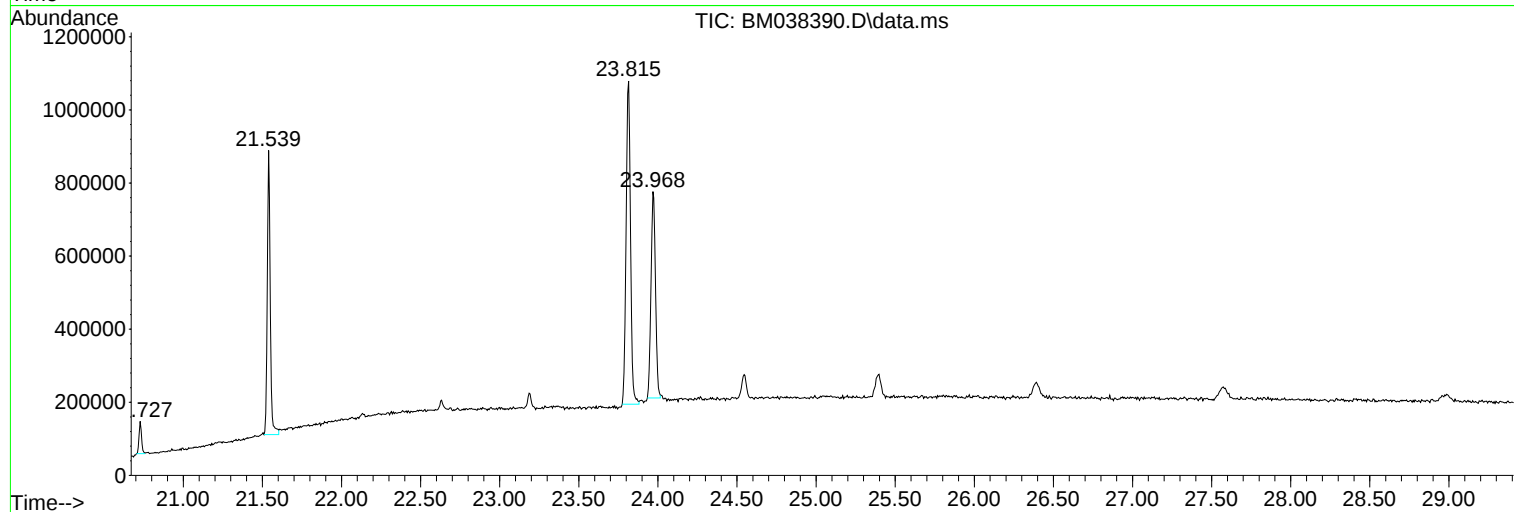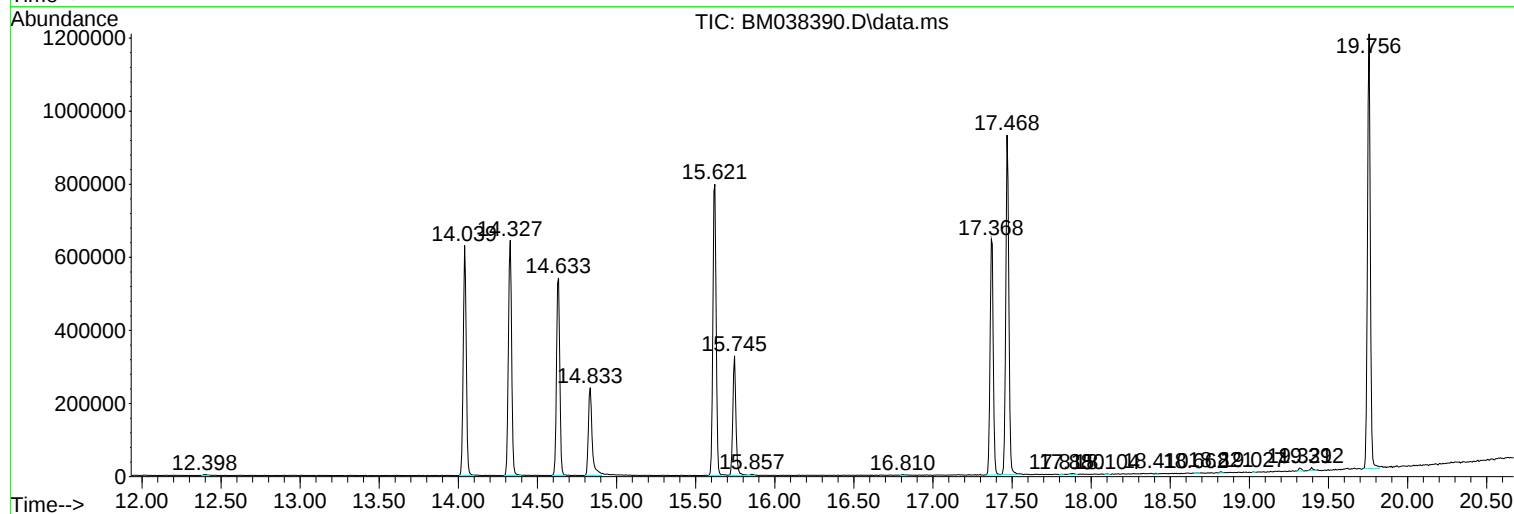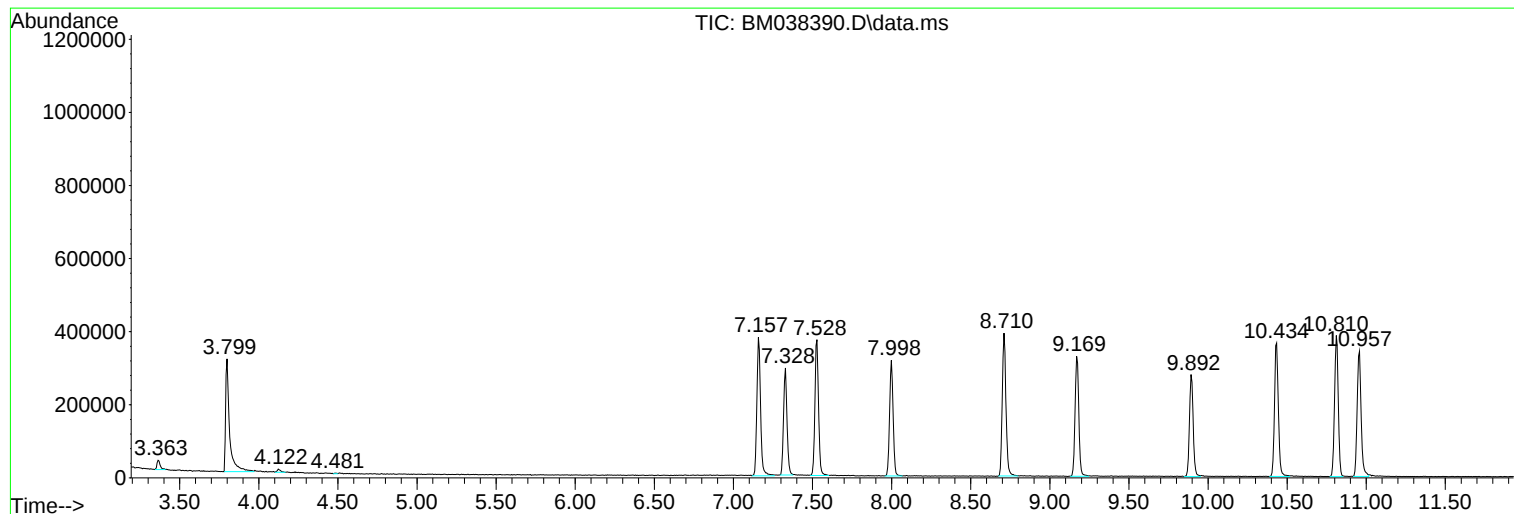

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038390.D
Acq On : 06 Jan 2023 17:30
Operator : CG/JU
Sample : PB150076BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038390.D
Acq On : 06 Jan 2023 17:30
Operator : CG/JU
Sample : PB150076BL
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK076

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc