

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
 Data File : BM038401.D
 Acq On : 07 Jan 2023 00:16
 Operator : CG/JU
 Sample : 01036-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COLD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
 Title : SVOA CALIBRATION

Signal : TIC: BM038401.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.363	26	30	35	rBV	27543	30510	1.40%	0.171%
2	3.804	101	105	119	rBV	84230	151925	6.97%	0.853%
3	4.022	138	142	147	rVB	12853	20621	0.95%	0.116%
4	4.128	156	160	168	rVB2	9041	14922	0.68%	0.084%
5	4.234	175	178	184	rVB5	8317	11542	0.53%	0.065%
6	4.504	221	224	227	rBV4	2777	3709	0.17%	0.021%
7	5.063	314	319	325	rBV3	5536	10571	0.48%	0.059%
8	6.381	538	543	545	rBV3	5014	6719	0.31%	0.038%
9	7.157	669	675	686	rBV	82000	130004	5.96%	0.730%
10	7.322	697	703	715	rBV	290434	448381	20.56%	2.516%
11	7.522	731	737	747	rBV	292838	460089	21.10%	2.582%
12	7.592	747	749	755	rVB4	3632	5094	0.23%	0.029%
13	7.992	810	817	830	rBV	293149	469263	21.52%	2.633%
14	8.710	932	939	948	rBV	198474	323947	14.86%	1.818%
15	9.169	1010	1017	1029	rBV	343703	551414	25.29%	3.094%
16	9.545	1078	1081	1089	rVB5	2990	4640	0.21%	0.026%
17	9.892	1132	1140	1149	rBV	276394	453423	20.79%	2.545%
18	10.428	1225	1231	1241	rBV	365821	593497	27.22%	3.331%
19	10.498	1241	1243	1253	rVV7	2922	6137	0.28%	0.034%
20	10.810	1288	1296	1305	rBV	363122	594467	27.26%	3.336%
21	10.951	1312	1320	1336	rBV	198300	345699	15.85%	1.940%
22	11.351	1383	1388	1391	rBV5	1655	2374	0.11%	0.013%
23	11.410	1395	1398	1402	rVB5	1361	2229	0.10%	0.013%
24	12.033	1499	1504	1508	rBV2	7919	11110	0.51%	0.062%
25	12.392	1560	1565	1573	rBV3	3870	7028	0.32%	0.039%
26	13.516	1748	1756	1761	rBV2	5909	8379	0.38%	0.047%
27	14.039	1837	1845	1854	rBV	668546	864961	39.66%	4.854%
28	14.321	1886	1893	1903	rBV	735945	1053495	48.31%	5.912%
29	14.627	1939	1945	1955	rVV	573310	806062	36.96%	4.524%
30	14.833	1975	1980	1992	rBV	35875	71560	3.28%	0.402%
31	15.410	2073	2078	2081	rBV2	3807	4853	0.22%	0.027%
32	15.615	2107	2113	2121	rBV	939305	1231082	56.45%	6.909%
33	15.739	2128	2134	2149	rVB	349365	471401	21.62%	2.645%
34	15.857	2151	2154	2159	rVB4	2945	3641	0.17%	0.020%
35	17.109	2365	2367	2371	rVB4	1812	2398	0.11%	0.013%
36	17.368	2405	2411	2418	rBV	634208	840995	38.57%	4.720%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
 Data File : BM038401.D
 Acq On : 07 Jan 2023 00:16
 Operator : CG/JU
 Sample : 01036-05
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0LD9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
 Title : SVOA CALIBRATION

37	17.468	2422	2428	2440	rVV	1096909	1461072	67.00%	8.199%
38	17.557	2440	2443	2447	rVB5	3013	4612	0.21%	0.026%
39	17.880	2494	2498	2501	rVB3	2143	2932	0.13%	0.016%
40	18.251	2556	2561	2567	rBV3	9959	17537	0.80%	0.098%
41	18.327	2569	2574	2577	rVB3	2877	4492	0.21%	0.025%
42	18.509	2602	2605	2607	rBV4	1729	2535	0.12%	0.014%
43	18.821	2655	2658	2660	rVB4	2620	2628	0.12%	0.015%
44	19.321	2738	2743	2746	rBV3	11813	16132	0.74%	0.091%
45	19.392	2752	2755	2758	rBV	7847	10108	0.46%	0.057%
46	19.421	2758	2760	2765	rVB4	5528	6331	0.29%	0.036%
47	19.515	2773	2776	2783	rBV9	13259	19124	0.88%	0.107%
48	19.662	2798	2801	2809	rVB7	7452	9644	0.44%	0.054%
49	19.756	2811	2817	2826	rBV	1394702	1777900	81.53%	9.977%
50	20.727	2978	2982	2987	rBV	77683	81068	3.72%	0.455%
51	21.539	3115	3120	3128	rBV	798398	1000303	45.87%	5.614%
52	23.809	3499	3506	3515	rBV	1132296	2180673	100.00%	12.238%
53	23.968	3527	3533	3544	rVB2	643388	1204027	55.21%	6.757%




Sum of corrected areas: 17819260

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038401.D
Acq On : 07 Jan 2023 00:16
Operator : CG/JU
Sample : 01036-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COLD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

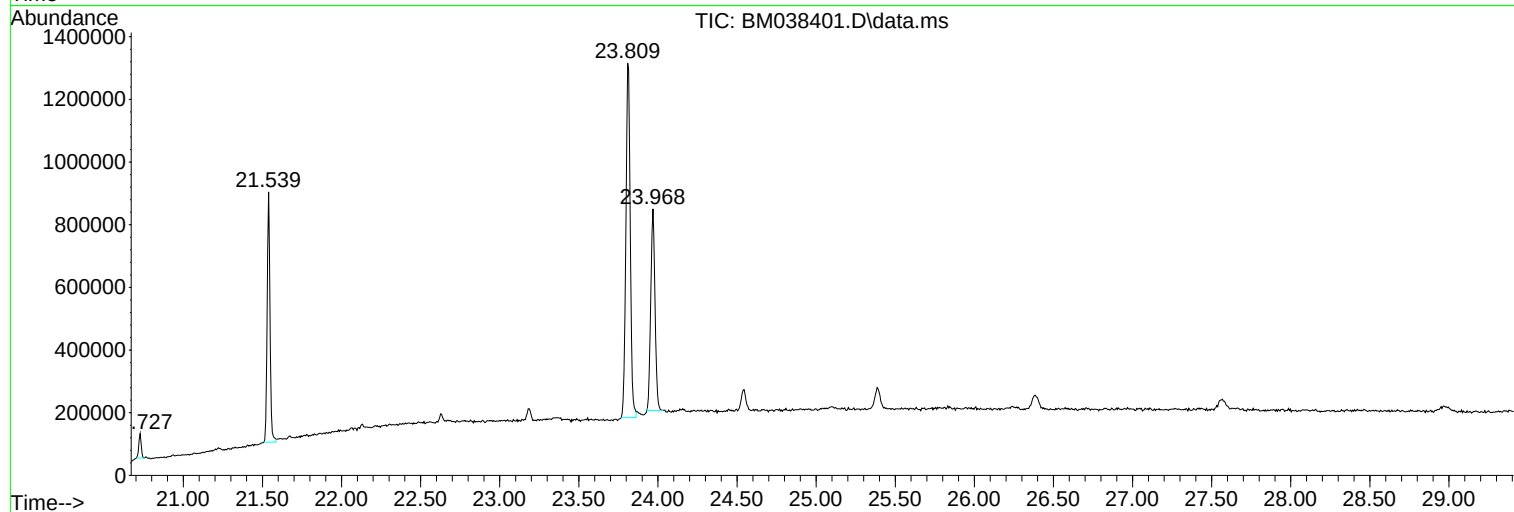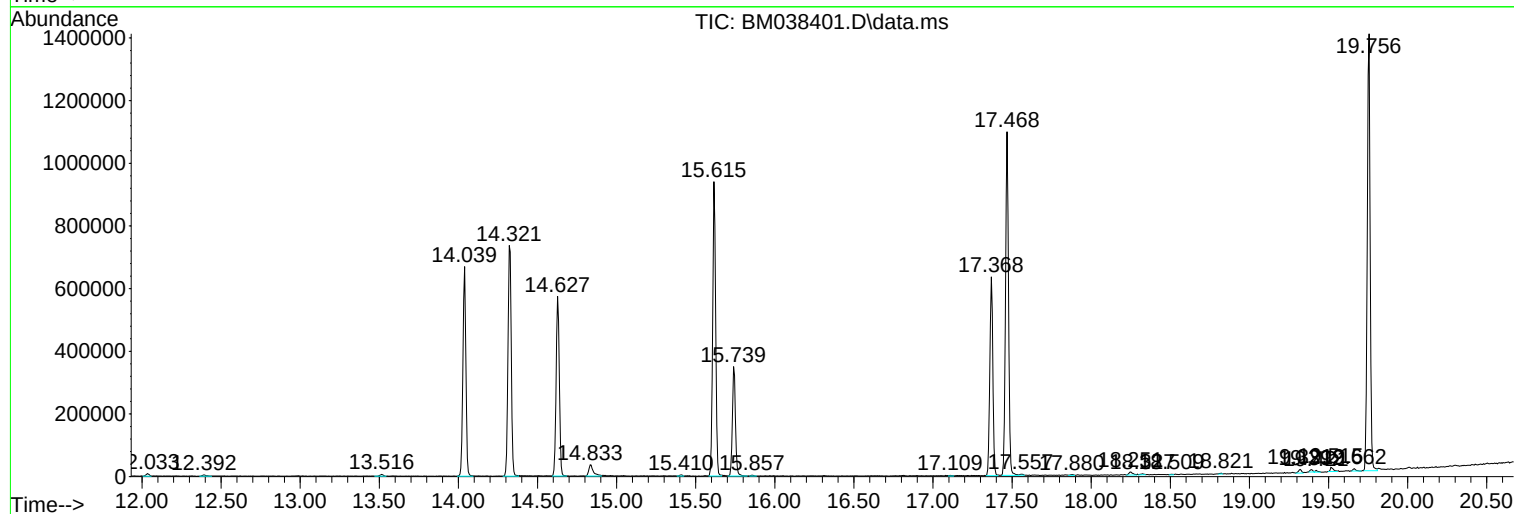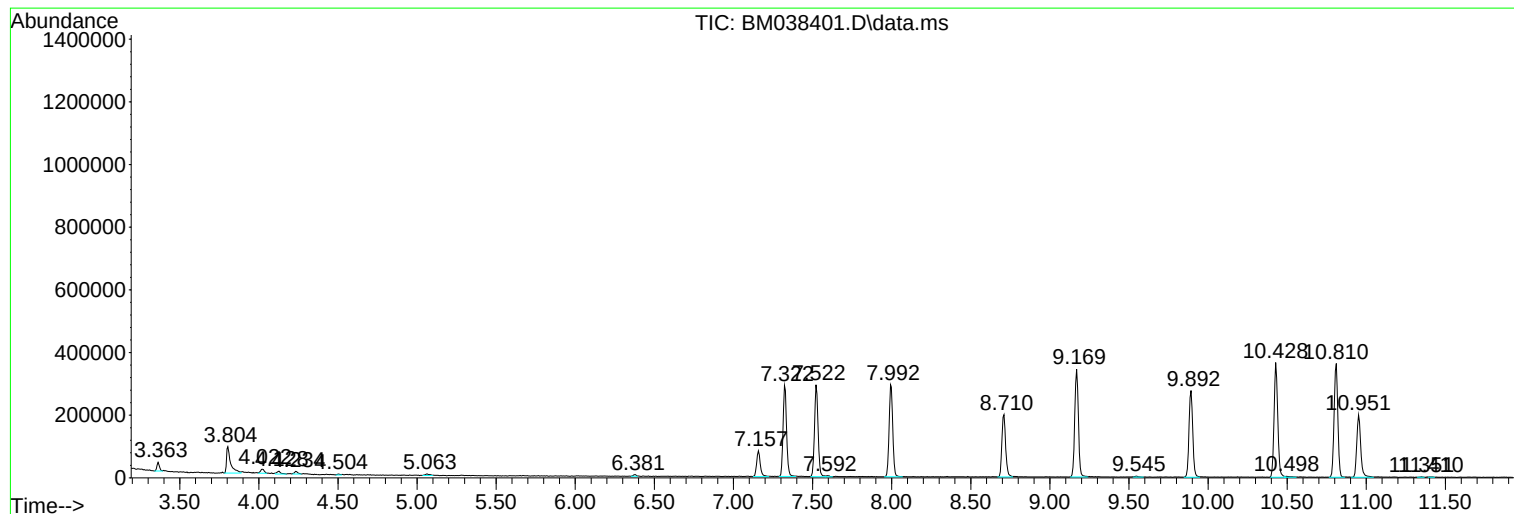

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038401.D
Acq On : 07 Jan 2023 00:16
Operator : CG/JU
Sample : 01036-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM010623\
Data File : BM038401.D
Acq On : 07 Jan 2023 00:16
Operator : CG/JU
Sample : 01036-05
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0LD9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM010423.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------