
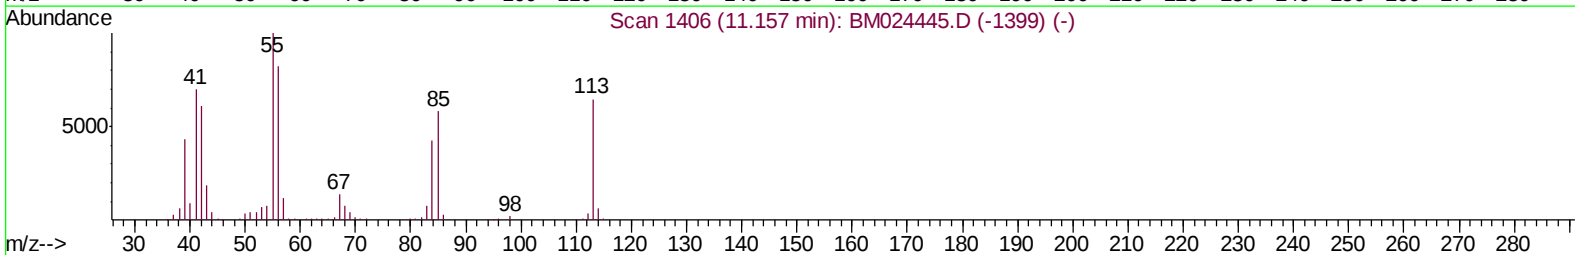
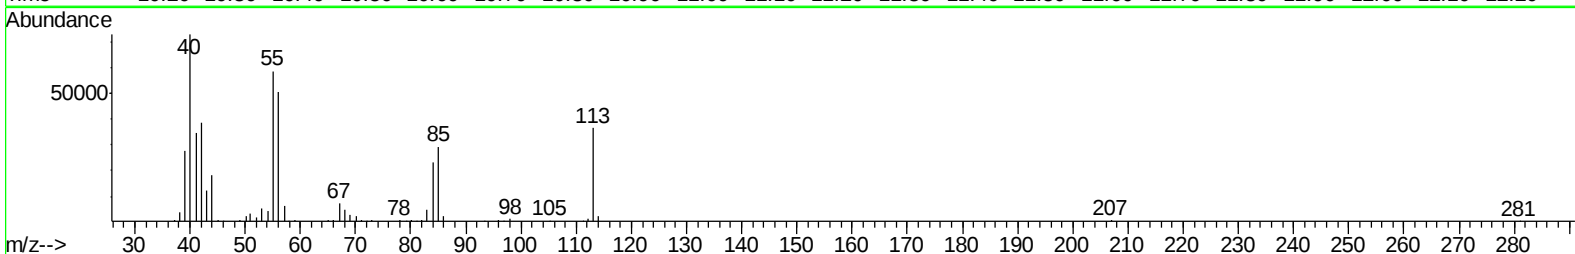


Data File : BM024451.D
Acq On : 10 Jan 2020 07:35
Operator : JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Jan 10 08:13:39 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 07:52:51 2020
Response via : Initial Calibration

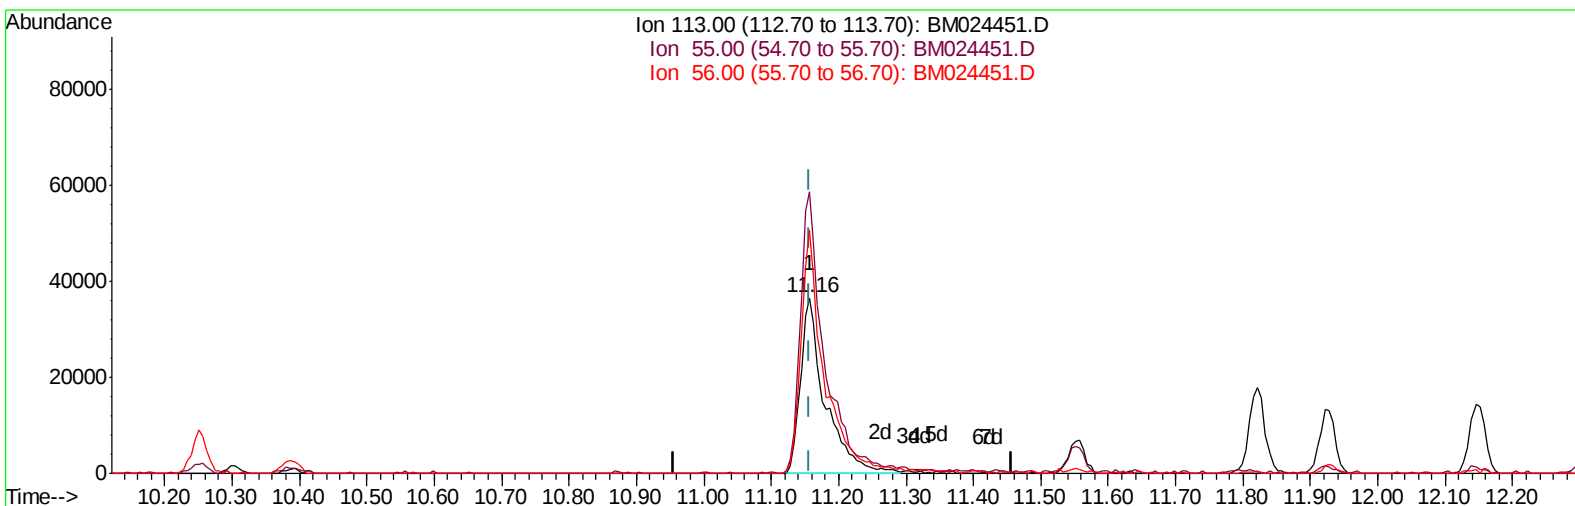

TIC: BM024451.D

(32) Caprolactam

11.157min (-0.000) 18.56ng/ul m

response 92686

Ion	Exp%	Act%
113.00	100	100
55.00	161.50	160.47
56.00	122.30	138.74
0.00	0.00	0.00