

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024430.D
 Acq On : 09 Jan 2020 18:31
 Operator : JU
 Sample : K6466-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BQ8

Quant Time: Jan 10 06:53:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 06:51:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	286060	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1113829	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.14	164	672253	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1445431	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1425913	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1708676	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.10	96	35452	5.35	ng/uL	0.00
5) Phenol-d5	6.68	99	131224	5.87	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	364676	27.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	412893	21.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	240878	13.42	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	259324	31.05	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	233216	29.13	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	438335	24.95	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	58168	2.94	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1640603	33.97	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1936897	31.07	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	44009	5.17	ng/ul	0.00
58) Fluorene-d10	15.14	176	1386456	32.39	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	152661	23.57	ng/ul	0.00
71) Anthracene-d10	16.99	188	2212042	32.68	ng/ul	0.00
79) Pyrene-d10	19.29	212	2551305	33.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2919051	33.46	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.61	163	109262	2.205	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024430.D
Acq On : 09 Jan 2020 18:31
Operator : JU
Sample : K6466-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BQ8

Quant Time: Jan 10 06:53:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 06:51:26 2020
Response via : Initial Calibration

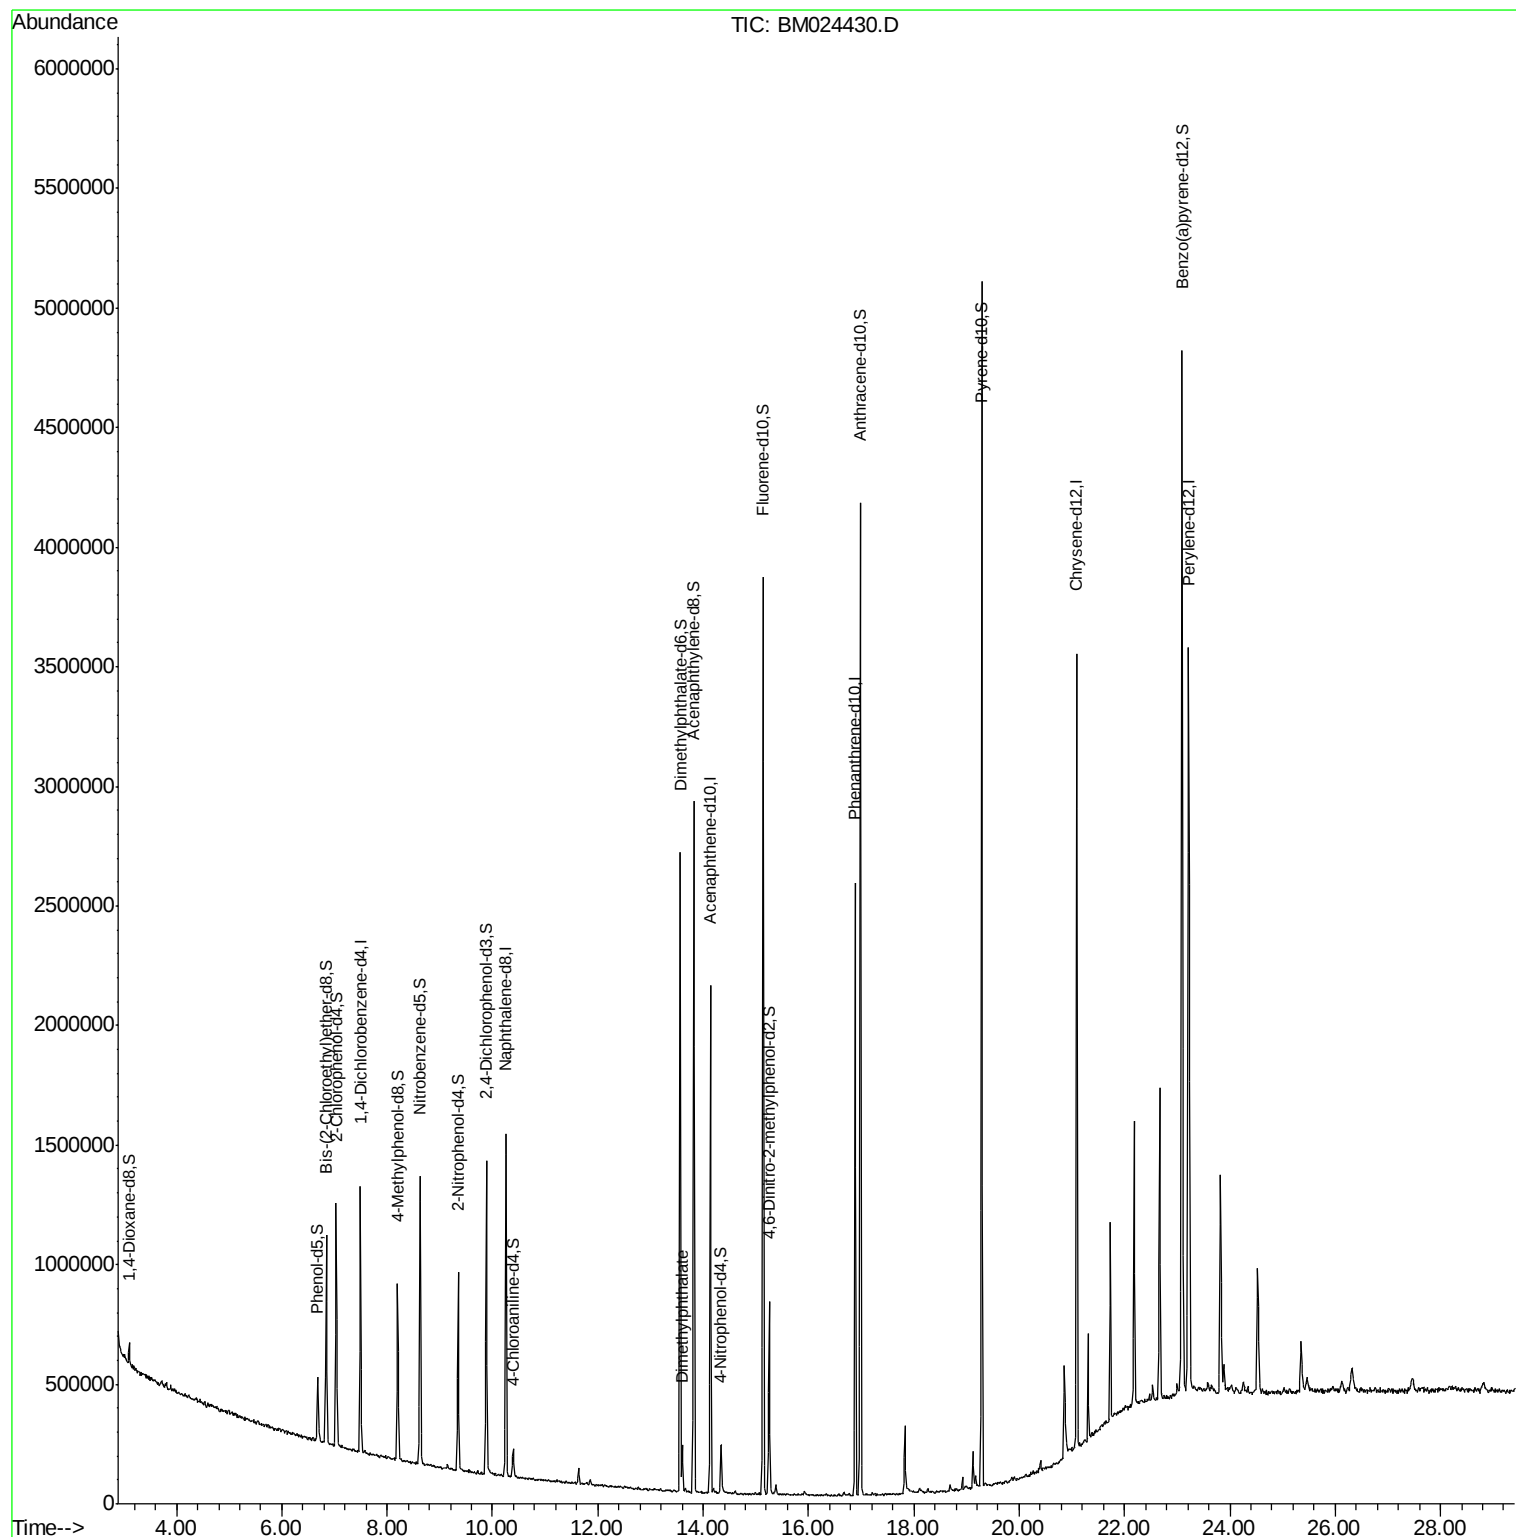

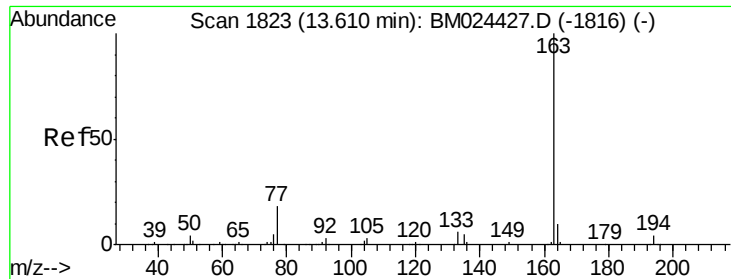

#45

Dimethylphthalate

Concen: 2.205 ng/ul

RT: 13.61 min Scan# 1823

Delta R.T. 0.00 min

Lab File: BM024430.D

Acq: 09 Jan 2020 18:31

Instrument :

BNA_M

ClientSampleId :

H0BQ8


Tot Ion:163 Resp: 109262

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 10.5 8.2 12.4

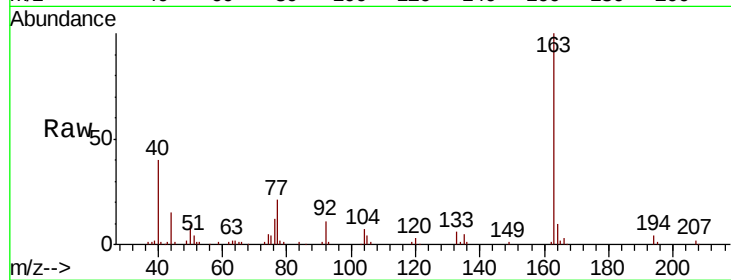

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

