

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024431.D
 Acq On : 09 Jan 2020 19:06
 Operator : JU
 Sample : K6466-16
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BP4

Quant Time: Jan 10 06:53:56 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 06:51:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.50	152	327066	20.00	ng/ul	0.00
18) Naphthalene-d8	10.26	136	1259813	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.14	164	737379	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1537797	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1484452	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1780259	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	35851	4.73	ng/uL	0.00
5) Phenol-d5	6.68	99	130931	5.13	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	369168	24.65	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	423882	19.64	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	240069	11.70	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	260284	27.55	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	226321	24.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	434058	21.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	43774	1.95	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1513728	28.58	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1794288	26.24	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	41253	4.42	ng/ul	0.00
58) Fluorene-d10	15.14	176	1302647	27.75	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	137374	19.94	ng/ul	0.00
71) Anthracene-d10	16.99	188	2047928	28.43	ng/ul	0.00
79) Pyrene-d10	19.29	212	2321028	29.27	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2637836	29.02	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.61	163	58005	1.067	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024431.D
Acq On : 09 Jan 2020 19:06
Operator : JU
Sample : K6466-16
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BP4

Quant Time: Jan 10 06:53:56 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 06:51:26 2020
Response via : Initial Calibration

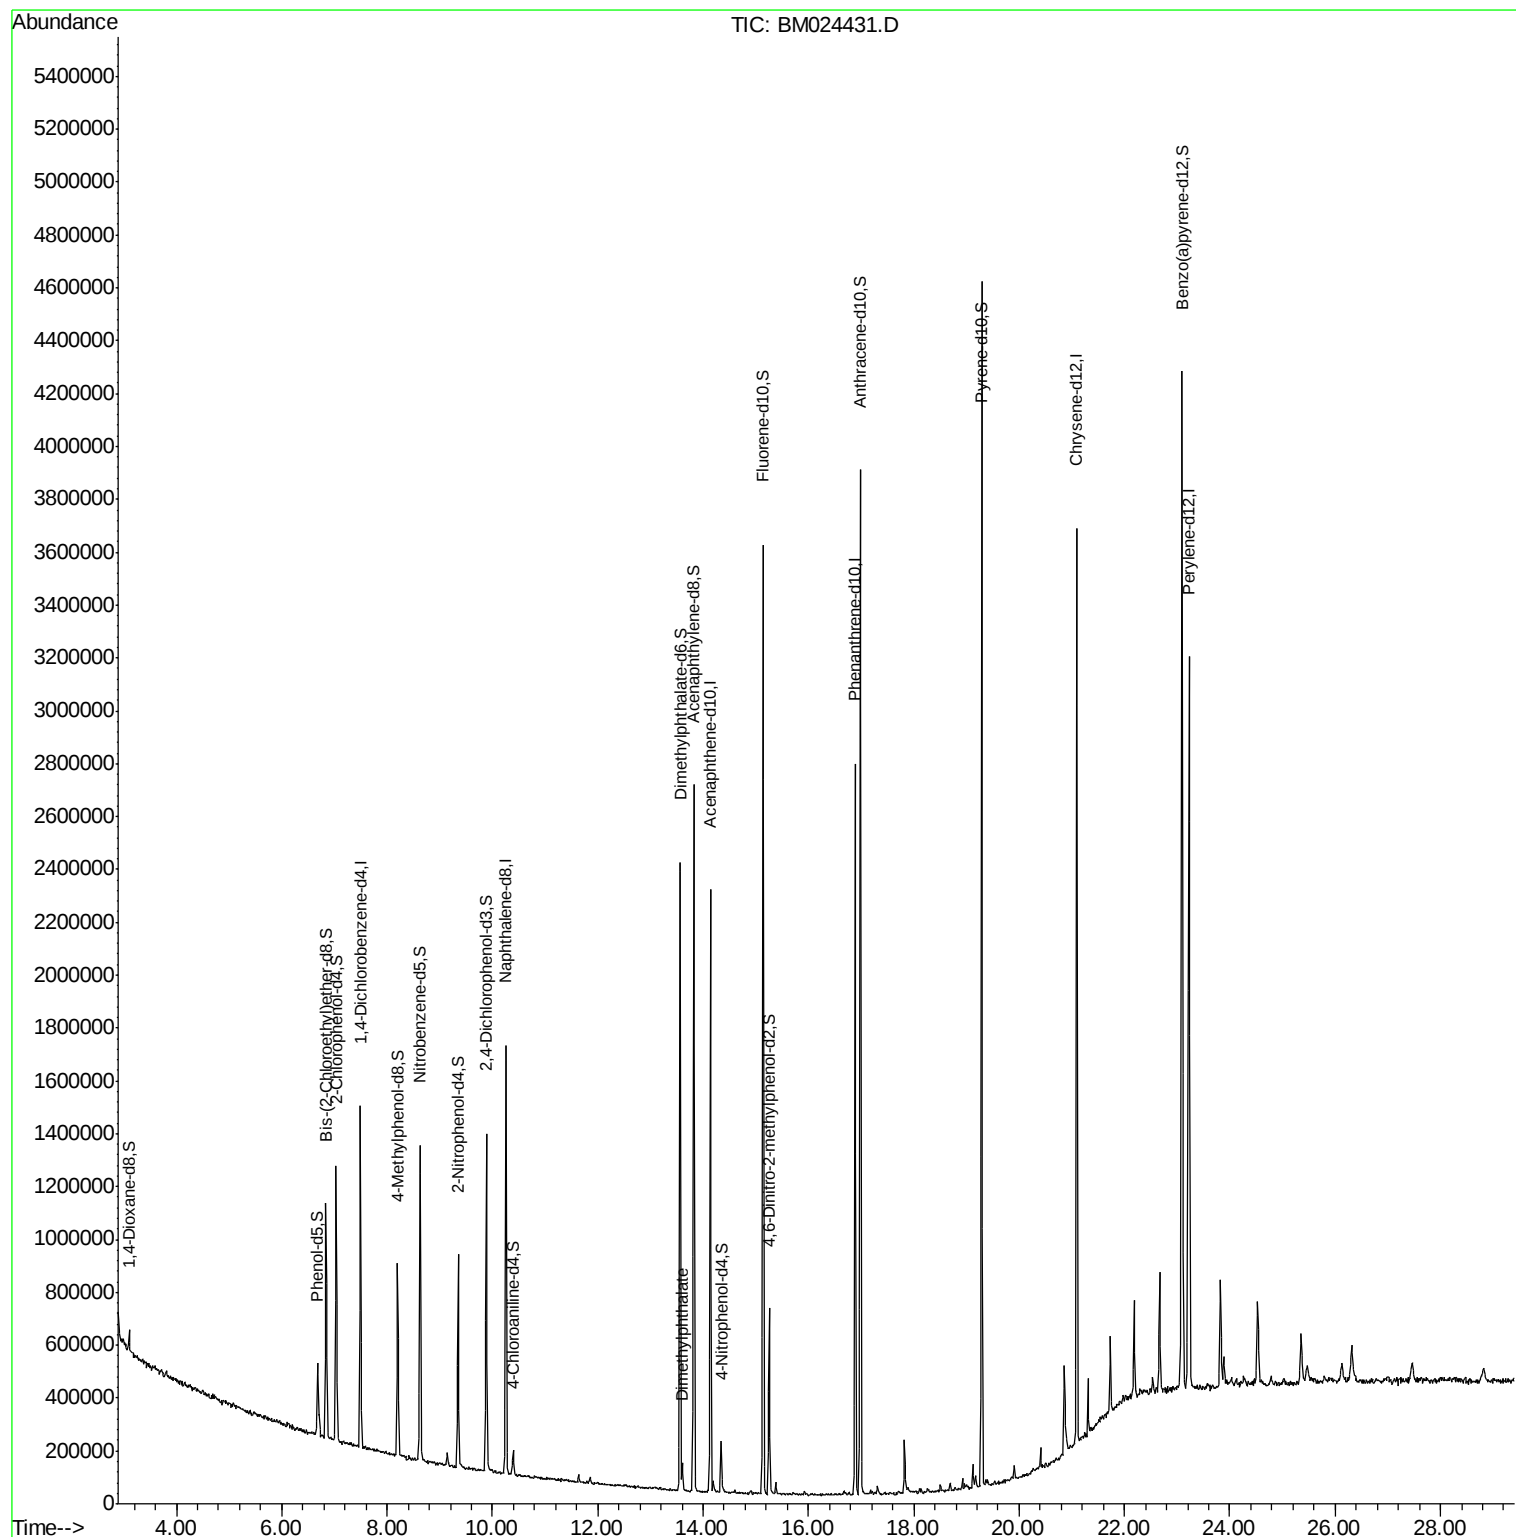

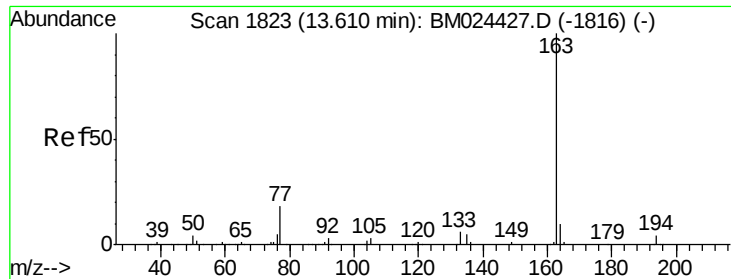

#45

Dimethylphthalate

Concen: 1.067 ng/ul

RT: 13.61 min Scan# 1823

Delta R.T. 0.00 min

Lab File: BM024431.D

Acq: 09 Jan 2020 19:06

Instrument :

BNA_M

ClientSampleId :

H0BP4


Tot Ion:163 Resp: 58005

Ion Ratio Lower Upper

163 100

194 3.7 3.2 4.8

164 9.9 8.2 12.4

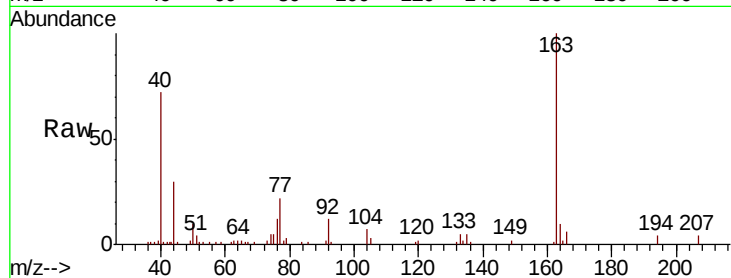

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

