

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024437.D
 Acq On : 09 Jan 2020 22:40
 Operator : JU
 Sample : K6466-22
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BR1

Quant Time: Jan 10 06:54:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 06:51:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	322509	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	1211834	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.14	164	698522	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1460362	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1444154	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1752935	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	39514	5.29	ng/uL	0.00
5) Phenol-d5	6.68	99	119974	4.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	354980	24.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	399057	18.75	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	224049	11.08	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	253298	27.87	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	205008	23.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	413457	21.63	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	47304	2.19	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1514902	30.19	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1753600	27.07	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	40657	4.60	ng/ul	0.00
58) Fluorene-d10	15.14	176	1286869	28.94	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	146012	22.32	ng/ul	0.00
71) Anthracene-d10	16.99	188	2157517	31.54	ng/ul	0.00
79) Pyrene-d10	19.29	212	2490584	32.28	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2922754	32.65	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.60	163	67124	1.304	ng/ul# 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024437.D
Acq On : 09 Jan 2020 22:40
Operator : JU
Sample : K6466-22
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BR1

Quant Time: Jan 10 06:54:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 06:51:26 2020
Response via : Initial Calibration

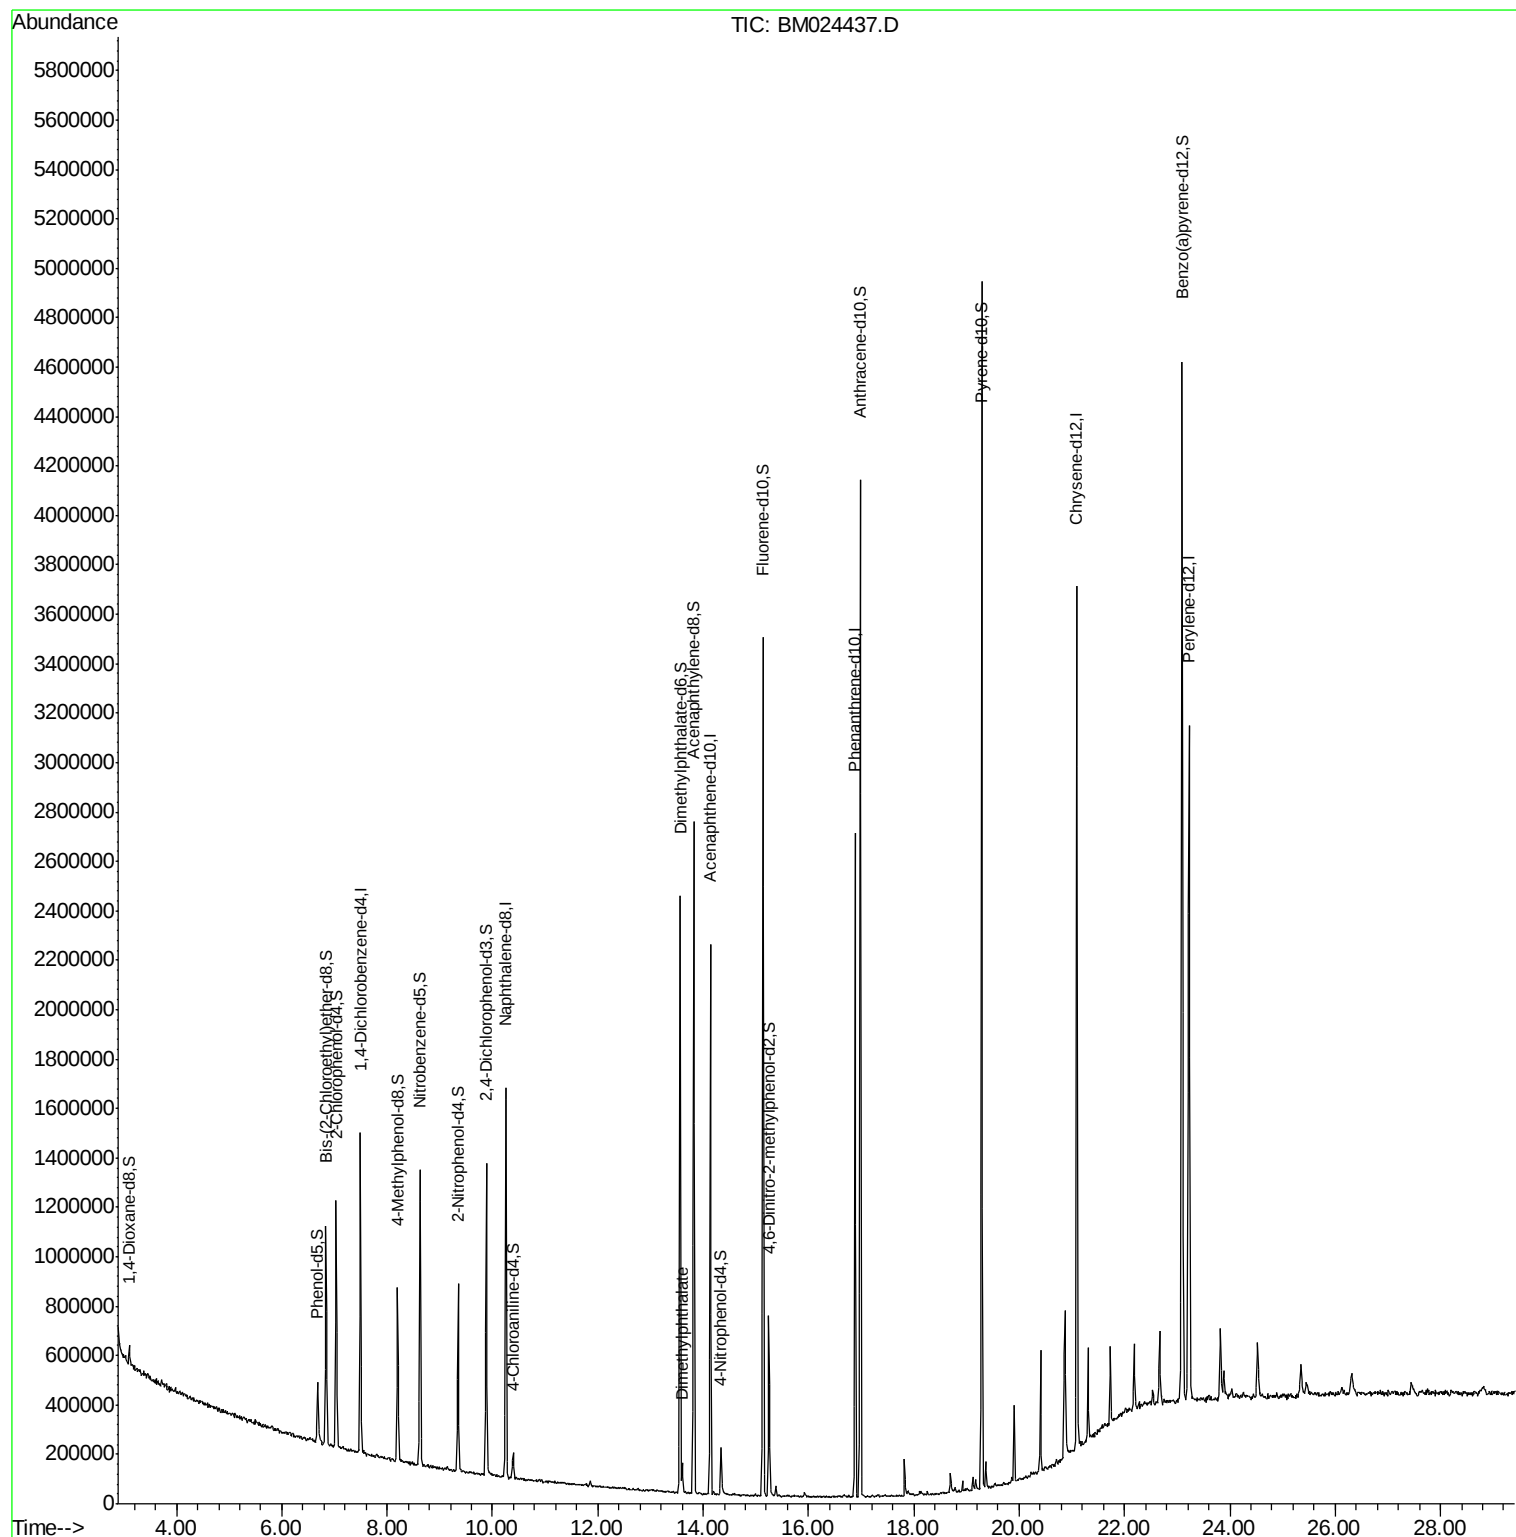

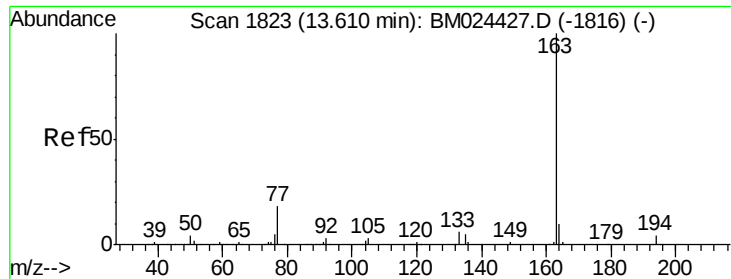

#45

Dimethylphthalate

Concen: 1.304 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. -0.01 min

Lab File: BM024437.D

Acq: 09 Jan 2020 22:40

Instrument :

BNA_M

ClientSampleId :

H0BR1


Tot Ion:163 Resp: 67124

Ion Ratio Lower Upper

163 100

194 4.3 3.2 4.8

164 8.2 8.2 12.4#

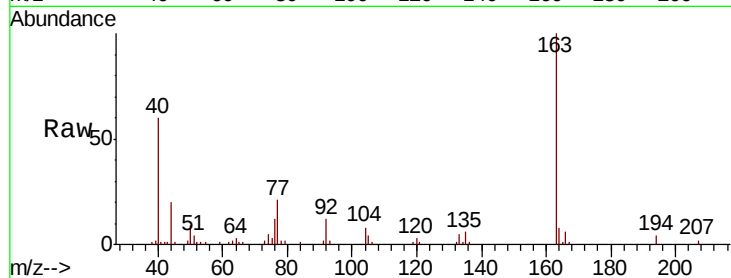

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

