

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024443.D
 Acq On : 10 Jan 2020 02:14
 Operator : JU
 Sample : K6466-06
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BP3

Quant Time: Jan 10 06:55:17 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 06:51:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	295228	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	1120933	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.14	164	669021	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1457057	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1471969	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1774443	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.10	96	37512	5.48	ng/uL	0.00
5) Phenol-d5	6.68	99	92367	4.01	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	325043	24.04	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	357129	18.33	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	184810	9.98	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	230761	27.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	188793	23.43	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	395107	22.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	32148	1.61	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1533886	31.92	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1768679	28.51	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	31862	3.76	ng/ul	0.00
58) Fluorene-d10	15.14	176	1326640	31.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	150062	22.99	ng/ul	0.00
71) Anthracene-d10	16.99	188	2172025	31.83	ng/ul	0.00
79) Pyrene-d10	19.29	212	2563272	32.59	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2953243	32.60	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.60	163	56541	1.147	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024443.D
Acq On : 10 Jan 2020 02:14
Operator : JU
Sample : K6466-06
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BP3

Quant Time: Jan 10 06:55:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 06:51:26 2020
Response via : Initial Calibration

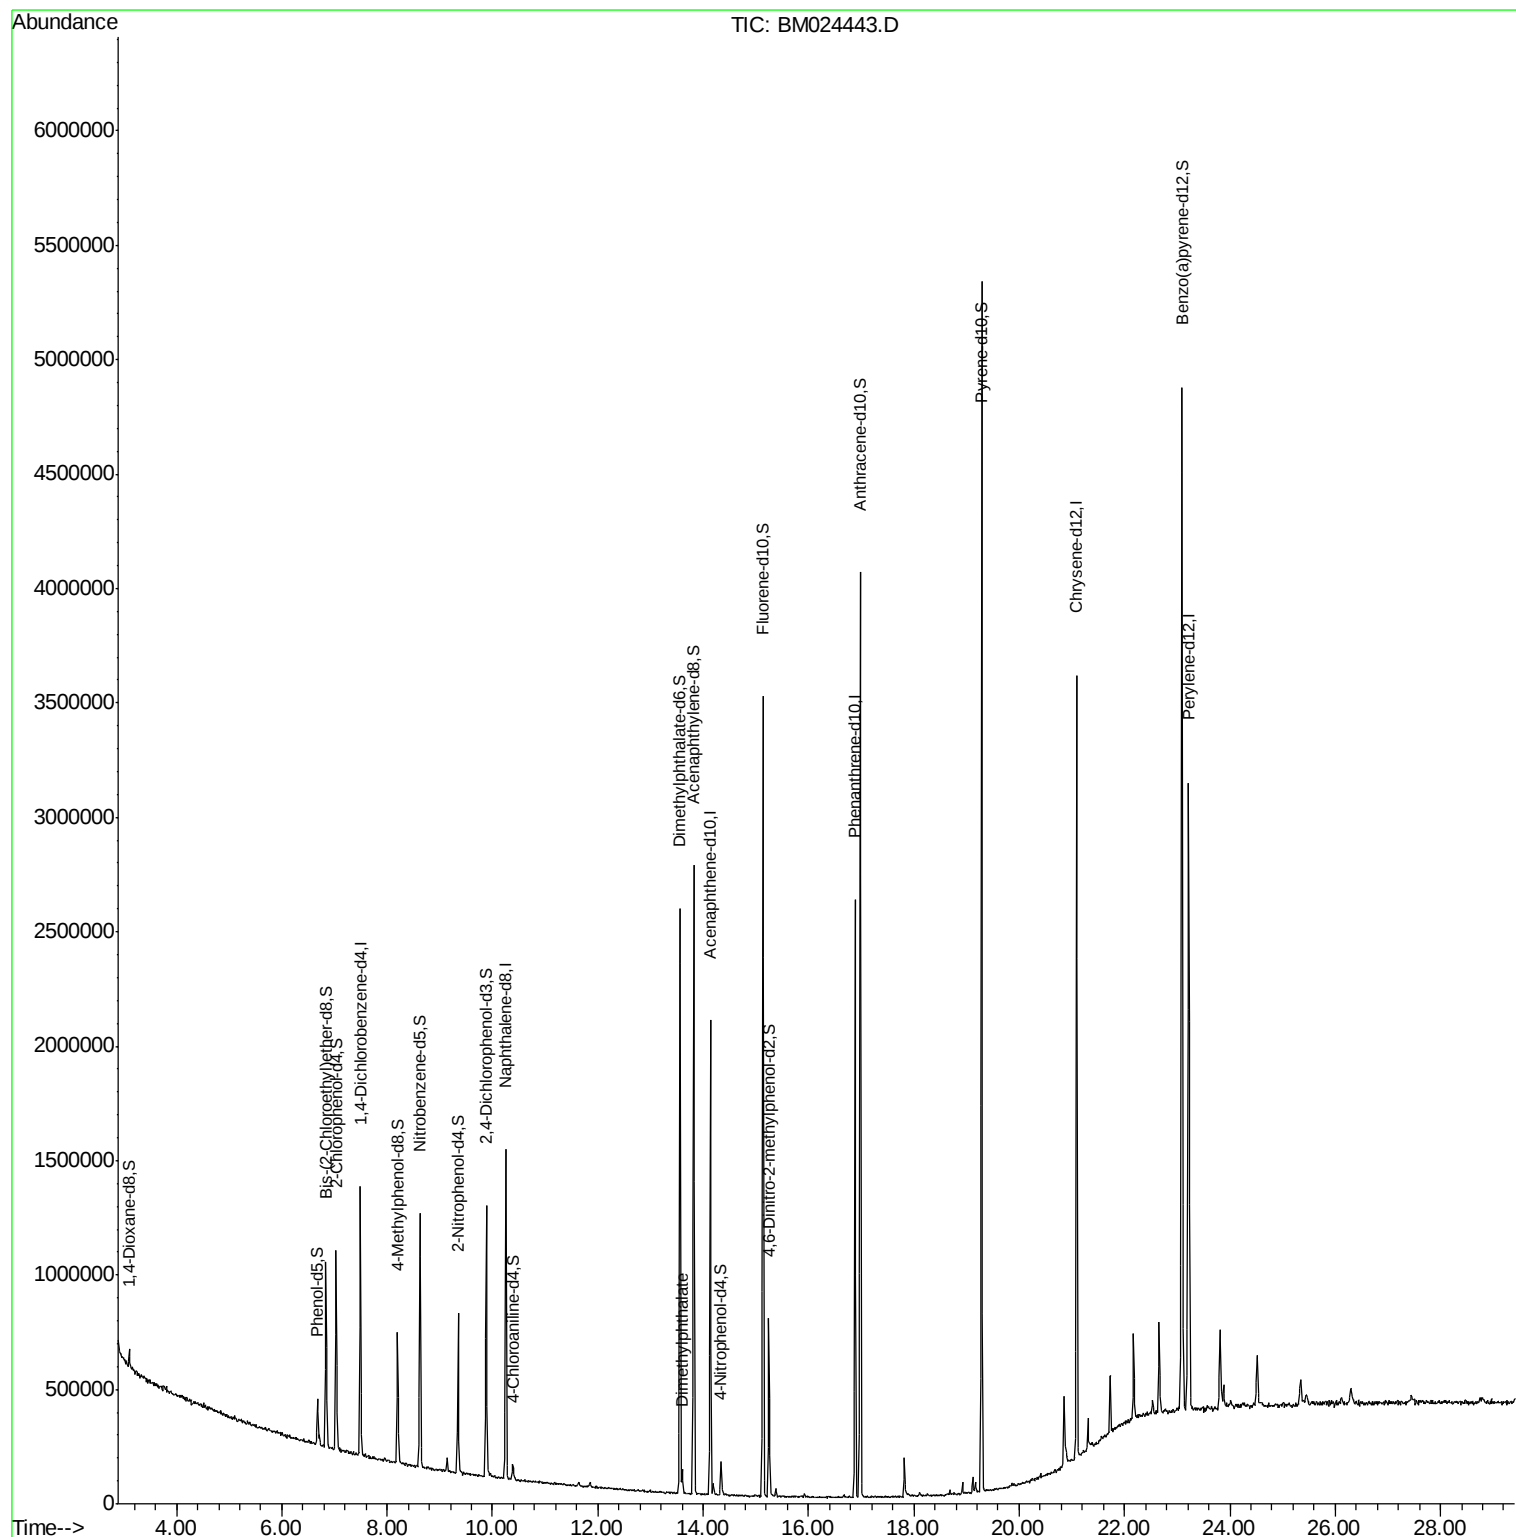


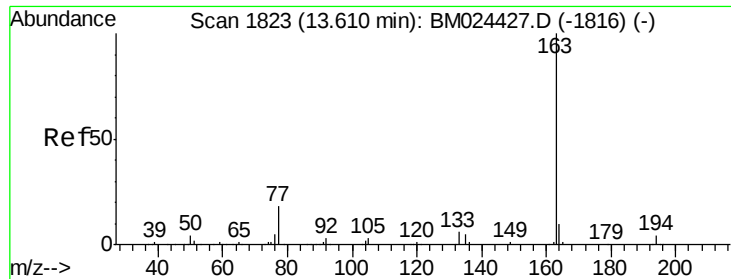

#45
 Dimethylphthalate
 Concen: 1.147 ng/ul
 RT: 13.60 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM024443.D
 Acq: 10 Jan 2020 02:14

Instrument :
 BNA_M
 ClientSampleId :
 H0BP3

Tot Ion:163 Resp: 56541
 Ion Ratio Lower Upper
 163 100
 194 3.4 3.2 4.8
 164 10.4 8.2 12.4

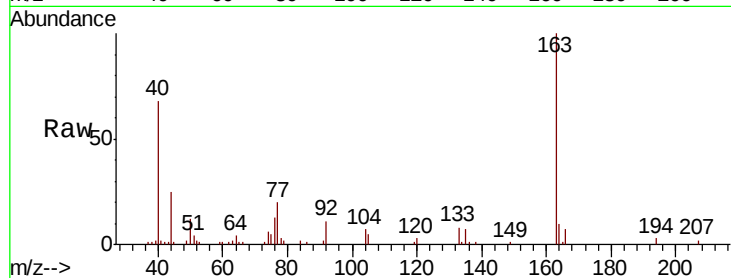

Abundance Ion 163.00 (162.70 to 163.70): E
 Ion 194.00 (193.70 to 194.70): E
 Ion 164.00 (163.70 to 164.70): E

