

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024444.D
 Acq On : 10 Jan 2020 02:50
 Operator : JU
 Sample : K6466-07
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BQ4

Quant Time: Jan 10 06:55:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 06:51:26 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	347943	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	1309936	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	735446	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1443446	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1351527	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1645137	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	44922	5.57	ng/uL	0.00
5) Phenol-d5	6.68	99	122435	4.51	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	385888	24.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	428768	18.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	239592	10.98	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	269629	27.45	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	227396	24.15	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	454629	22.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	38402	1.65	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1574642	29.81	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1836944	26.93	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	35017	3.76	ng/ul	0.00
58) Fluorene-d10	15.14	176	1340722	28.63	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.26	200	148123	22.90	ng/ul	0.00
71) Anthracene-d10	16.99	188	2124189	31.42	ng/ul	0.00
79) Pyrene-d10	19.29	212	2437835	33.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2779925	33.09	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.60	163	77921	1.437	ng/ul 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024444.D
Acq On : 10 Jan 2020 02:50
Operator : JU
Sample : K6466-07
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BQ4

Quant Time: Jan 10 06:55:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 06:51:26 2020
Response via : Initial Calibration

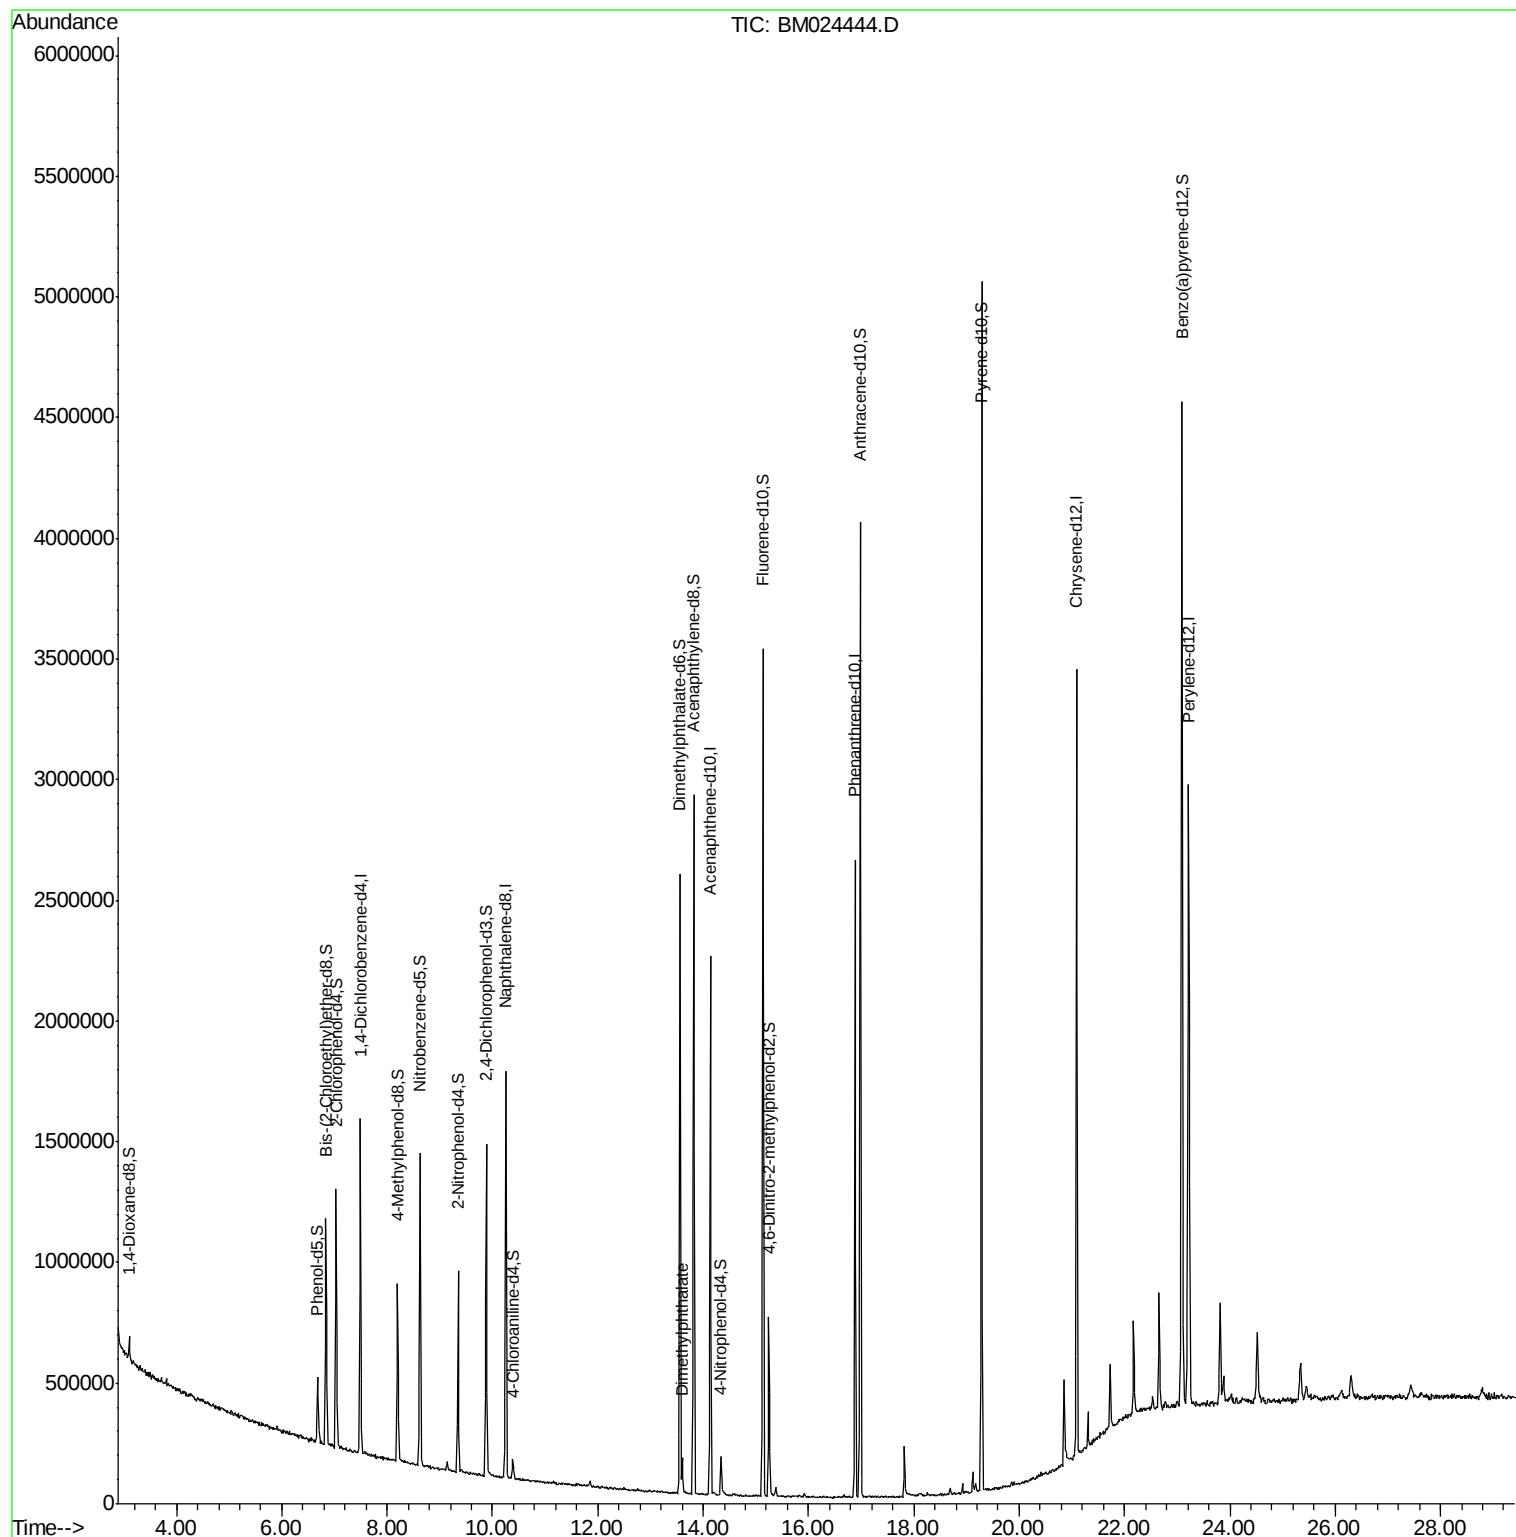


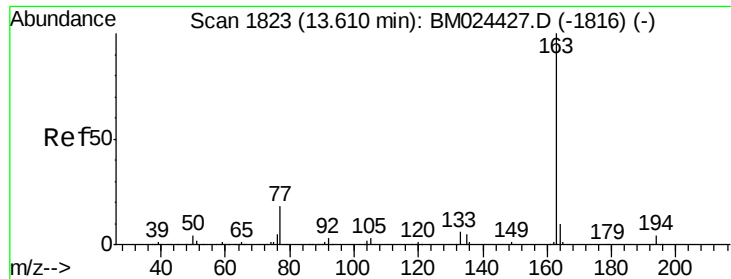

#45
 Dimethylphthalate
 Concen: 1.437 ng/ul
 RT: 13.60 min Scan# 1822
 Delta R.T. -0.01 min
 Lab File: BM024444.D
 Acq: 10 Jan 2020 02:50

Instrument :
 BNA_M
 ClientSampleId :
 H0BQ4

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.2	4.8
164	8.7	8.2	12.4

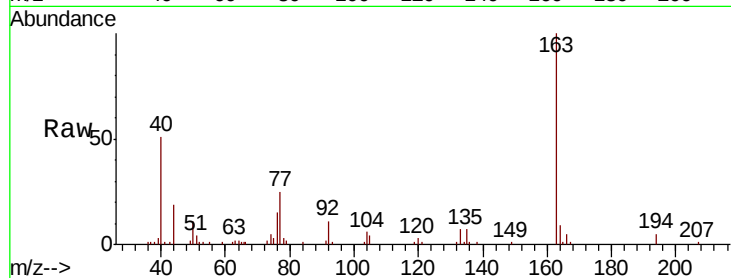

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

