

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024446.D
 Acq On : 10 Jan 2020 04:37
 Operator : JU
 Sample : K6466-08
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BQ5

Quant Time: Jan 10 07:55:06 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 07:52:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	302321	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	1156734	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	679410	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1446041	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1440574	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1677896	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	38664	5.52	ng/uL	0.00
5) Phenol-d5	6.68	99	120700	5.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	359627	25.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	397861	19.94	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	225292	11.88	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	254960	29.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	198372	23.86	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	434893	23.84	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	43449	2.11	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1651736	33.85	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1923962	30.54	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	37174	4.32	ng/ul	0.00
58) Fluorene-d10	15.13	176	1411773	32.64	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	146169	22.56	ng/ul	0.00
71) Anthracene-d10	16.98	188	2286466	33.76	ng/ul	0.00
79) Pyrene-d10	19.29	212	2648745	34.42	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2928976	34.19	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.60	163	56673	1.132	ng/ul 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024446.D
Acq On : 10 Jan 2020 04:37
Operator : JU
Sample : K6466-08
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BQ5

Quant Time: Jan 10 07:55:06 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 07:52:51 2020
Response via : Initial Calibration

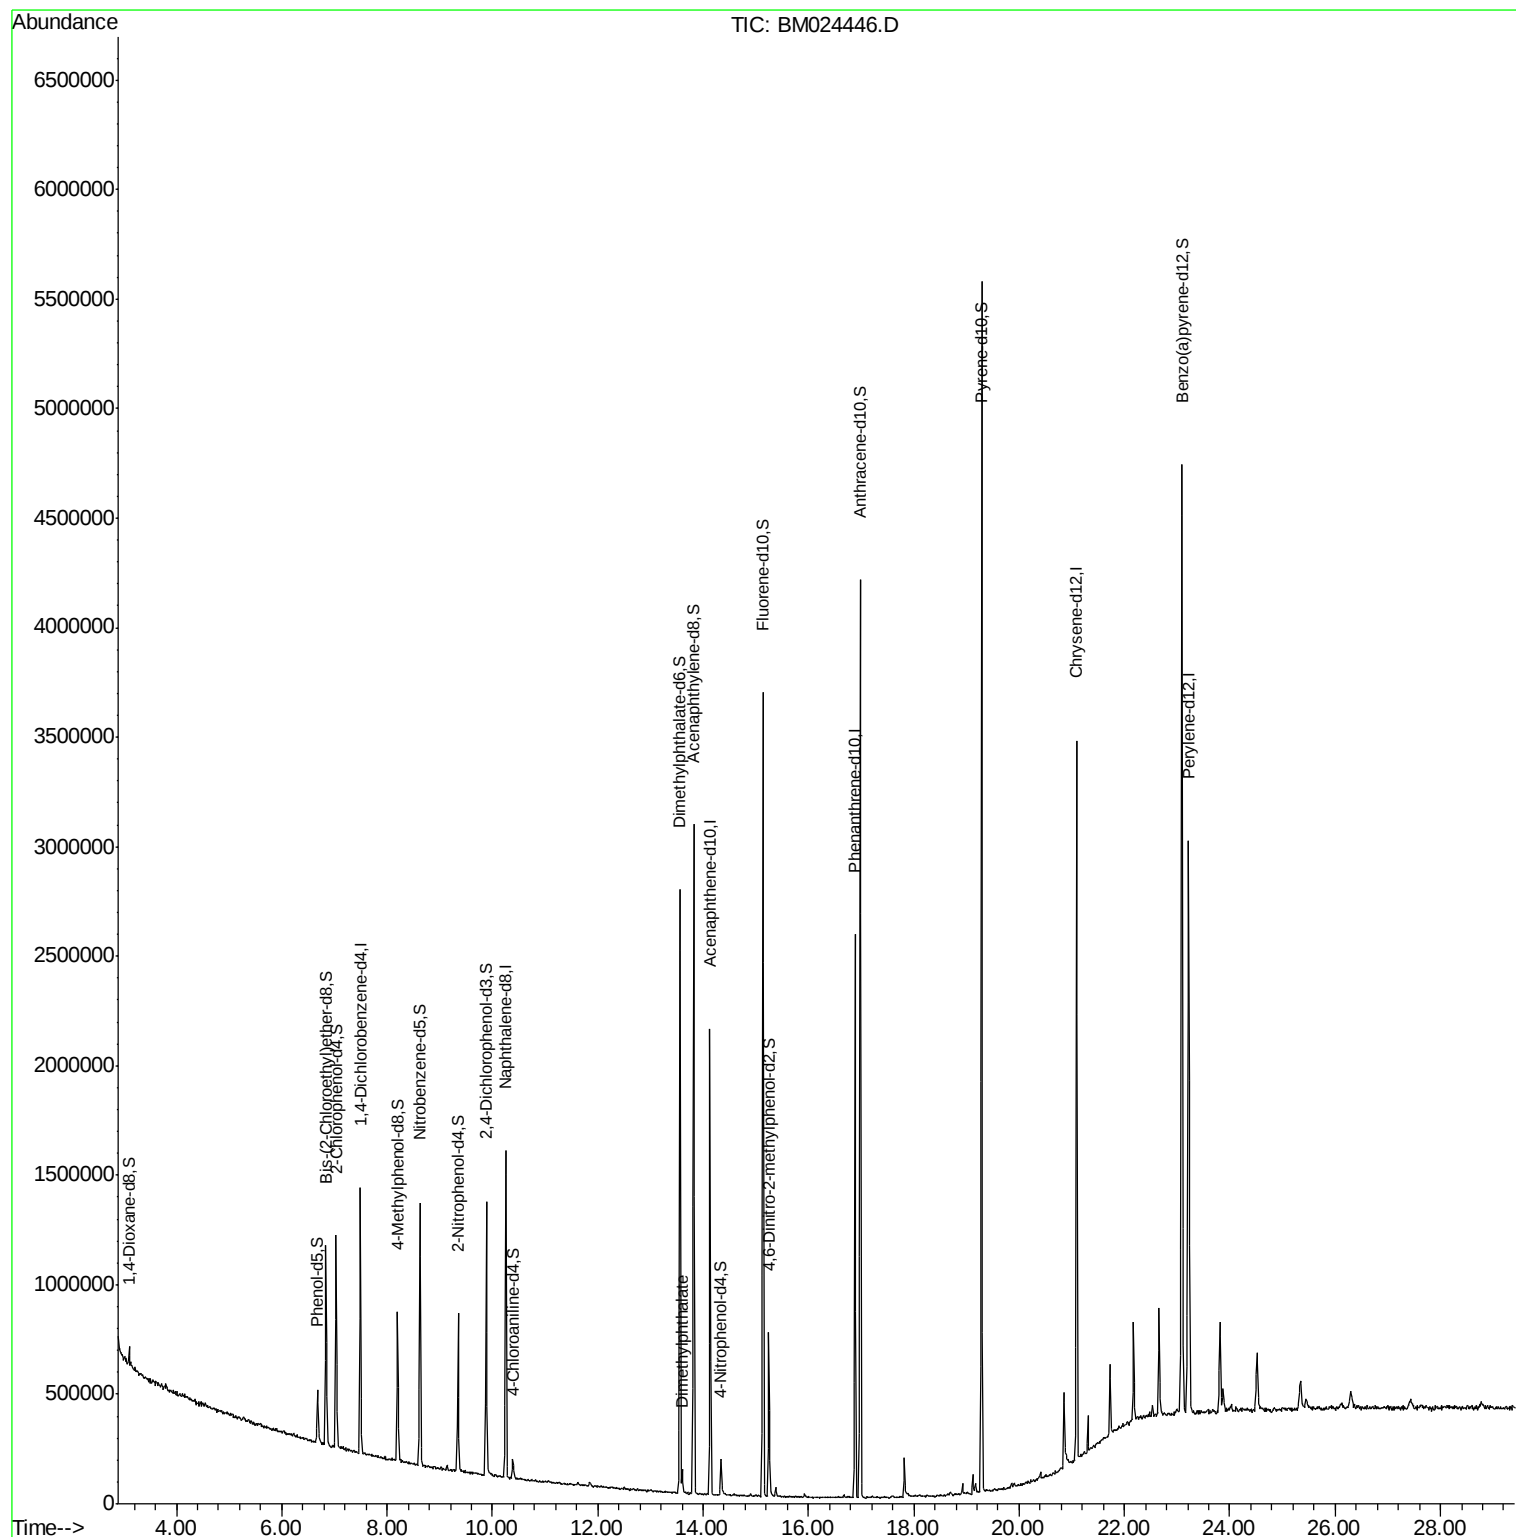

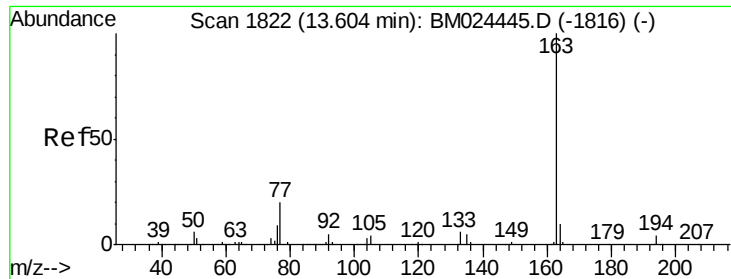

#45

Dimethylphthalate

Concen: 1.132 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. -0.00 min

Lab File: BM024446.D

Acq: 10 Jan 2020 04:37

Instrument :

BNA_M

ClientSampleId :

H0BQ5


Tot Ion:163 Resp: 56673

Ion Ratio Lower Upper

163 100

194 4.8 3.2 4.8

164 8.5 8.2 12.4

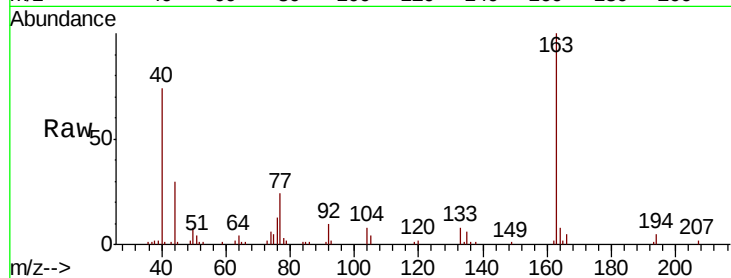

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

