

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024448.D
 Acq On : 10 Jan 2020 05:48
 Operator : JU
 Sample : K6466-10
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BP8

Quant Time: Jan 10 07:55:18 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 07:52:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	274658	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	1044934	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	621448	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1354222	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1377928	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1660301	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	38105	5.99	ng/uL	0.00
5) Phenol-d5	6.68	99	93556	4.36	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	317935	25.28	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	343974	18.97	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	184042	10.68	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	225751	28.81	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	174818	23.27	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	364652	22.13	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	21083	1.13	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1374780	30.80	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1645634	28.55	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	28470	3.62	ng/ul	0.00
58) Fluorene-d10	15.13	176	1192935	30.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	126187	20.80	ng/ul	0.00
71) Anthracene-d10	16.98	188	1897964	29.92	ng/ul	0.00
79) Pyrene-d10	19.29	212	2278800	30.95	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2636415	31.10	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.60	163	51788	1.131	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024448.D
Acq On : 10 Jan 2020 05:48
Operator : JU
Sample : K6466-10
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BP8

Quant Time: Jan 10 07:55:18 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 07:52:51 2020
Response via : Initial Calibration

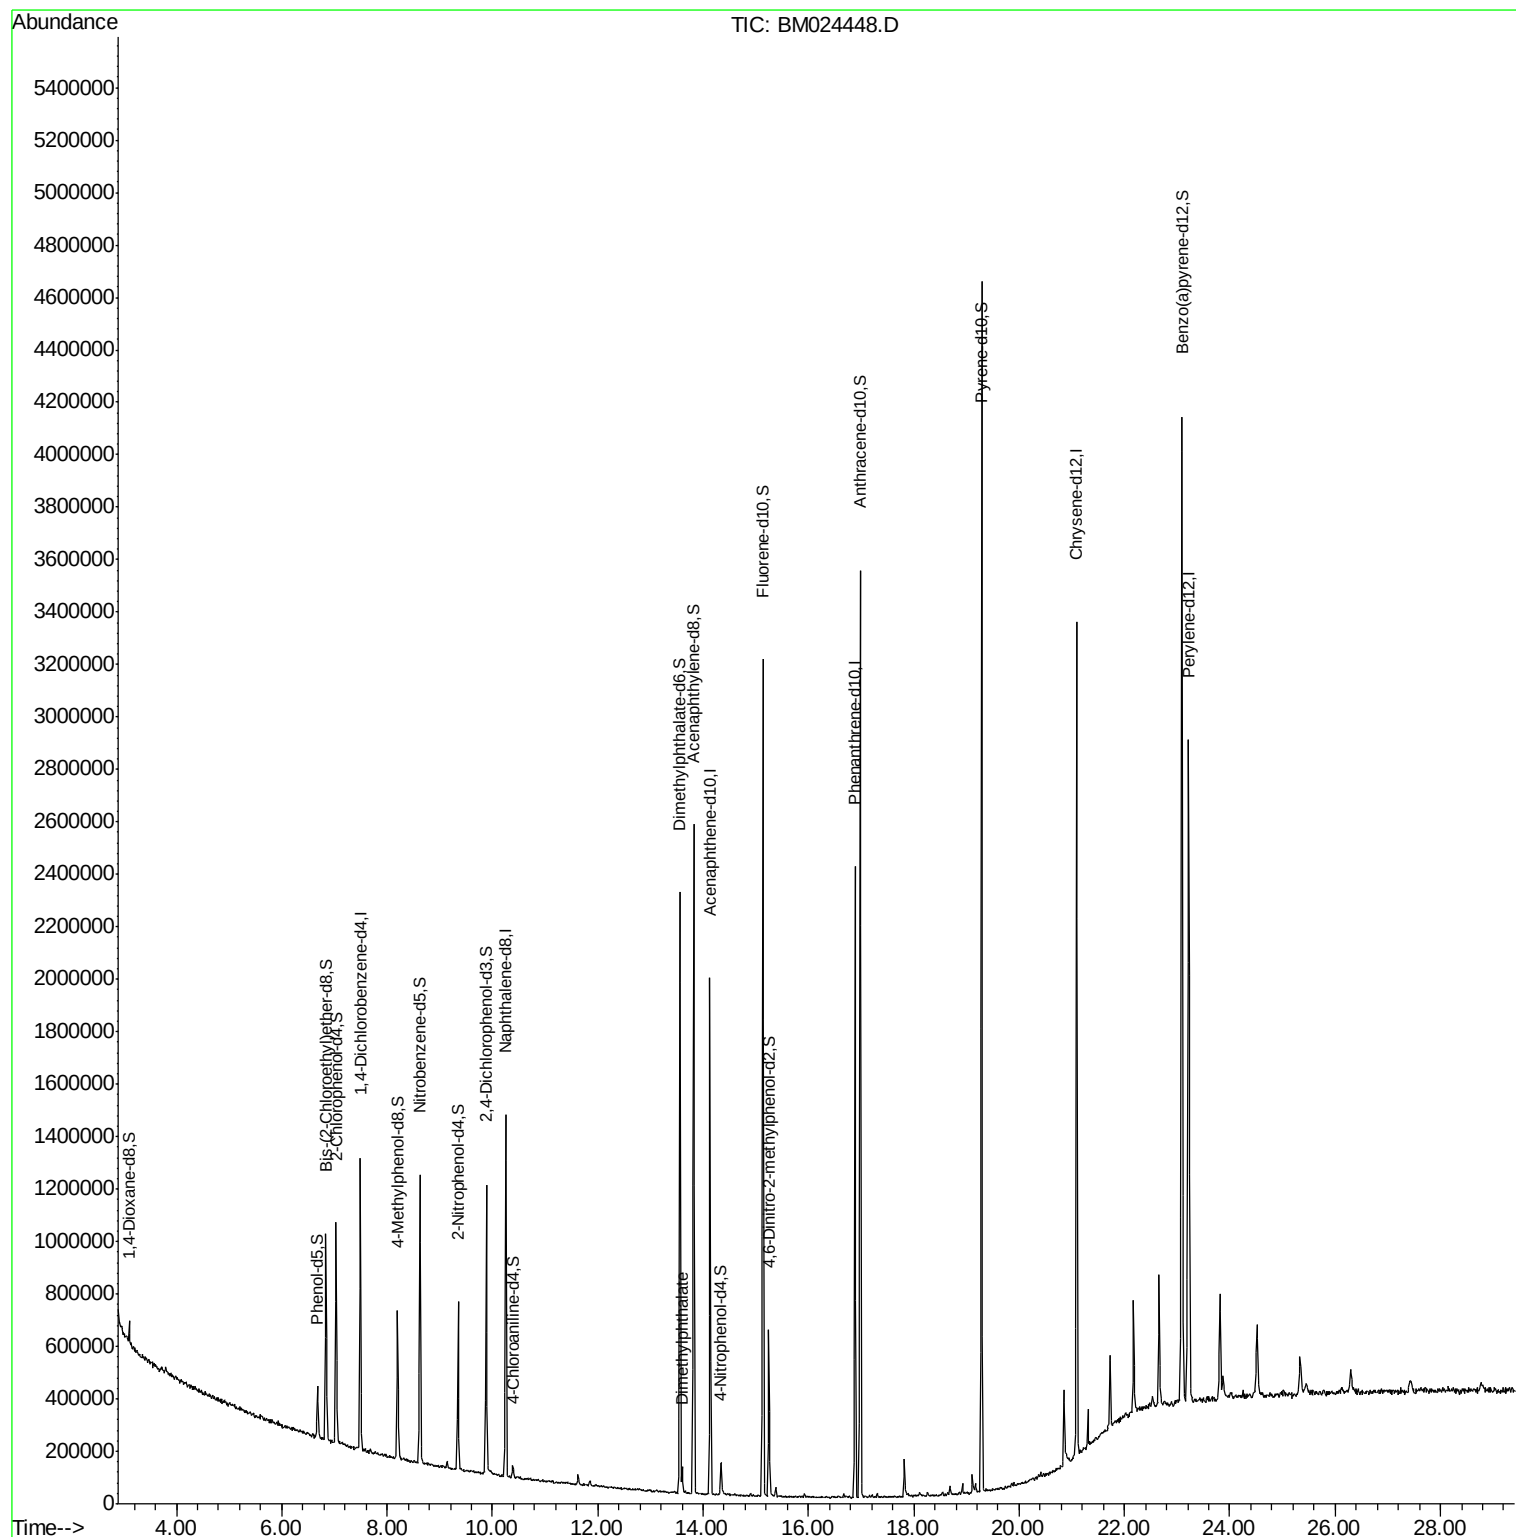

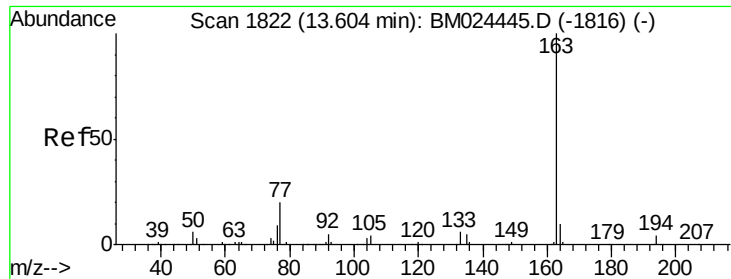

#45

Dimethylphthalate

Concen: 1.131 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. 0.00 min

Lab File: BM024448.D

Acq: 10 Jan 2020 05:48

Instrument :

BNA_M

ClientSampleId :

H0BP8


Tot Ion:163 Resp: 51788

Ion Ratio Lower Upper

163 100

194 3.3 3.2 4.8

164 9.6 8.2 12.4

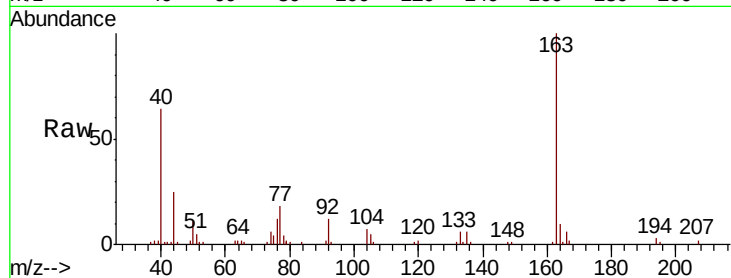

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

