

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024449.D
 Acq On : 10 Jan 2020 06:24
 Operator : JU
 Sample : K6466-11
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BP9

Quant Time: Jan 10 07:55:24 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 07:52:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	264729	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	996642	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	596609	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1289384	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1334274	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1617286	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.10	96	36530	5.95	ng/uL	0.00
5) Phenol-d5	6.68	99	103874	5.03	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	296553	24.46	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	334311	19.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	188294	11.34	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	207428	27.75	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	158274	22.09	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	341897	21.75	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	50949	2.87	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1285249	29.99	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1486152	26.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.35	143	33404	4.42	ng/ul	0.00
58) Fluorene-d10	15.13	176	1099551	28.95	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	128878	22.31	ng/ul	0.00
71) Anthracene-d10	16.98	188	1892246	31.33	ng/ul	0.00
79) Pyrene-d10	19.29	212	2291260	32.14	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2674039	32.38	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.60	163	69260	1.575	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024449.D
Acq On : 10 Jan 2020 06:24
Operator : JU
Sample : K6466-11
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BP9

Quant Time: Jan 10 07:55:24 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 07:52:51 2020
Response via : Initial Calibration

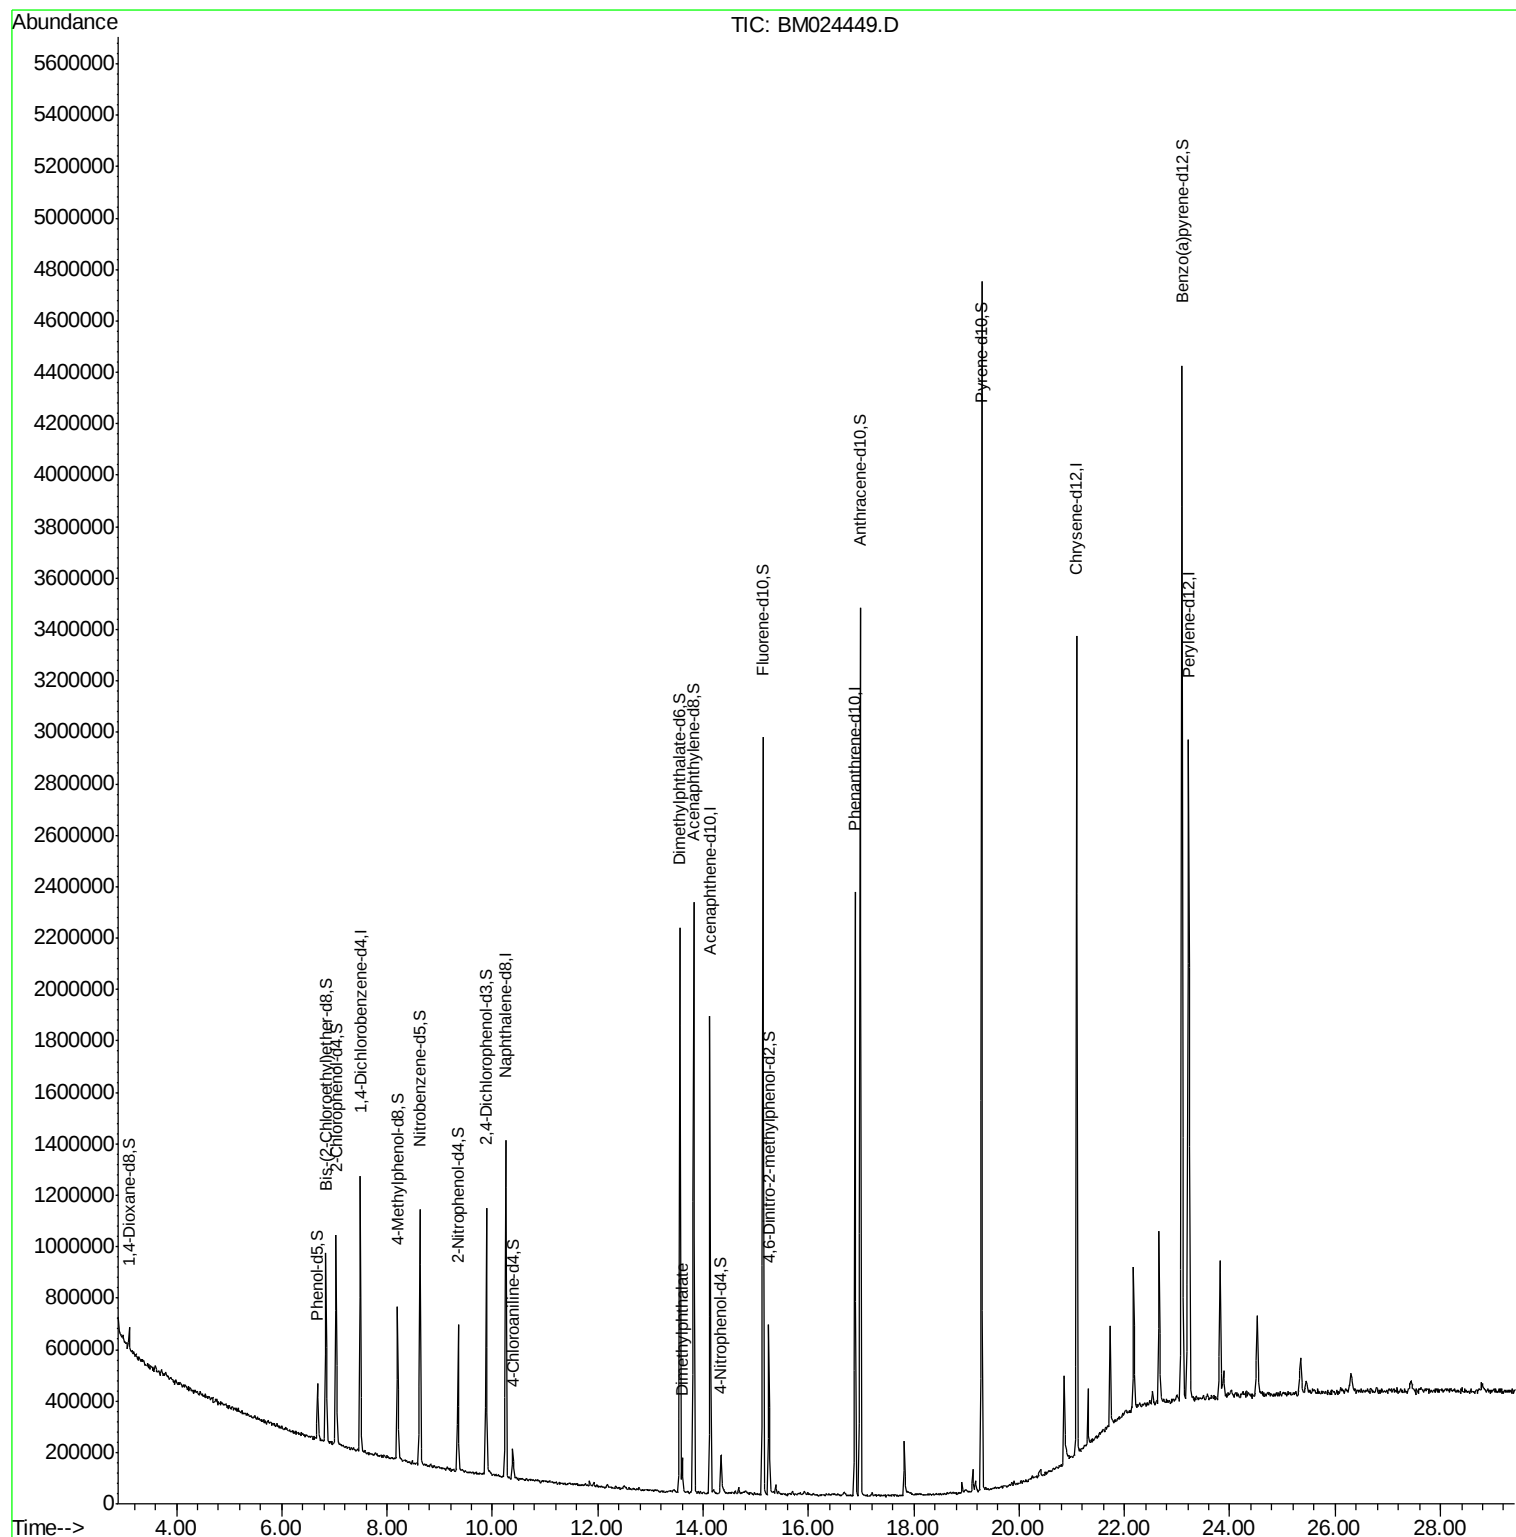

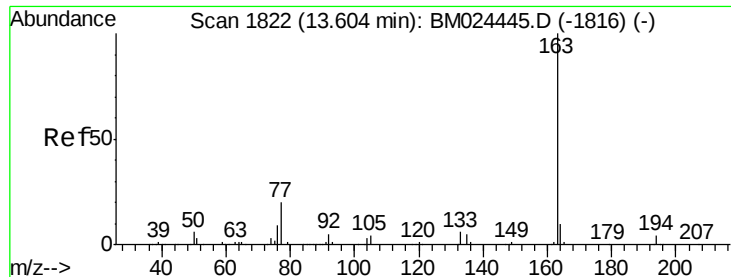

#45

Dimethylphthalate

Concen: 1.575 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. -0.00 min

Lab File: BM024449.D

Acq: 10 Jan 2020 06:24

Instrument :

BNA_M

ClientSampleId :

H0BP9


Tot Ion:163 Resp: 69260

Ion Ratio Lower Upper

163 100

194 3.3 3.2 4.8

164 10.3 8.2 12.4

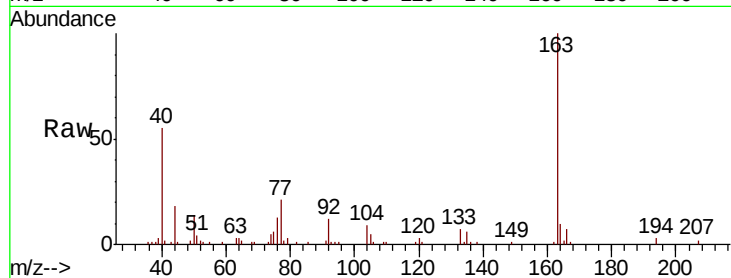

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

