

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024453.D
 Acq On : 10 Jan 2020 10:13
 Operator : JU
 Sample : L1022-01
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BP6

Quant Time: Jan 10 11:45:15 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 07:52:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	243059	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	883086	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	529186	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.89	188	1169691	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1174833	20.00	ng/ul	0.00
86) Perylene-d12	23.23	264	1410012	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.10	96	30199	5.36	ng/uL	0.00
5) Phenol-d5	6.68	99	92832	4.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	255025	22.91	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	282865	17.63	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	162591	10.66	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	172647	26.07	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	125466	19.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	295452	21.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	35554	2.26	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1132131	29.78	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1315463	26.80	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	28381	4.23	ng/ul	0.00
58) Fluorene-d10	15.13	176	1003666	29.79	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	110142	21.02	ng/ul	0.00
71) Anthracene-d10	16.98	188	1738477	31.73	ng/ul	0.00
79) Pyrene-d10	19.29	212	2043524	32.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2283048	31.71	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.60	163	82561	2.117	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024453.D
Acq On : 10 Jan 2020 10:13
Operator : JU
Sample : L1022-01
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BP6

Quant Time: Jan 10 11:45:15 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 07:52:51 2020
Response via : Initial Calibration

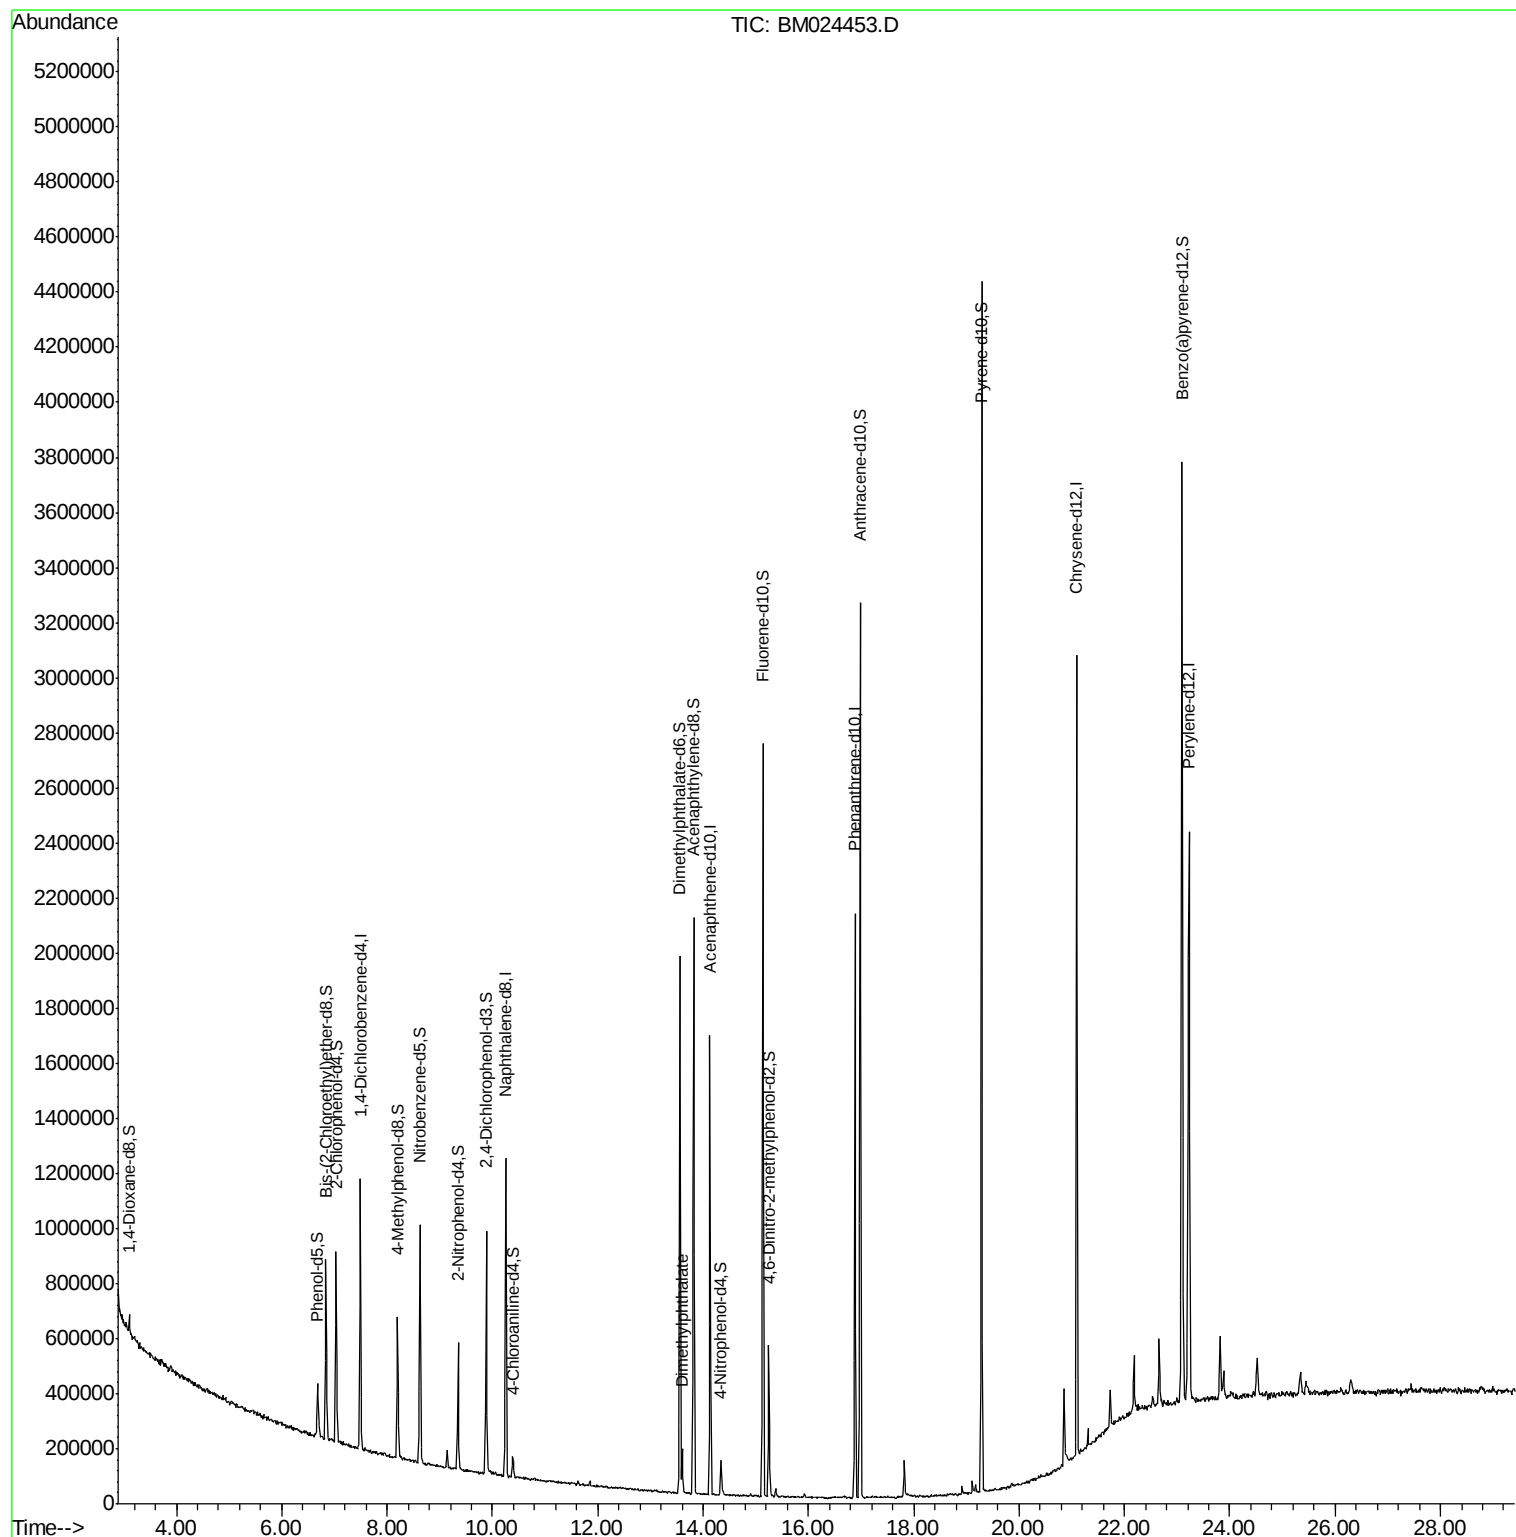


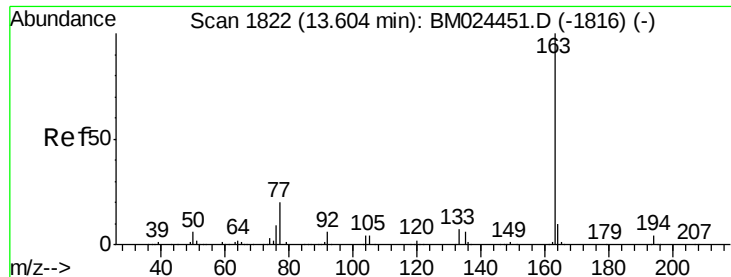

#45
 Dimethylphthalate
 Concen: 2.117 ng/ul
 RT: 13.60 min Scan# 1822
 Delta R.T. -0.00 min
 Lab File: BM024453.D
 Acq: 10 Jan 2020 10:13

Instrument :
 BNA_M
 ClientSampleId :
 H0BP6

Tot Ion	Ratio	Lower	Upper
163	100		
194	3.4	3.2	4.8
164	9.9	8.2	12.4

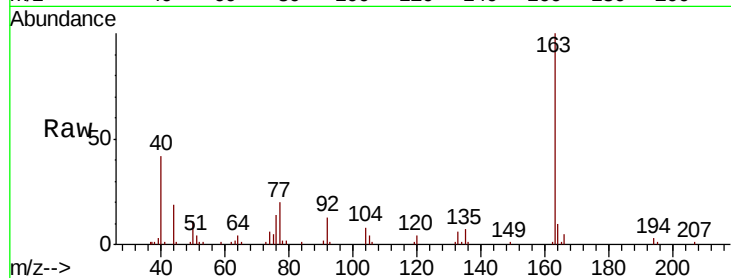

Abundance

Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

