

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
 Data File : BM024455.D
 Acq On : 10 Jan 2020 11:25
 Operator : JU
 Sample : L1022-03
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 H0BR3

Quant Time: Jan 10 12:41:11 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Jan 10 07:52:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.49	152	234122	20.00	ng/ul	0.00
18) Naphthalene-d8	10.25	136	845529	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.13	164	505142	20.00	ng/ul	0.00
62) Phenanthrene-d10	16.88	188	1083562	20.00	ng/ul	0.00
78) Chrysene-d12	21.09	240	1143277	20.00	ng/ul	0.00
86) Perylene-d12	23.22	264	1372406	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.10	96	36806	6.78	ng/uL	0.00
5) Phenol-d5	6.68	99	94429	5.17	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.84	67	262447	24.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.03	132	298249	19.30	ng/ul	0.00
13) 4-Methylphenol-d8	8.20	113	165083	11.24	ng/ul	0.00
19) Nitrobenzene-d5	8.63	128	181525	28.63	ng/ul	0.00
22) 2-Nitrophenol-d4	9.35	143	135058	22.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	9.88	165	291354	21.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.39	131	24546	1.63	ng/ul	0.00
44) Dimethylphthalate-d6	13.56	166	1097752	30.25	ng/ul	0.00
47) Acenaphthylene-d8	13.82	160	1308685	27.94	ng/ul	0.00
52) 4-Nitrophenol-d4	14.34	143	27008	4.22	ng/ul	0.00
58) Fluorene-d10	15.13	176	1001864	31.15	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.25	200	106540	21.94	ng/ul	0.00
71) Anthracene-d10	16.98	188	1699700	33.49	ng/ul	0.00
79) Pyrene-d10	19.29	212	2035207	33.32	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.09	264	2394317	34.17	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.60	163	56639	1.521	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM010920\
Data File : BM024455.D
Acq On : 10 Jan 2020 11:25
Operator : JU
Sample : L1022-03
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
H0BR3

Quant Time: Jan 10 12:41:11 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM010820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Jan 10 07:52:51 2020
Response via : Initial Calibration

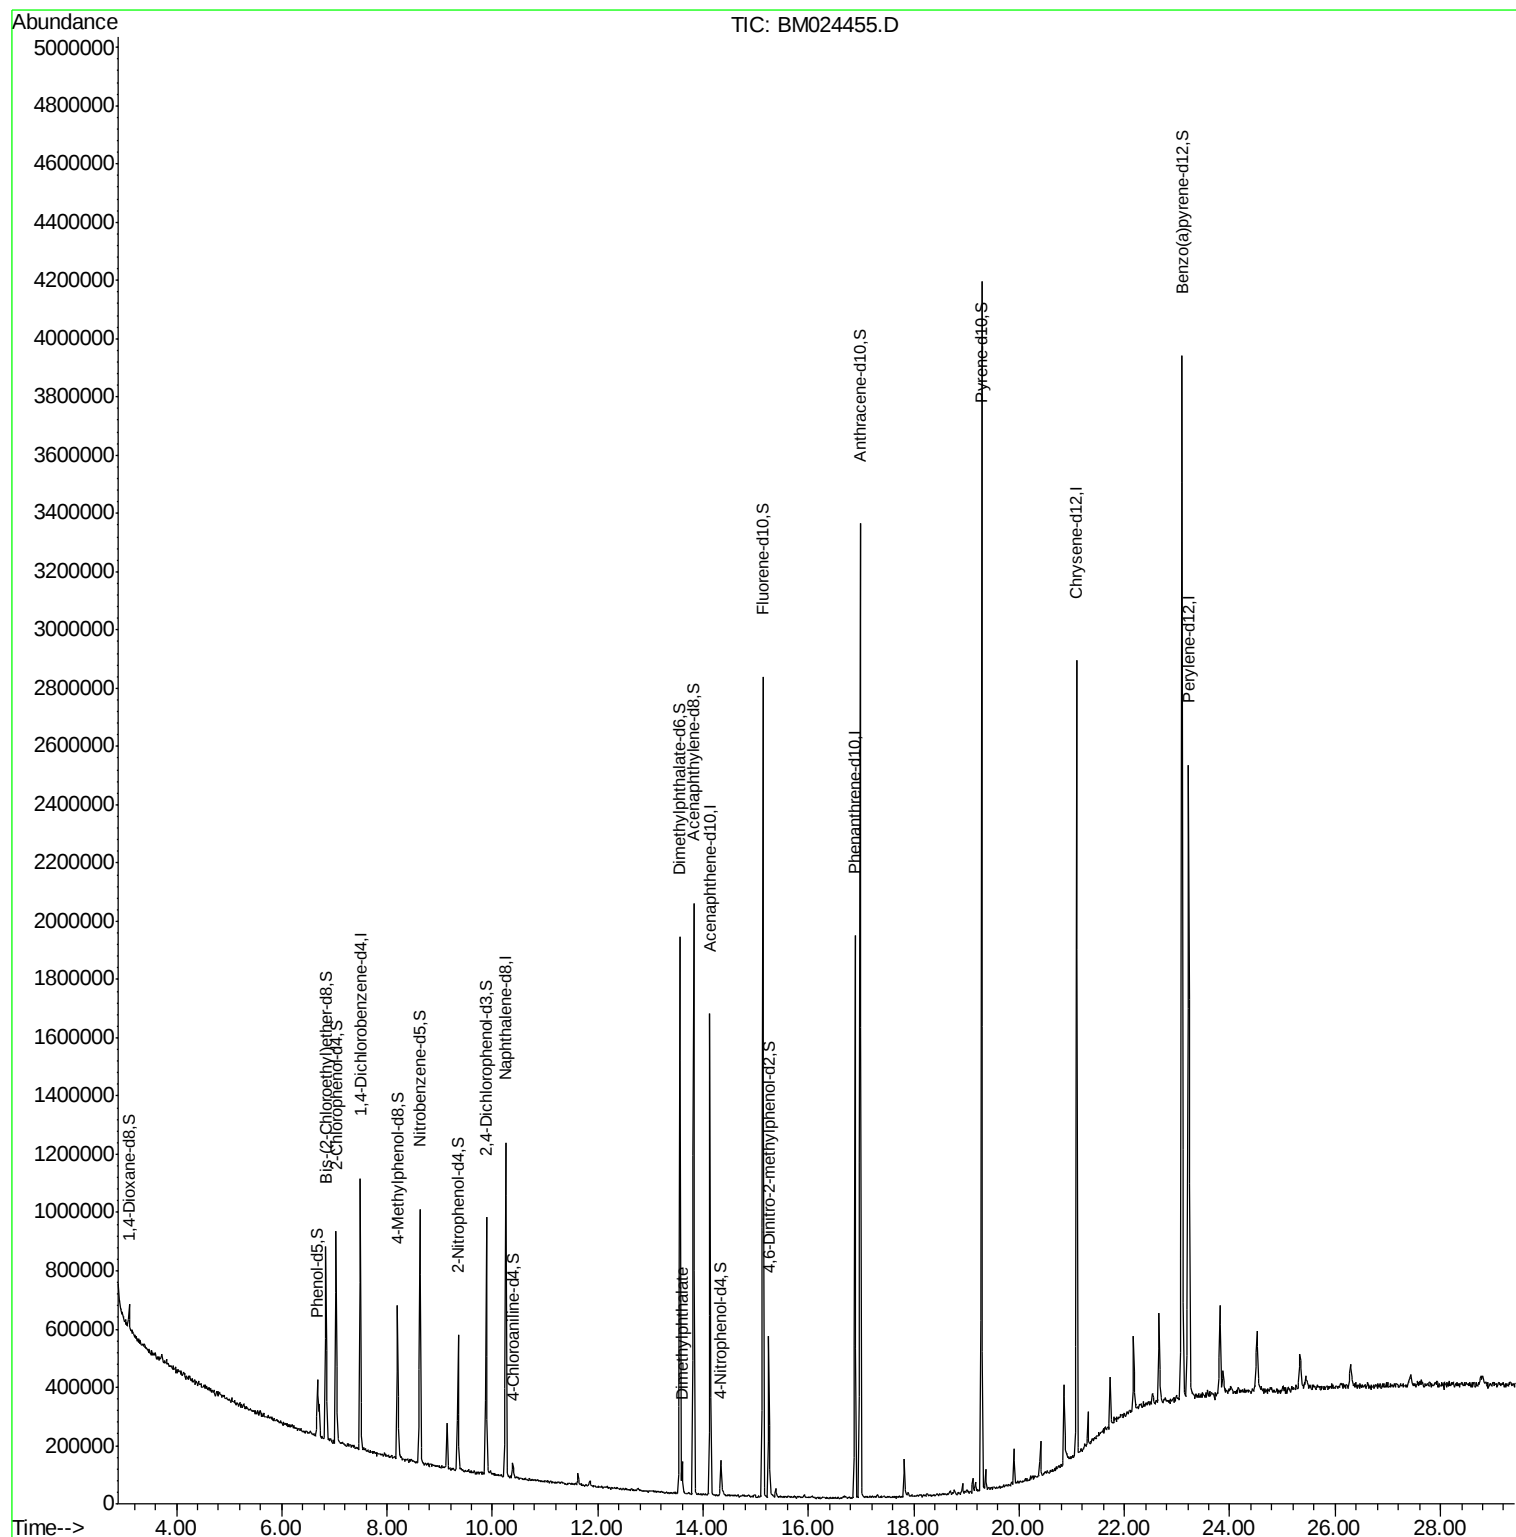

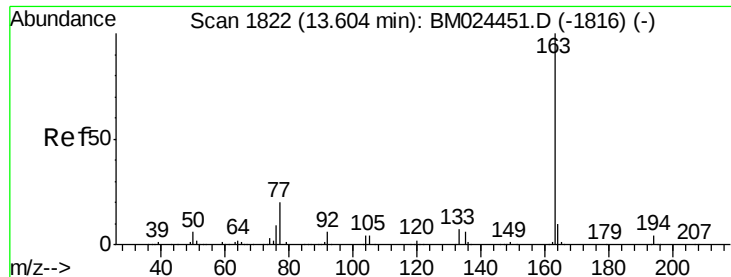

#45

Dimethylphthalate

Concen: 1.521 ng/ul

RT: 13.60 min Scan# 1822

Delta R.T. 0.00 min

Lab File: BM024455.D

Acq: 10 Jan 2020 11:25

Instrument :

BNA_M

ClientSampleId :

H0BR3


Tot Ion:163 Resp: 56639

Ion Ratio Lower Upper

163 100

194 3.8 3.2 4.8

164 9.5 8.2 12.4

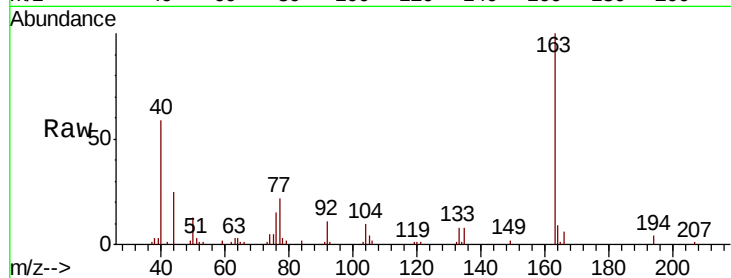

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

