
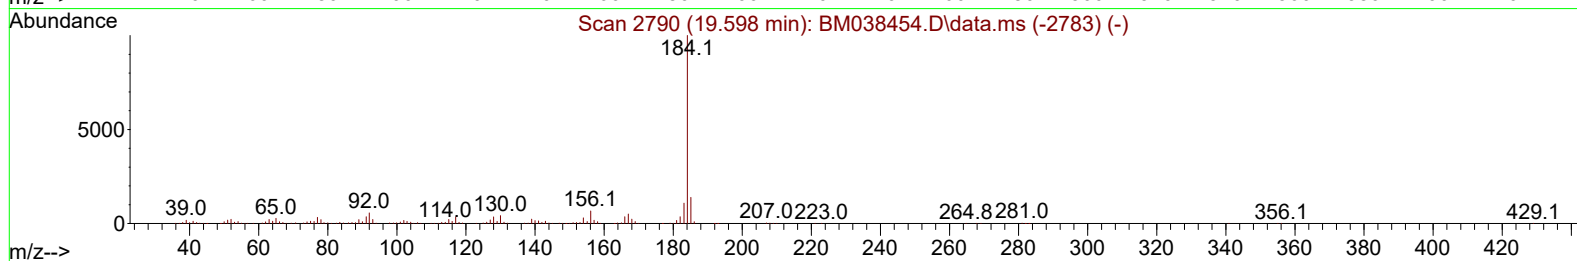
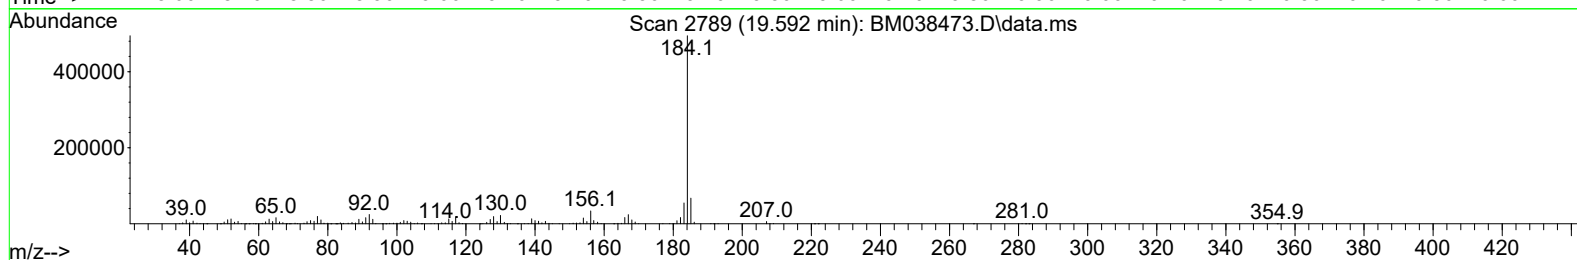


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011823\
Data File : BM038473.D
Acq On : 18 Jan 2023 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 07:28:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 06:09:42 2023
Response via : Initial Calibration

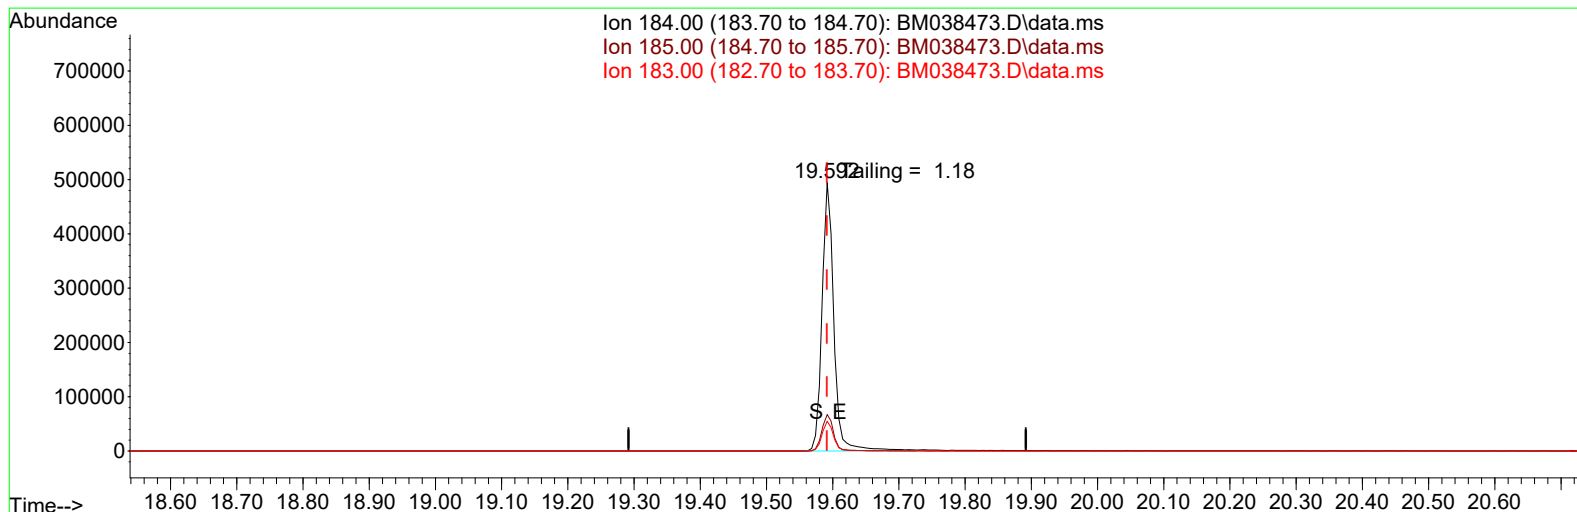

TIC: BM038473.D\data.ms

(77) Benzidine




19.592min (+ 0.000) 0.00 ng

response 613918

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.63
183.00	10.80	11.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011823\
 Data File : BM038473.D
 Acq On : 18 Jan 2023 09:57
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 19 07:28:50 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jan 19 06:09:42 2023
 Response via : Initial Calibration

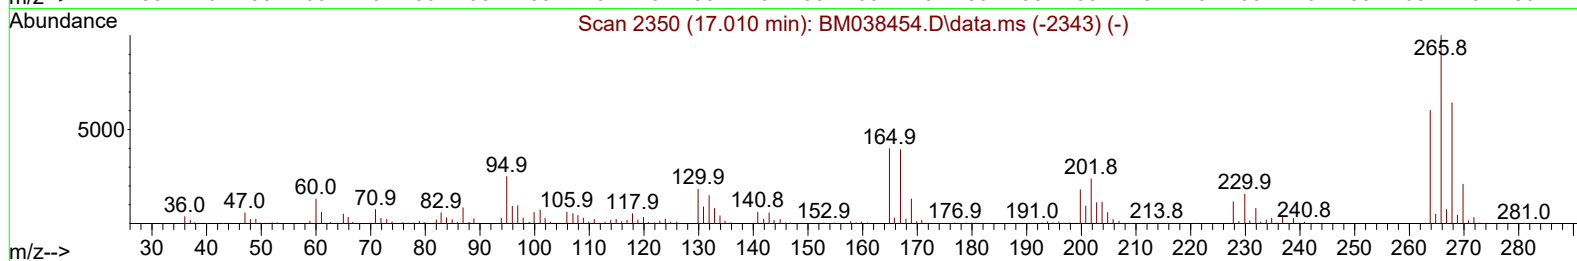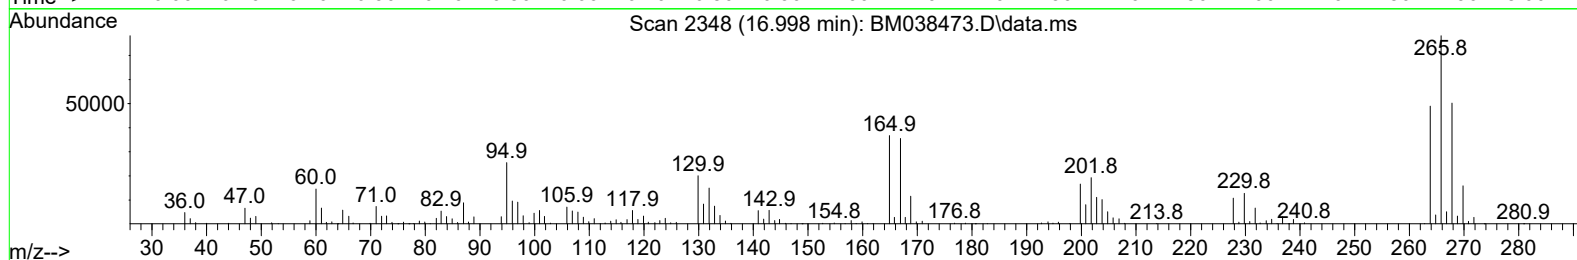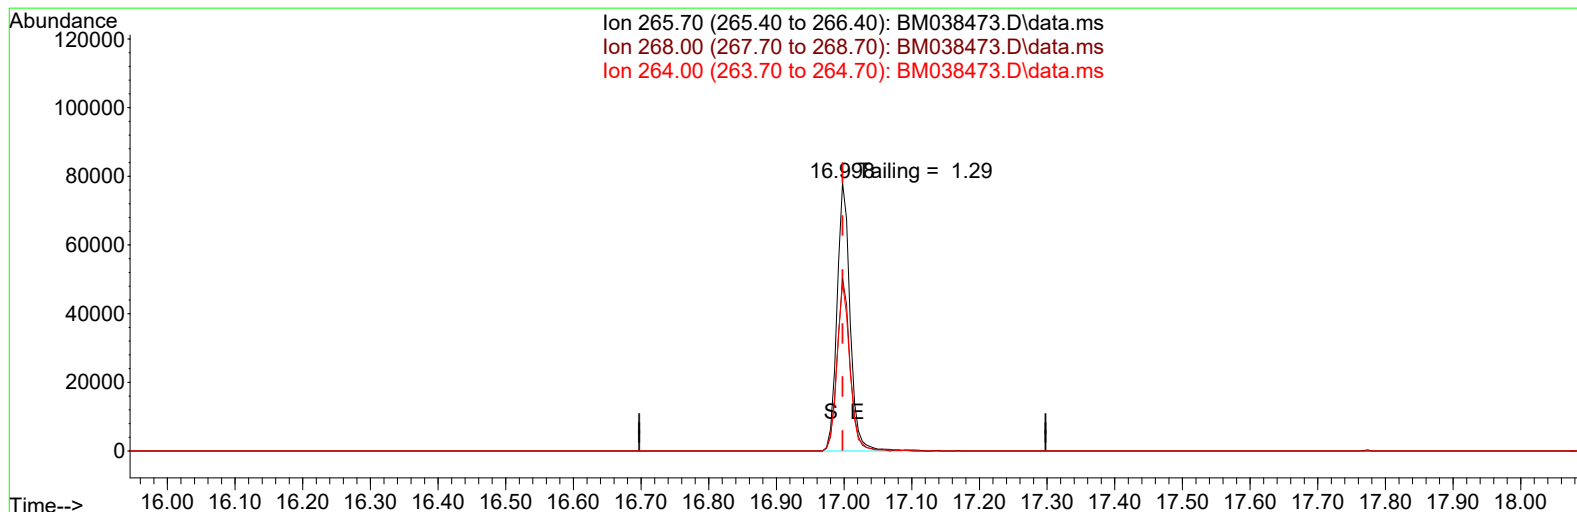

TIC: BM038473.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 0.00 ng

response 104915

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.26
264.00	60.20	62.60
0.00	0.00	0.00