


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011823\
Data File : BM038473.D
Acq On : 18 Jan 2023 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 06:09:42 2023

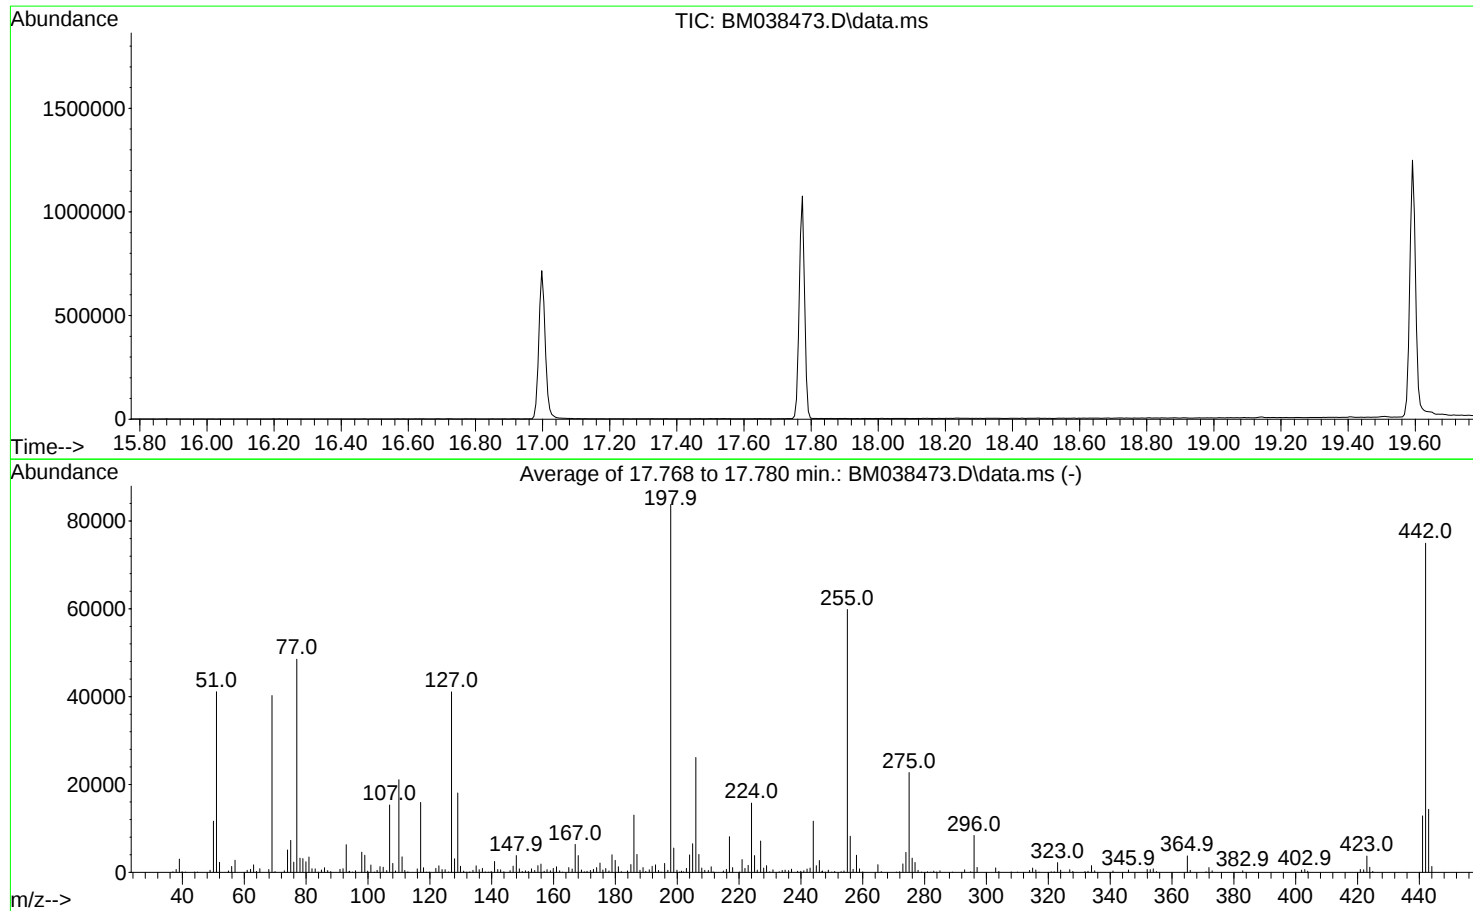




AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2473

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.1	41115	PASS
68	69	0.00	2	1.6	656	PASS
69	198	0.00	100	48.0	40235	PASS
70	69	0.00	2	0.4	163	PASS
127	198	10	80	49.1	41093	PASS
197	198	0.00	2	0.5	458	PASS
198	198	100	100	100.0	83771	PASS
199	198	5	9	6.6	5522	PASS
275	198	10	60	27.1	22731	PASS
365	198	1	100	4.5	3730	PASS
441	198	0.01	100	15.3	12854	PASS
442	442	50	100	100.0	74941	PASS
443	442	15	24	19.1	14329	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011823\
Data File : BM038473.D
Acq On : 18 Jan 2023 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 19 07:28:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 06:09:42 2023
Response via : Initial Calibration

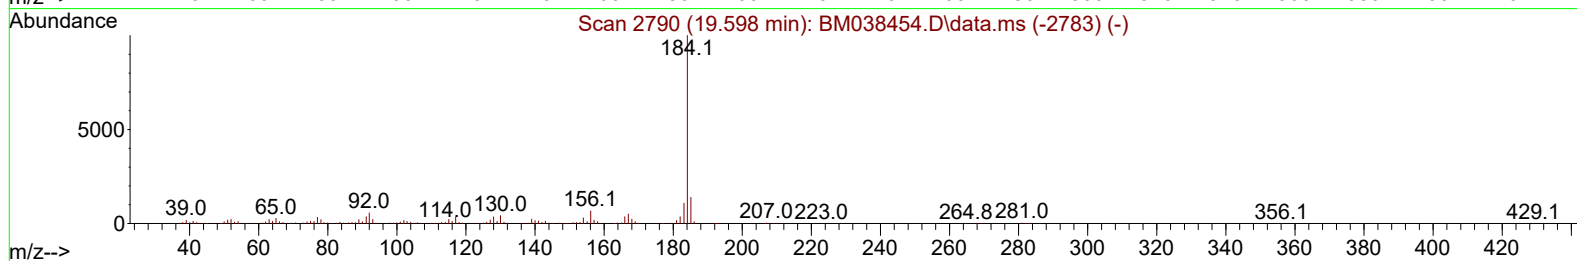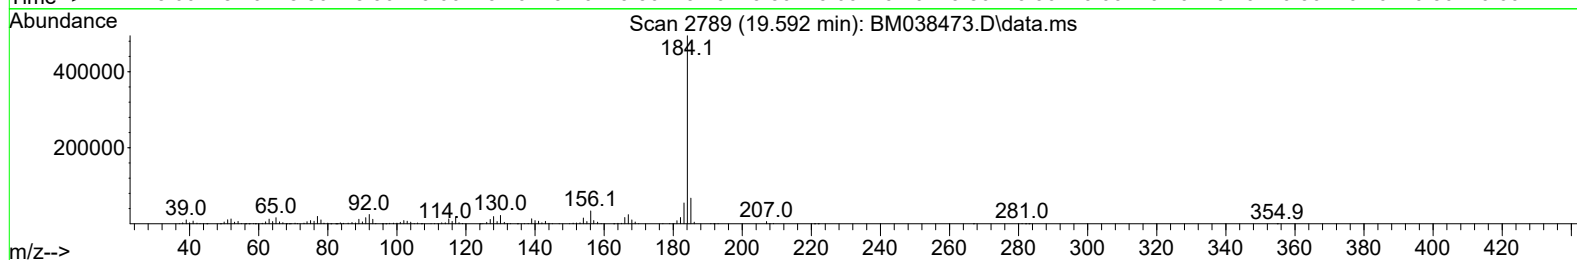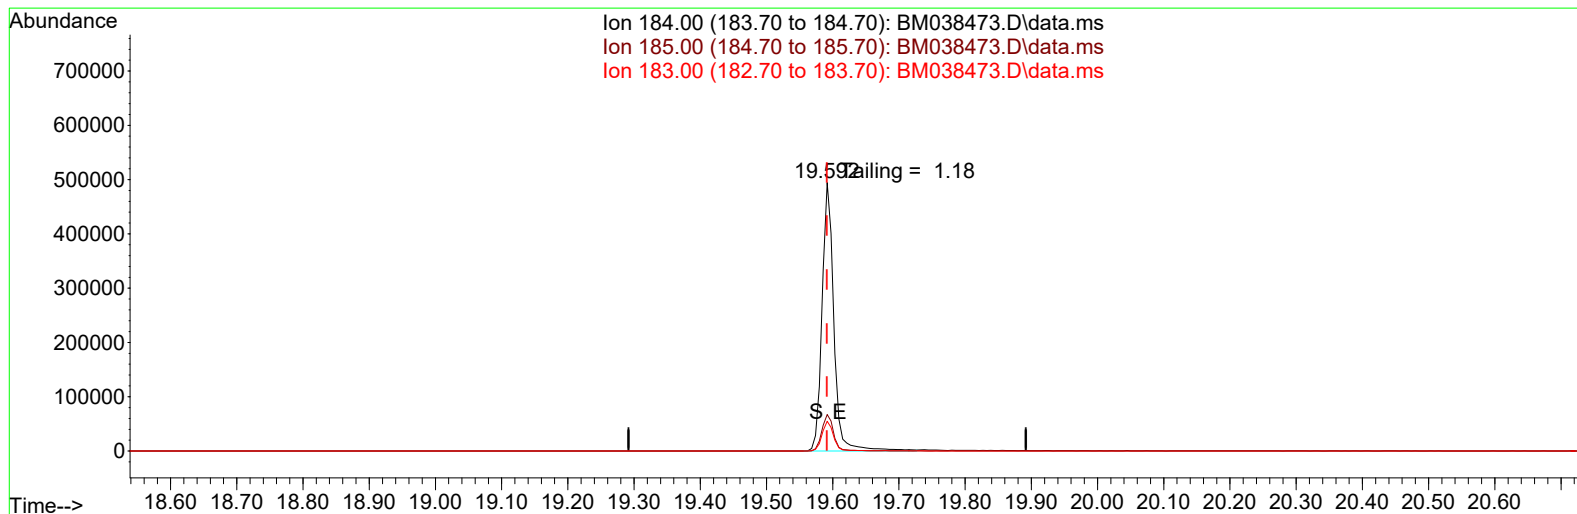

TIC: BM038473.D\data.ms

(77) Benzidine

19.592min (+ 0.000) 0.00 ng




response 613918

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.63
183.00	10.80	11.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011823\
Data File : BM038473.D
Acq On : 18 Jan 2023 09:57
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 19 07:28:50 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 06:09:42 2023
Response via : Initial Calibration

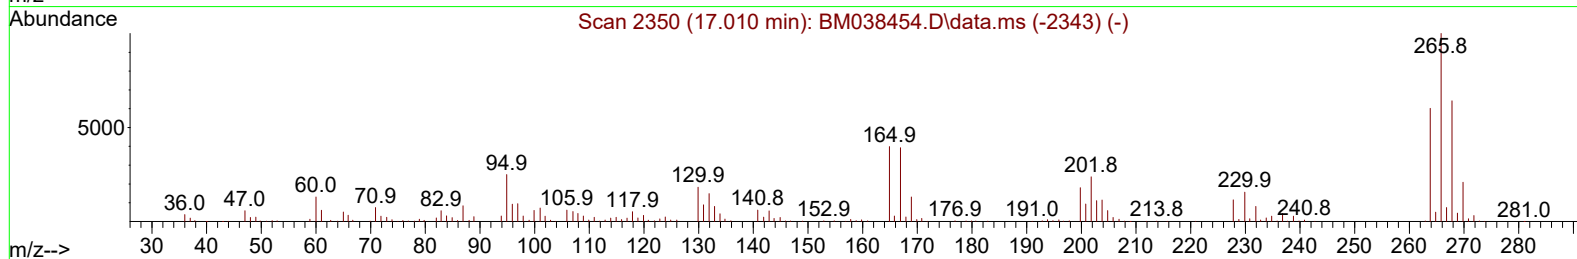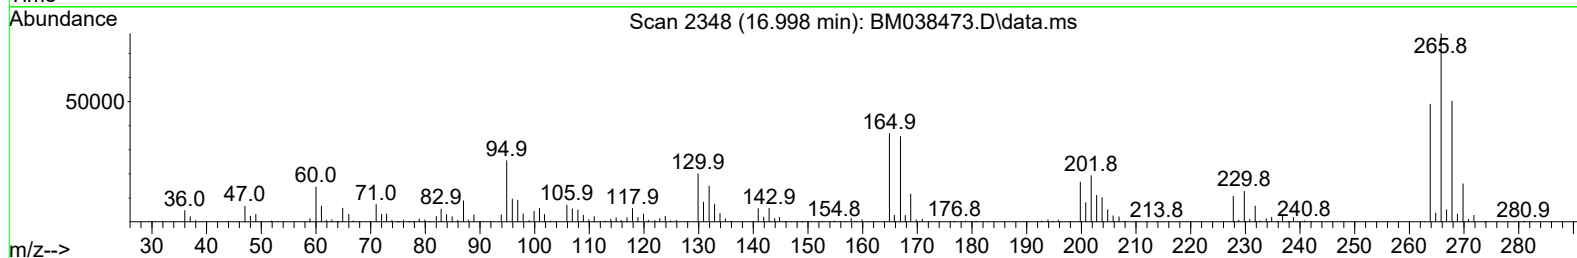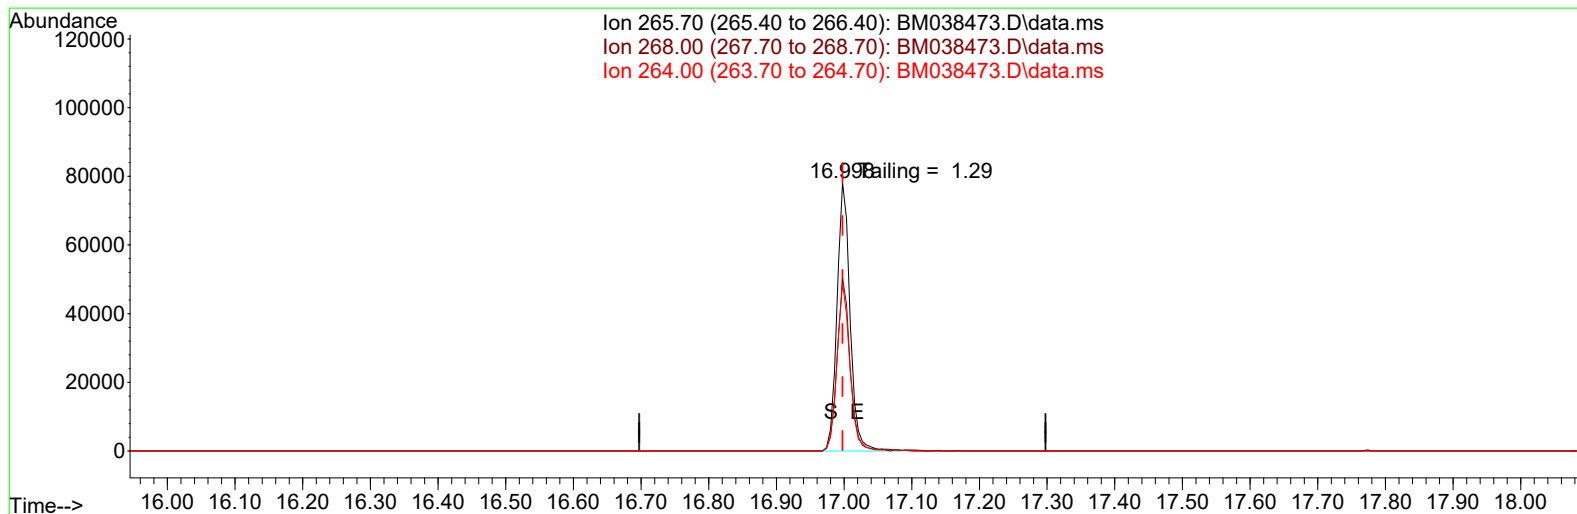

TIC: BM038473.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 0.00 ng

response 104915

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.26
264.00	60.20	62.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/18/2023	BNA_M	<u>BM038473.D</u>
Compound Name	Response	Retention Time
DDT	357930	20.815
DDD	2993	20.421
DDE	0	19.9
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2993	360923	0.83

Instrument :
BNA_M
ClientSampleId :
DFTPP