

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
 Data File : BM038486.D
 Acq On : 19 Jan 2023 12:42
 Operator : CG/JU
 Sample : PB150215BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150215BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038486.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	312	318	327	rBV	604537	825330	39.15%	5.899%
2	5.522	391	397	408	rBV	1474077	2001460	94.93%	14.305%
3	7.134	664	671	692	rBV	1272356	1944668	92.24%	13.900%
4	7.969	807	813	822	rBV	248544	378735	17.96%	2.707%
5	9.145	1006	1013	1026	rBV	693054	1074921	50.98%	7.683%
6	10.781	1284	1291	1300	rBV	256798	424204	20.12%	3.032%
7	13.233	1701	1708	1717	rBV	1421237	1926983	91.40%	13.773%
8	14.604	1935	1941	1950	rVB	328676	465606	22.08%	3.328%
9	16.092	2188	2194	2207	rBV	1133402	1416725	67.20%	10.126%
10	17.345	2401	2407	2416	rBV	360984	475308	22.54%	3.397%
11	19.956	2846	2851	2860	rBV	1970992	2108336	100.00%	15.069%
12	21.515	3112	3116	3125	rBV2	338672	440911	20.91%	3.151%
13	23.933	3521	3527	3535	rBV2	247942	507682	24.08%	3.629%




Sum of corrected areas: 13990869

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038486.D
Acq On : 19 Jan 2023 12:42
Operator : CG/JU
Sample : PB150215BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

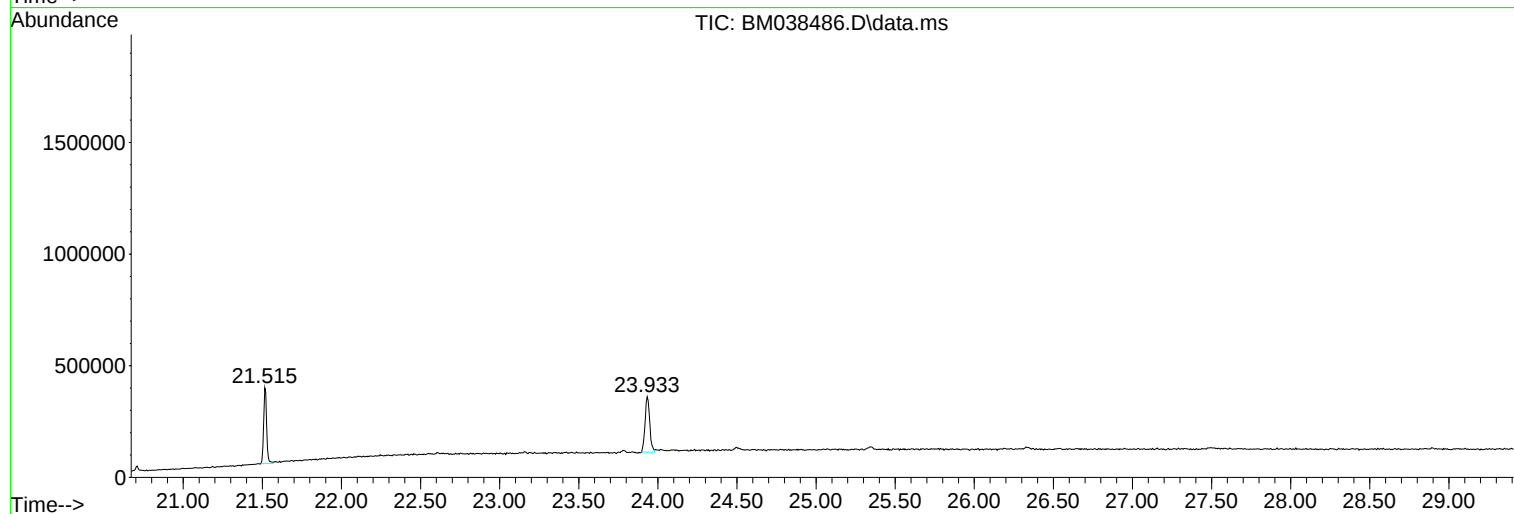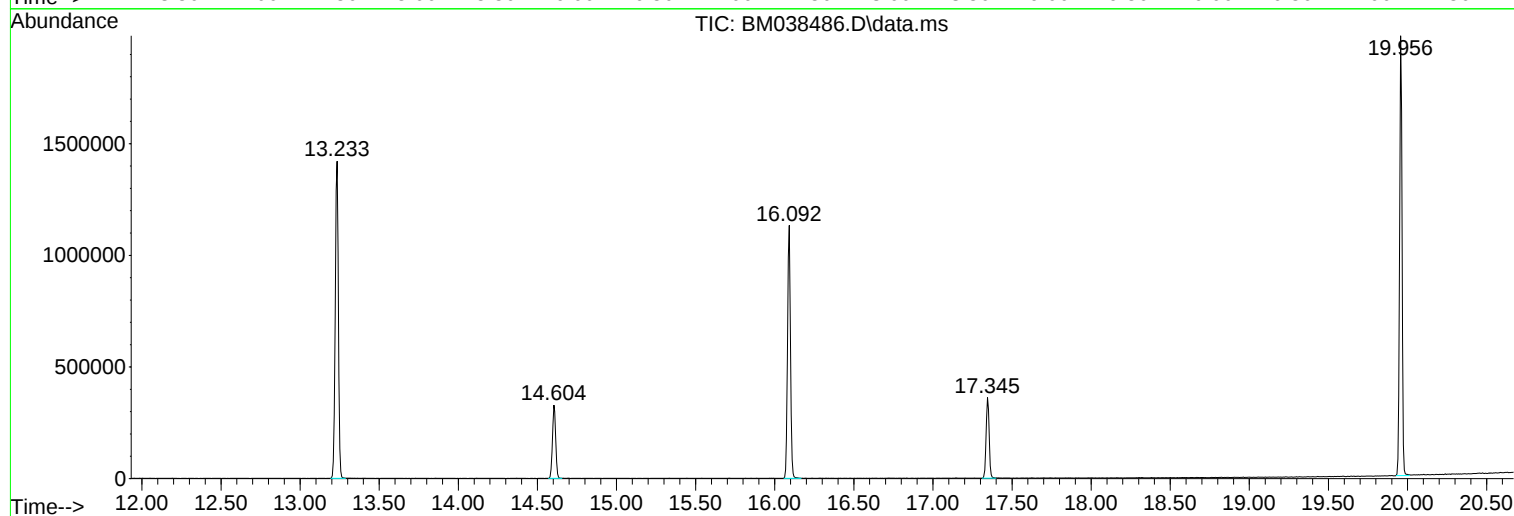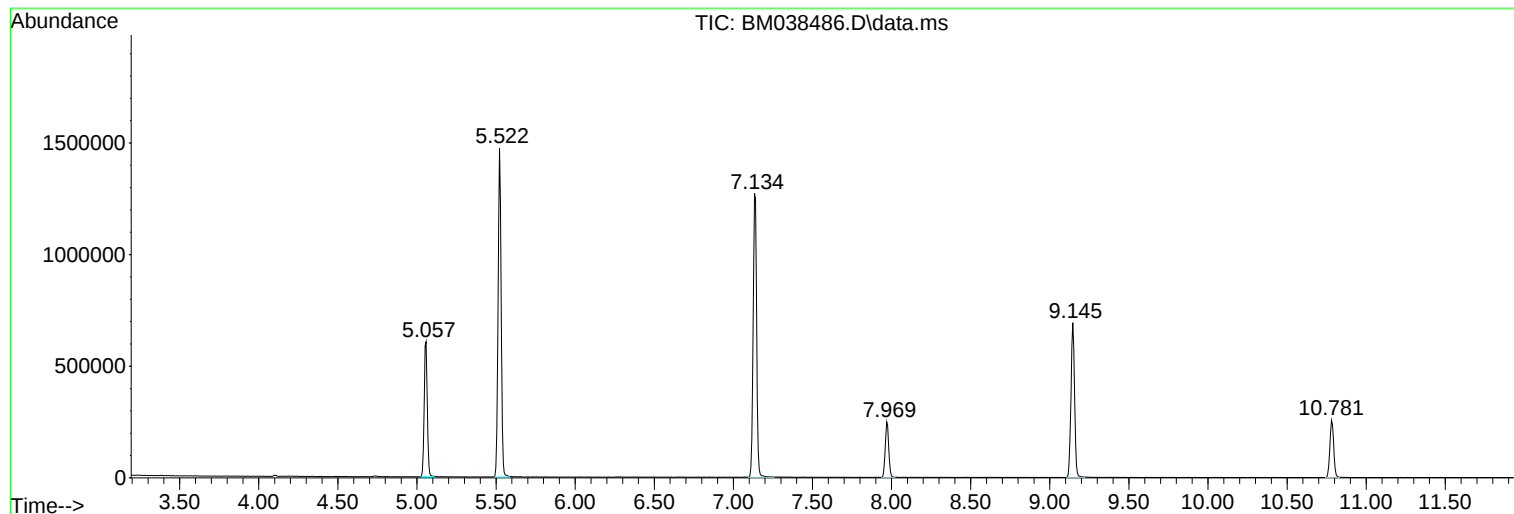

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038486.D
Acq On : 19 Jan 2023 12:42
Operator : CG/JU
Sample : PB150215BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150215BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.057	43.58 ng	825330	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	28		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
5	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		

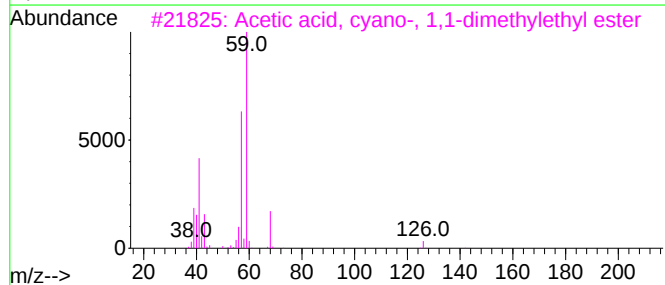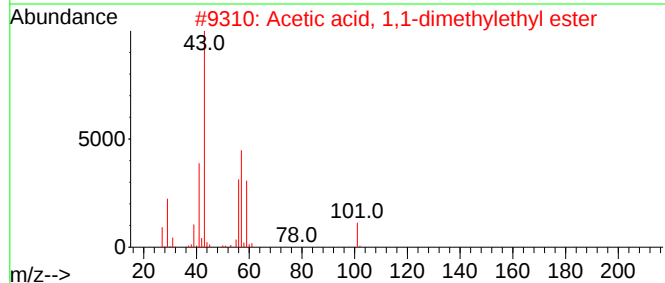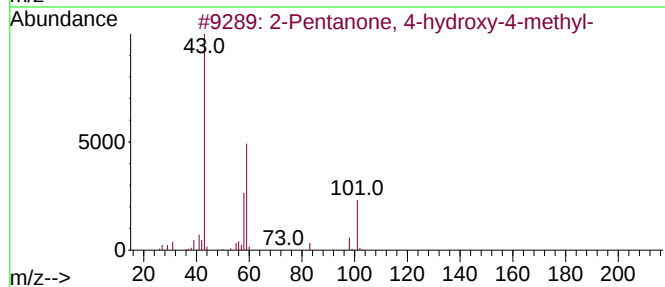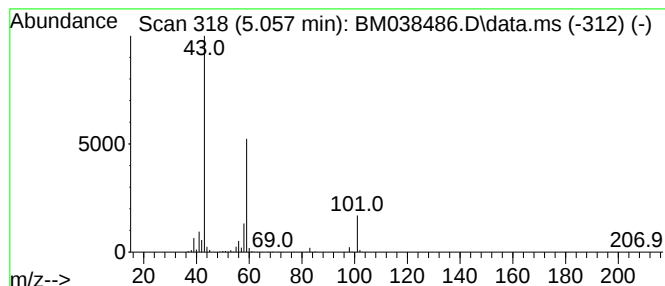

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038486.D
Acq On : 19 Jan 2023 12:42
Operator : CG/JU
Sample : PB150215BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.057	43.6	ng	825330	1	7.969	378735	20.0