

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
 Data File : BM038491.D
 Acq On : 19 Jan 2023 17:13
 Operator : CG/JU
 Sample : PB150215BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150215BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038491.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.058	312	318	330	rBV	693917	911380	38.55%	5.357%
2	5.522	391	397	408	rBV	1705942	2247703	95.09%	13.212%
3	7.140	664	672	689	rBV	1437436	2157802	91.28%	12.684%
4	7.969	805	813	826	rBV	406742	618544	26.17%	3.636%
5	9.145	1006	1013	1029	rBV	764889	1196093	50.60%	7.031%
6	10.781	1284	1291	1304	rBV	423405	687689	29.09%	4.042%
7	13.233	1701	1708	1715	rBV	1596017	2122425	89.79%	12.476%
8	14.604	1935	1941	1951	rBV	560583	749576	31.71%	4.406%
9	16.092	2188	2194	2204	rBV	1246152	1569595	66.40%	9.226%
10	17.345	2401	2407	2419	rBV	577080	764778	32.35%	4.495%
11	19.962	2846	2852	2857	rBV	2051973	2363871	100.00%	13.895%
12	21.521	3112	3117	3122	rBV	613480	736240	31.15%	4.328%
13	23.939	3521	3528	3537	rBV	453126	886387	37.50%	5.210%




Sum of corrected areas: 17012083

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038491.D
Acq On : 19 Jan 2023 17:13
Operator : CG/JU
Sample : PB150215BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

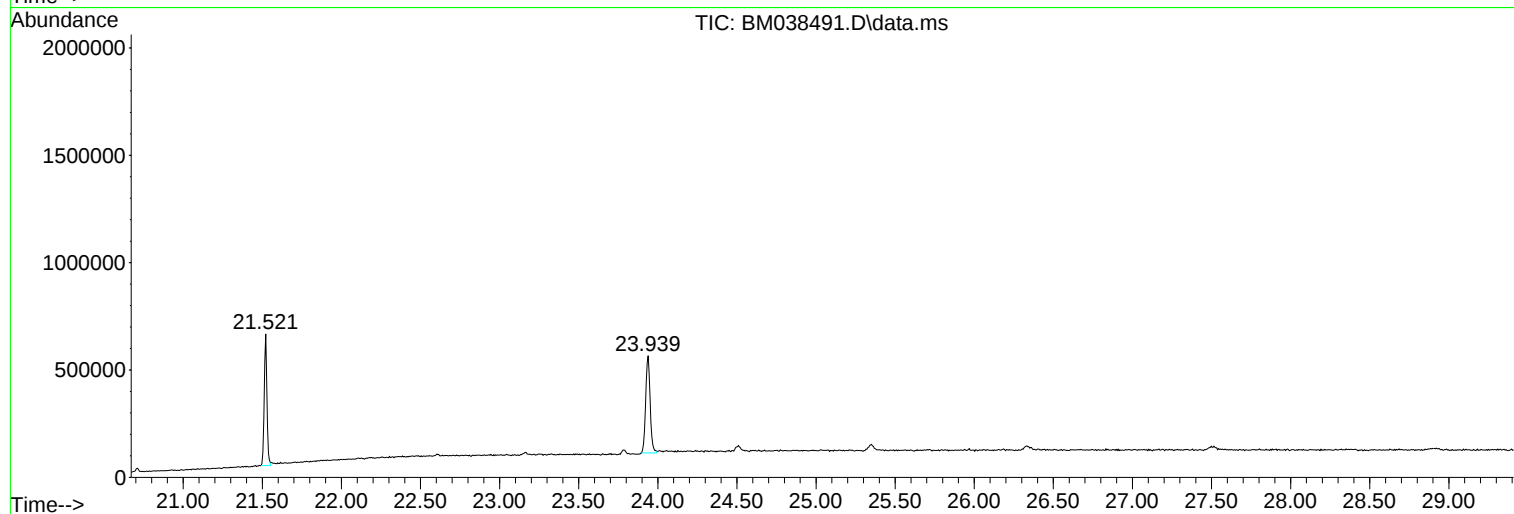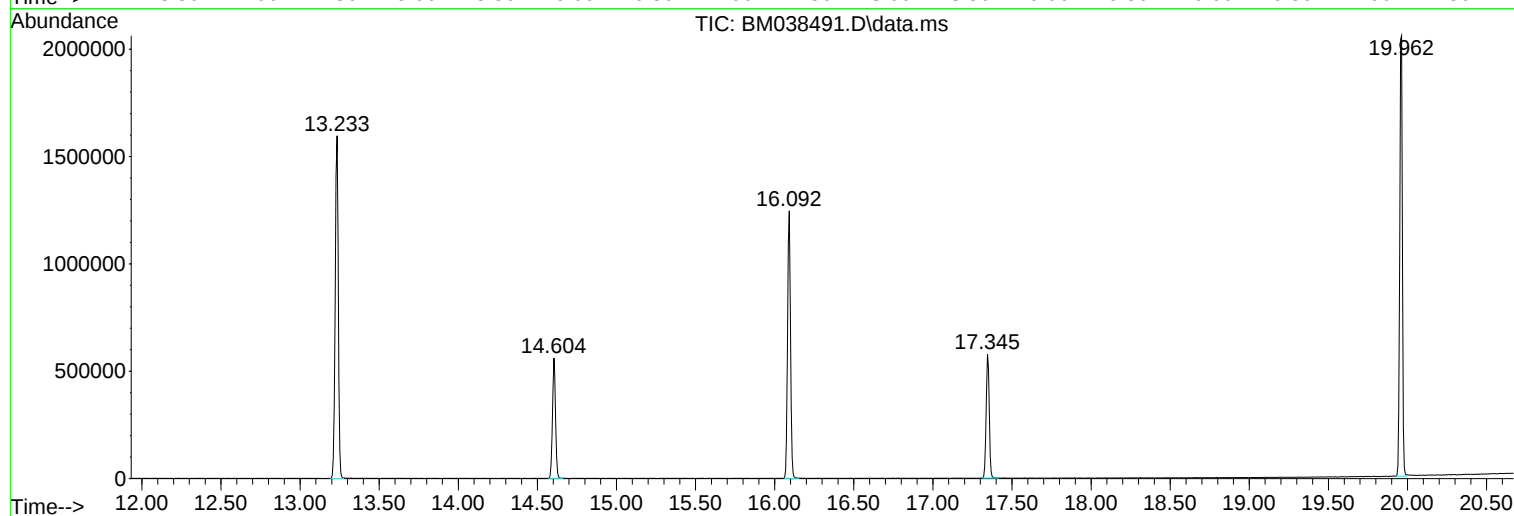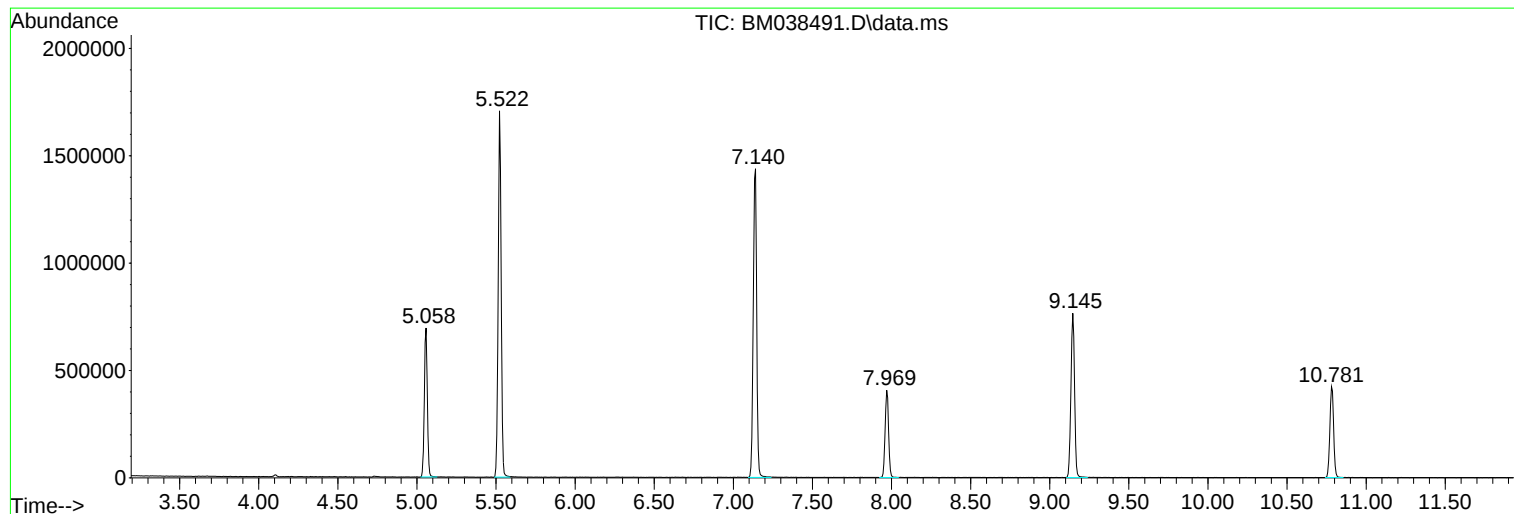

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038491.D
Acq On : 19 Jan 2023 17:13
Operator : CG/JU
Sample : PB150215BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150215BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.058	29.47 ng	911380	1,4-Dichlorobenzene-d4	7.969

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	38		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27		
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		

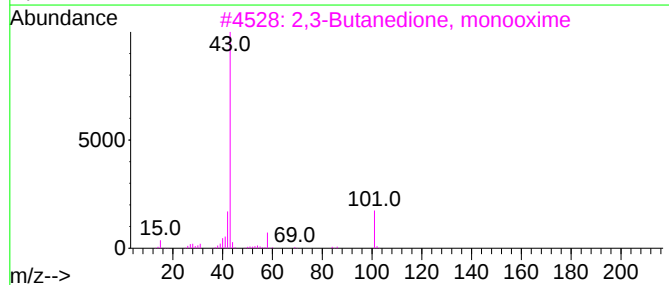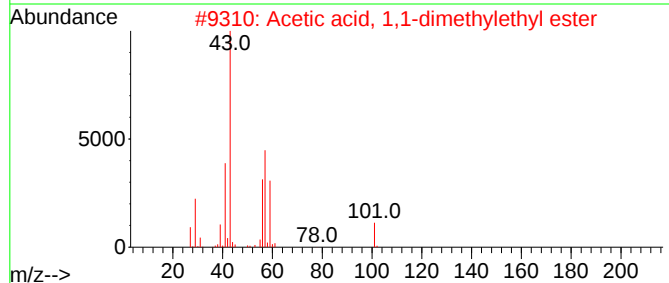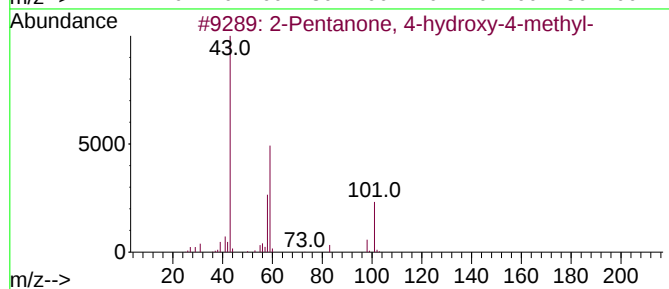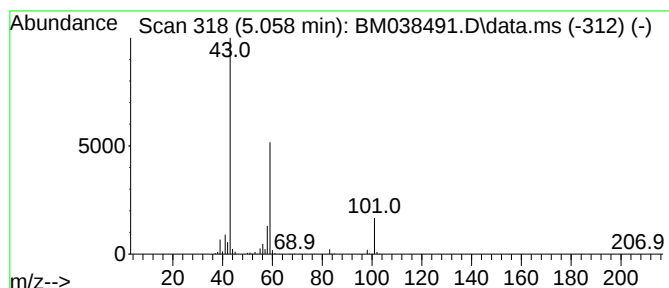

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038491.D
Acq On : 19 Jan 2023 17:13
Operator : CG/JU
Sample : PB150215BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150215BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.058	29.5	ng	911380	1	7.969	618544	20.0