


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038484.D
Acq On : 19 Jan 2023 08:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jan 19 06:09:42 2023

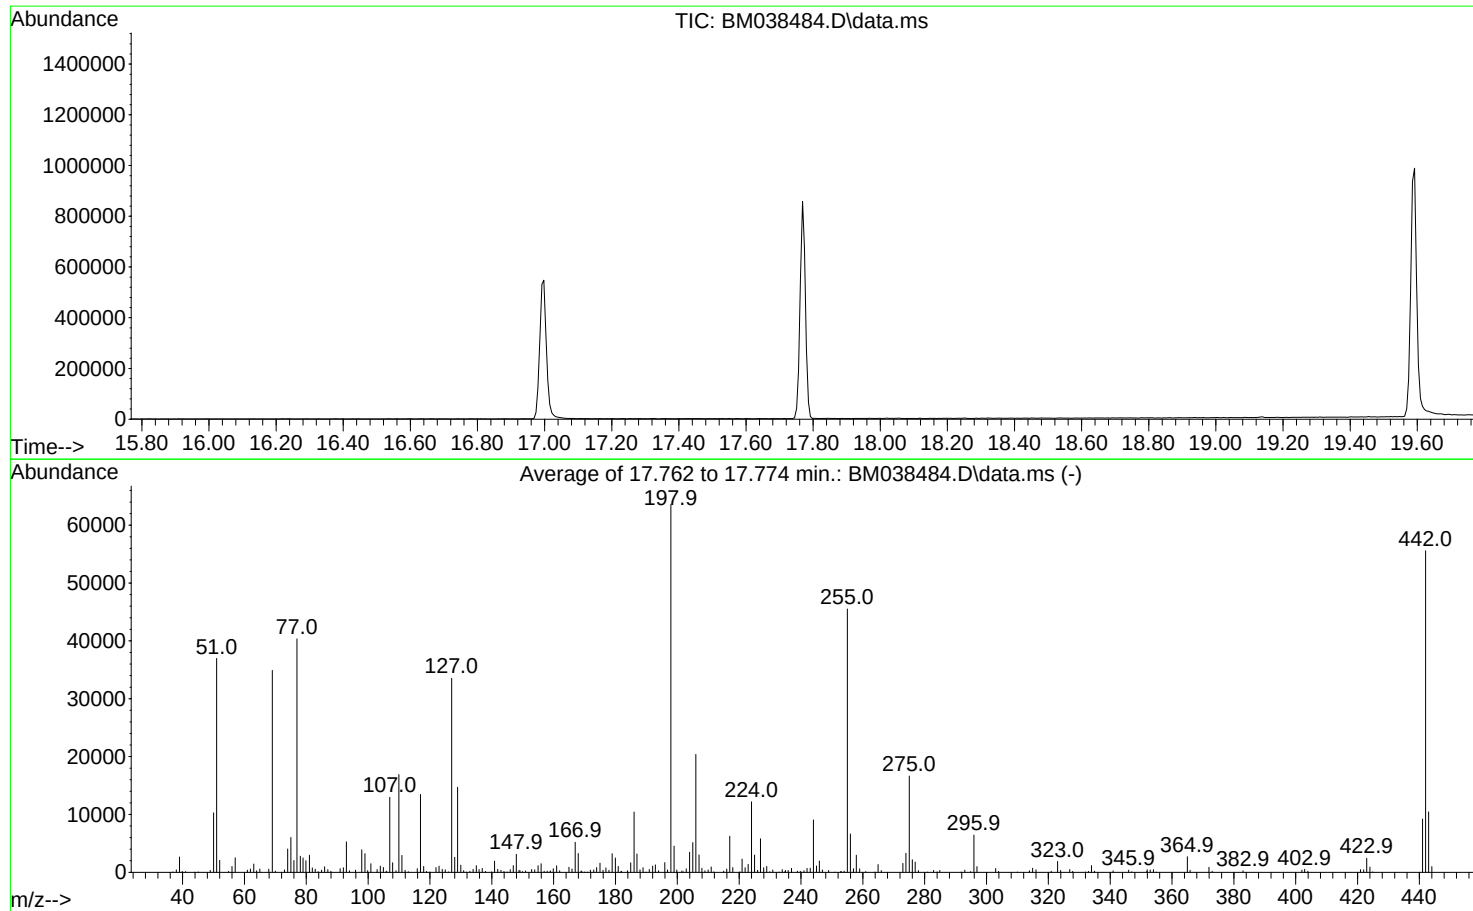




AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.1	36965	PASS
68	69	0.00	2	1.6	543	PASS
69	198	0.00	100	54.9	34896	PASS
70	69	0.00	2	0.6	218	PASS
127	198	10	80	52.8	33547	PASS
197	198	0.00	2	0.6	412	PASS
198	198	100	100	100.0	63589	PASS
199	198	5	9	7.1	4532	PASS
275	198	10	60	26.1	16626	PASS
365	198	1	100	4.2	2687	PASS
441	198	0.01	100	14.5	9191	PASS
442	442	50	100	100.0	55568	PASS
443	442	15	24	18.8	10436	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038484.D
Acq On : 19 Jan 2023 08:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 20 05:15:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 06:09:42 2023
Response via : Initial Calibration

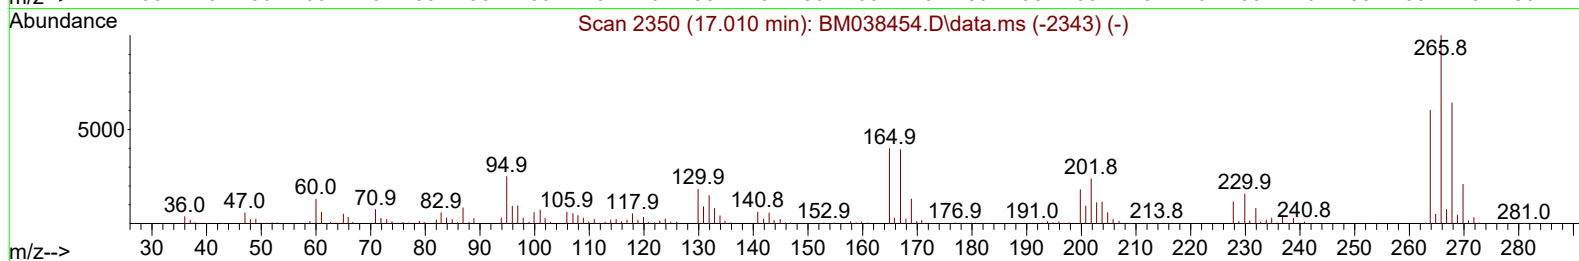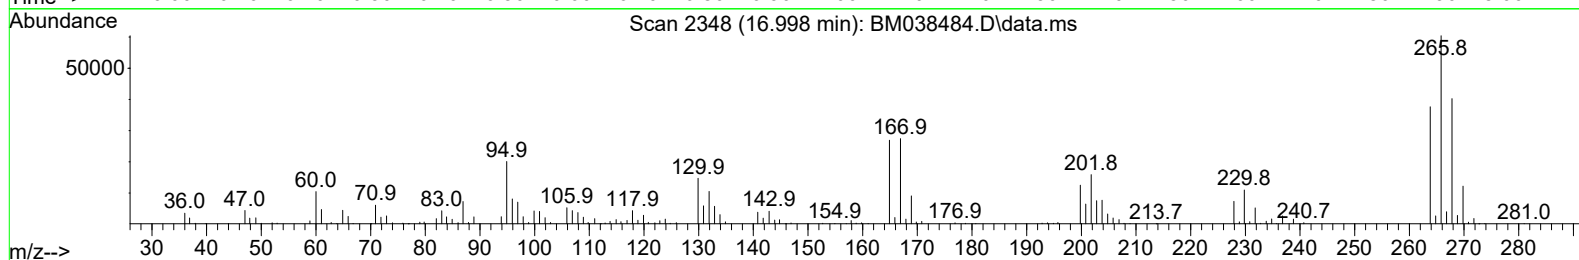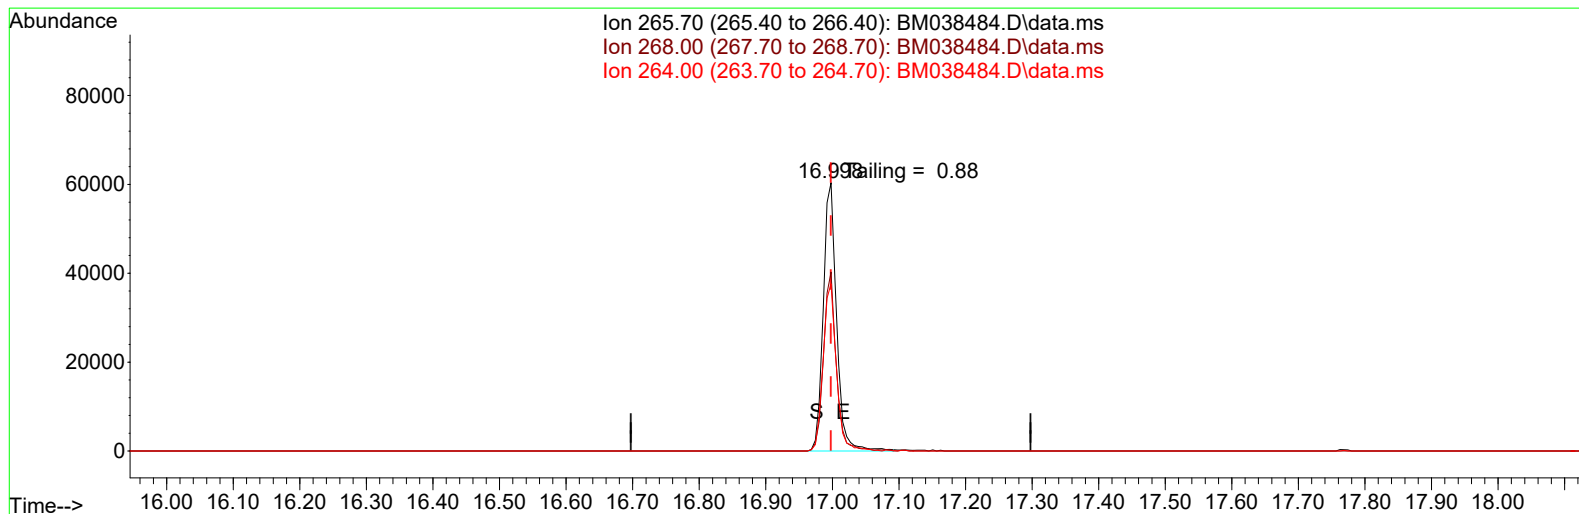

TIC: BM038484.D\data.ms

(70) Pentachlorophenol (C)

16.998min (+ 0.000) 0.00 ng




response 84593

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	66.66
264.00	60.20	62.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM011923\
Data File : BM038484.D
Acq On : 19 Jan 2023 08:20
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 20 05:15:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM011623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jan 19 06:09:42 2023
Response via : Initial Calibration

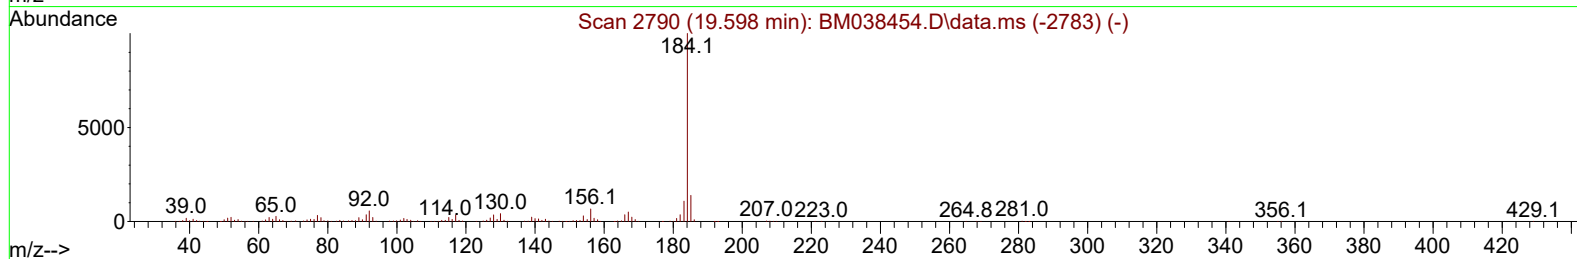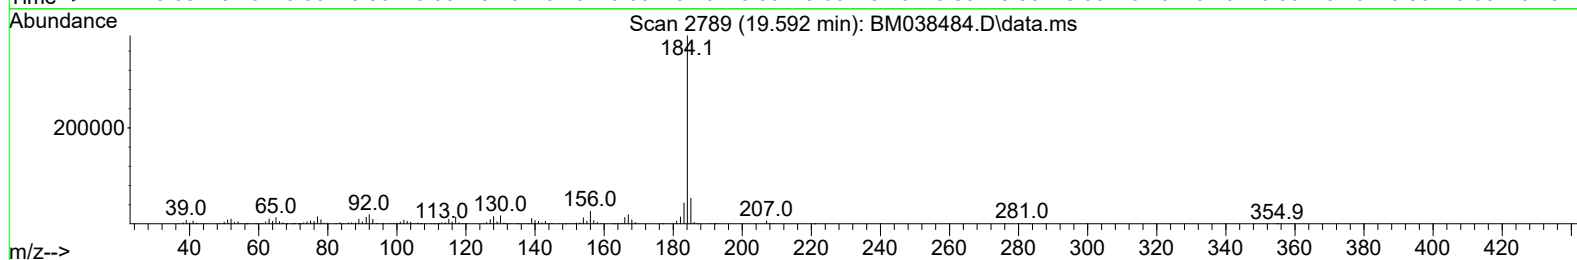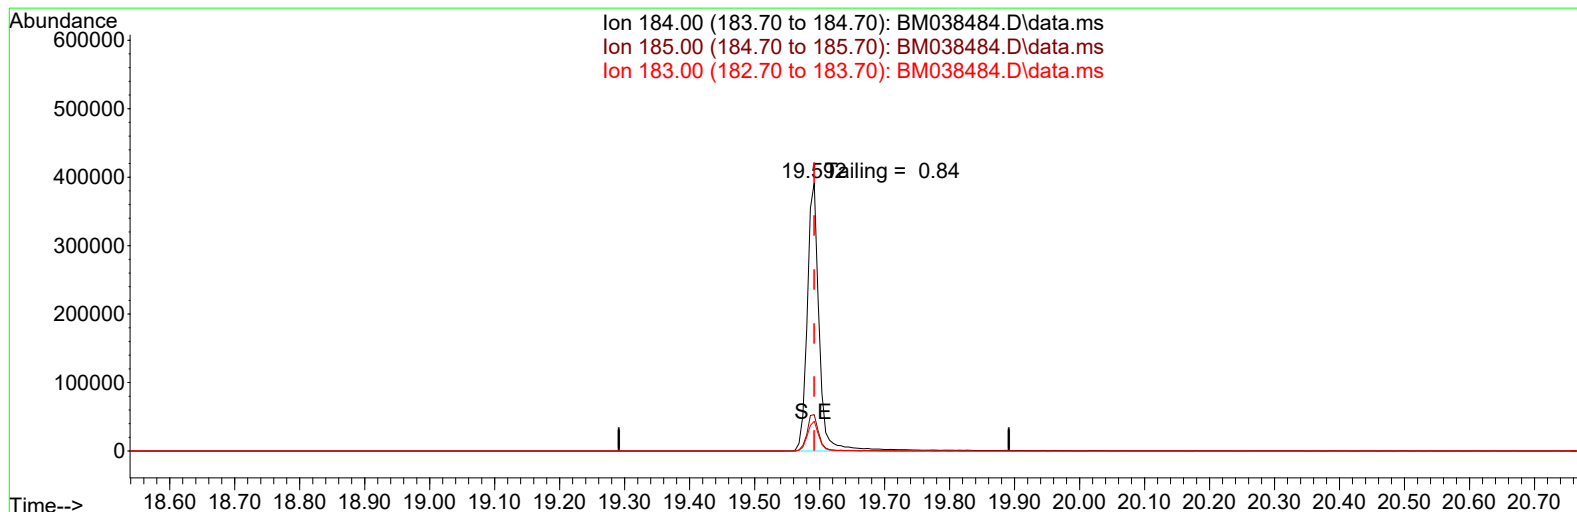

TIC: BM038484.D\data.ms

(77) Benzidine

19.592min (+ 0.000) 0.00 ng

response 504614

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	13.55
183.00	10.80	11.09
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/19/2023	BNA_M	<u>BM038484.D</u>
Compound Name	Response	Retention Time
DDT	278207	20.809
DDD	2244	20.427
DDE	0	19.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2244	280451	0.80

Instrument :
BNA_M
ClientSampleId :
DFTPP