

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012521\
 Data File : BM028530.D
 Acq On : 25 Jan 2021 15:42
 Operator : CG/JU
 Sample : L5214-01
 Misc : SFAM-MDL-W-01
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT1-2021-01

Manual Integrations
 APPROVED

mohammad
 1/27/2021 1:07:14 PM

Quant Time: Jan 25 16:12:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 25 12:52:04 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.992	152	26161	20.00	ng/ul	0.00
20) Naphthalene-d8	10.810	136	104988	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.639	164	58864	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.368	188	118330	20.00	ng/ul	0.00
79) Chrysene-d12	21.497	240	114533	20.00	ng/ul	0.00
88) Perylene-d12	23.774	264	114979	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.269	96	2031	3.26	ng/uL	0.00
4) Pyridine-d5	3.722	84	34555	19.39	ng/ul	0.00
7) Phenol-d5	7.151	99	78817	35.96	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.316	67	49467	35.71	ng/ul	0.00
11) 2-Chlorophenol-d4	7.516	132	67885	36.25	ng/ul	0.00
15) 4-Methylphenol-d8	8.704	113	66341	37.25	ng/ul	0.00
21) Nitrobenzene-d5	9.169	128	32134	37.42	ng/ul	0.00
24) 2-Nitrophenol-d4	9.886	143	35328	38.19	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.428	165	60988	35.09	ng/ul	0.00
31) 4-Chloroaniline-d4	10.945	131	85110	36.62	ng/ul	0.00
46) Dimethylphthalate-d6	14.045	166	172727	36.60	ng/ul	0.00
49) Acenaphthylene-d8	14.333	160	224584	39.08	ng/ul	0.00
54) 4-Nitrophenol-d4	14.833	143	31128	37.59	ng/ul	0.00
60) Fluorene-d10	15.627	176	143824	36.23	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.751	200	26641	35.04	ng/ul	0.00
73) Anthracene-d10	17.462	188	215675	36.67	ng/ul	0.00
81) Pyrene-d10	19.739	212	232093	35.67	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.633	264	223622	35.41	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.310	88	853	1.28	ng/uL#	91
5) Pyridine	3.746	79	7296	4.08	ng/ul#	75
6) Benzaldehyde	7.122	77	4837	5.51	ng/ul	95
8) Phenol	7.175	94	9140	4.12	ng/ul	96
10) Bis(2-Chloroethyl)ether	7.410	93	7687	4.16	ng/ul	95
12) 2-Chlorophenol	7.551	128	8091	4.26	ng/ul	97
13) 2-Methylphenol	8.439	108	6789	4.01	ng/ul	99
14) 2,2'-oxybis(1-Chloropr...	8.528	45	12088	3.82	ng/ul	97
16) Acetophenone	8.828	105	11341	4.16	ng/ul	97
17) N-Nitroso-di-n-propyla...	8.810	70	5385	3.99	ng/ul	99
18) 4-Methylphenol	8.769	108	7370	4.07	ng/ul	100
19) Hexachloroethane	9.081	117	3273	3.90	ng/ul	96
22) Nitrobenzene	9.210	77	8752	4.14	ng/ul	93
23) Isophorone	9.733	82	14574	3.96	ng/ul	99
25) 2-Nitrophenol	9.922	139	4325	4.32	ng/ul	95
26) 2,4-Dimethylphenol	9.980	107	7973	4.05	ng/ul	99
27) Bis(2-Chloroethoxy)met...	10.216	93	9959	4.16	ng/ul	99
29) 2,4-Dichlorophenol	10.457	162	7109	4.23	ng/ul	95
30) Naphthalene	10.857	128	24657	4.11	ng/ul	98
32) 4-Chloroaniline	10.969	127	9598	4.24	ng/ul	98
33) Hexachlorobutadiene	11.133	225	4700	4.12	ng/ul	96
34) Caprolactam	11.751	113	1737	3.51	ng/ul	90
35) 4-Chloro-3-methylphenol	12.086	107	6996	4.07	ng/ul	99
36) 2-Methylnaphthalene	12.469	142	16542	4.09	ng/ul	98

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012521\
 Data File : BM028530.D
 Acq On : 25 Jan 2021 15:42
 Operator : CG/JU
 Sample : L5214-01
 Misc : SFAM-MDL-W-01
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT1-2021-01


Manual Integrations
 APPROVED

mohammad
 1/27/2021 1:07:14 PM

Quant Time: Jan 25 16:12:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Jan 25 12:52:04 2021
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
37) 1-Methylnaphthalene	12.680	142	16534	4.25	ng/ul	96
39) 1,2,4,5-Tetrachloroben...	12.833	216	8332	4.12	ng/ul	100
40) Hexachlorocyclopentadiene	12.804	237	3770	3.62	ng/ul	97
41) 2,4,6-Trichlorophenol	13.074	196	4946	3.91	ng/ul	94
42) 2,4,5-Trichlorophenol	13.145	196	5426	3.99	ng/ul	88
43) 1,1'-Biphenyl	13.469	154	21043	4.08	ng/ul	97
44) 2-Chloronaphthalene	13.516	162	16471	4.10	ng/ul	98
45) 2-Nitroaniline	13.721	65	4134	3.73	ng/ul	98
47) Dimethylphthalate	14.086	163	20212	4.18	ng/ul	99
48) 2,6-Dinitrotoluene	14.216	165	3617	3.79	ng/ul	96
50) Acenaphthylene	14.363	152	24538	4.18	ng/ul	97
51) 3-Nitroaniline	14.545	138	3381	3.89	ng/ul	95
52) Acenaphthene	14.698	153	17623	4.16	ng/ul	96
53) 2,4-Dinitrophenol	14.763	184	1663	3.19	ng/ul	90
55) 4-Nitrophenol	14.845	109	2743	4.15	ng/ul#	81
56) Dibenzofuran	15.033	168	23908	4.21	ng/ul	100
57) 2,4-Dinitrotoluene	15.004	165	5030	3.91	ng/ul#	92
58) 2,3,4,6-Tetrachlorophenol	15.257	232	4328	3.92	ng/ul#	97
59) Diethylphthalate	15.445	149	19473	3.92	ng/ul	99
61) Fluorene	15.680	166	19977	4.23	ng/ul	99
62) 4-Chlorophenyl-phenyle...	15.668	204	9874	4.19	ng/ul	97
63) 4-Nitroaniline	15.698	138	3357	4.44	ng/ul	94
66) 4,6-Dinitro-2-methylph...	15.762	198	3200	3.92	ng/ul#	71
67) N-Nitrosodiphenylamine	15.880	169	16143	4.06	ng/ul	95
68) 4-Bromophenyl-phenylether	16.562	248	5684	3.94	ng/ul	95
69) Hexachlorobenzene	16.674	284	6518	3.99	ng/ul	97
70) Atrazine	16.821	200	5587	3.80	ng/ul	100
71) Pentachlorophenol	17.015	266	3091	3.35	ng/ul	96
72) Phenanthrene	17.409	178	30416	4.20	ng/ul	99
74) Anthracene	17.498	178	31102	4.22	ng/ul	99
75) 1,2,3,4-Tetrachloroben...	13.439	216	8229	4.05	ng/uL	97
76) Pentachlorobenzene	14.951	250	7685	3.87	ng/uL	97
77) Carbazole	17.762	167	26944	4.32	ng/ul	99
78) Di-n-butylphthalate	18.315	149	32501	3.78	ng/ul	99
80) Fluoranthene	19.403	202	34084	3.96	ng/ul	100
82) Pyrene	19.762	202	35450	4.01	ng/ul	99
83) Butylbenzylphthalate	20.639	149	15303	3.82	ng/ul	100
84) 3,3'-Dichlorobenzidine	21.415	252	12043	5.11	ng/ul	97
85) Benzo(a)anthracene	21.486	228	33308	4.25	ng/ul	100
86) Bis(2-ethylhexyl)phtha...	21.403	149	23005	3.71	ng/ul	99
87) Chrysene	21.539	228	32426	4.25	ng/ul	99
89) Di-n-octyl phthalate	22.286	149	39701	3.67	ng/ul	100
90) Benzo(b)fluoranthene	23.086	252	33911	4.30	ng/ul	97
91) Benzo(k)fluoranthene	23.133	252	32680m	4.25	ng/ul	
93) Benzo(a)pyrene	23.674	252	30160	4.23	ng/ul	98
94) Indeno(1,2,3-cd)pyrene	26.085	276	36801	4.37	ng/ul	97
95) Dibenzo(a,h)anthracene	26.091	278	31473	4.40	ng/ul	96
96) Benzo(g,h,i)perylene	26.791	276	30650	4.32	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2
1,4-Dioxane
Concen: 1.28 ng/uL
RT: 3.310 min Scan# 21
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Tgt Ion: 88 Resp: 853
Ion Ratio Lower Upper
88 100
43 51.9 30.7 46.1#
58 80.3 66.0 99.0

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM

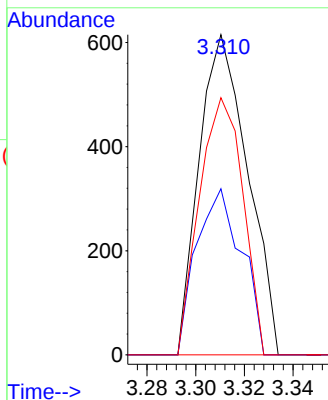


#5
Pyridine
Concen: 4.08 ng/uL
RT: 3.746 min Scan# 95
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42



Tgt Ion: 79 Resp: 7296
Ion Ratio Lower Upper
79 100
52 128.6 74.5 111.7#
51 47.8 37.5 56.3

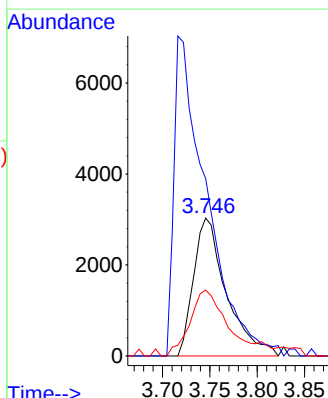







#6
Benzaldehyde
Concen: 5.51 ng/ul
RT: 7.122 min Scan# 669
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:	77	Resp:	4837
Ion	Ratio	Lower	Upper
77	100		
105	94.0	77.2	115.8
106	99.3	73.8	110.6

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM



#8
Phenol
Concen: 4.12 ng/ul
RT: 7.175 min Scan# 678
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42


Tgt Ion:	94	Resp:	9140
Ion	Ratio	Lower	Upper
94	100		
65	33.4	24.1	36.1
66	39.8	32.6	49.0





#10
Bis(2-Chloroethyl)ether
Concen: 4.16 ng/ul
RT: 7.410 min Scan# 718
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01






Tgt Ion: 93 Resp: 7687


Ion	Ratio	Lower	Upper
93	100		
63	86.1	64.8	97.2
95	30.4	25.7	38.5

Manual Integrations
APPROVED

mohammad
1/27/2021 1:07:14 PM


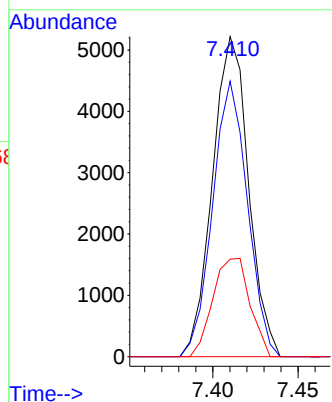



#12
2-Chlorophenol
Concen: 4.26 ng/ul
RT: 7.551 min Scan# 742
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42



Tgt Ion: 128 Resp: 8091

Ion	Ratio	Lower	Upper
128	100		
64	46.6	38.0	57.0
130	30.4	27.2	40.8

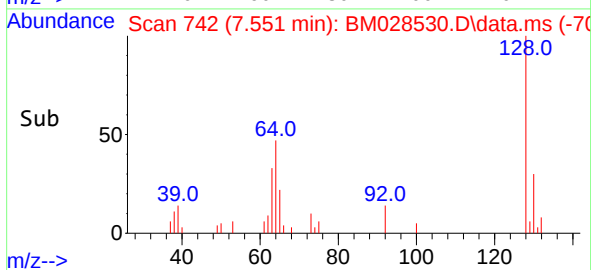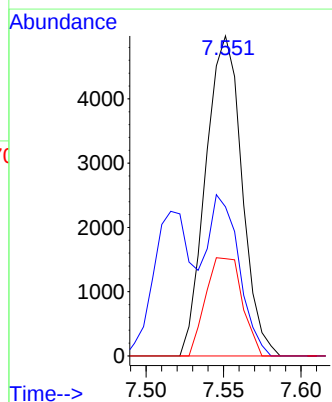







#13
2-Methylphenol
Concen: 4.01 ng/ul
RT: 8.439 min Scan# 893
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion: 108 Resp: 6789
Ion Ratio Lower Upper
108 100
107 88.3 69.6 104.4

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM




#14
2,2'-oxybis(1-Chloropropane)
Concen: 3.82 ng/ul
RT: 8.528 min Scan# 908
Delta R.T. 0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion: 45 Resp: 12088
Ion Ratio Lower Upper
45 100
77 12.7 9.7 14.5
79 9.9 6.8 10.2

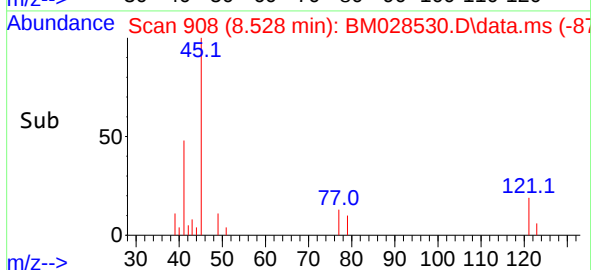







#16
Acetophenone
Concen: 4.16 ng/ul
RT: 8.828 min Scan# 959
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42





Tgt Ion:105 Resp: 11341
Ion Ratio Lower Upper
105 100
77 74.9 61.5 92.3
51 30.3 26.4 39.6

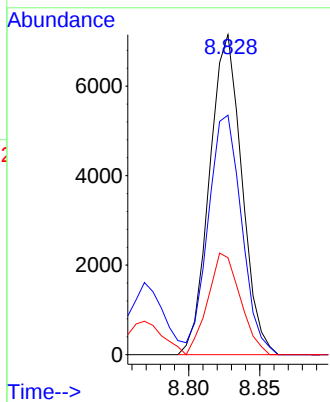

#17
N-Nitroso-di-n-propylamine
Concen: 3.99 ng/ul
RT: 8.810 min Scan# 956
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion: 70 Resp: 5385
Ion Ratio Lower Upper
70 100
42 74.9 60.4 90.6
101 10.5 8.4 12.6
130 23.0 17.0 25.6



Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01


Manual Integrations
APPROVED

mohammad
1/27/2021 1:07:14 PM



#18
4-Methylphenol
Concen: 4.07 ng/ul
RT: 8.769 min Scan# 949
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Tgt Ion:108 Resp: 7370
Ion Ratio Lower Upper
108 100
107 112.2 90.1 135.1

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM

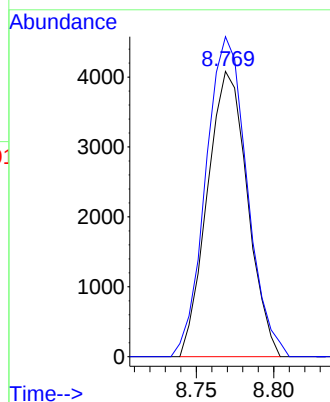


#19
Hexachloroethane
Concen: 3.90 ng/ul
RT: 9.081 min Scan# 1002
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42



Tgt Ion:117 Resp: 3273
Ion Ratio Lower Upper
117 100
201 91.2 76.9 115.3
199 59.7 46.9 70.3

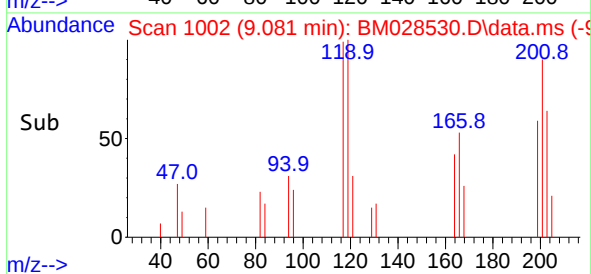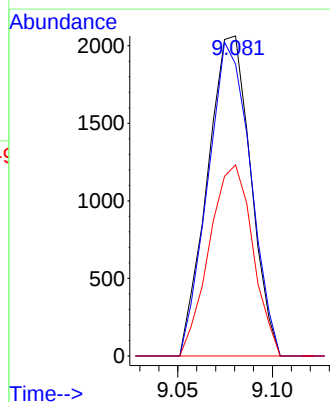

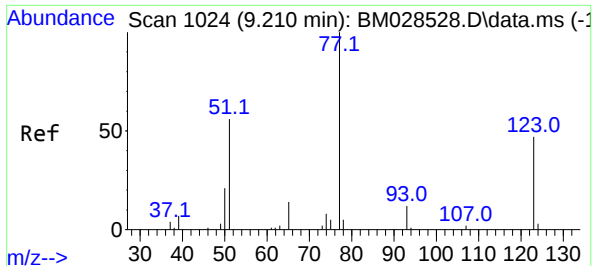





#22
Nitrobenzene
Concen: 4.14 ng/ul
RT: 9.210 min Scan# 1024
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion: 77 Resp: 8752
Ion Ratio Lower Upper
77 100
123 40.1 37.0 55.6
65 14.3 11.4 17.0

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM

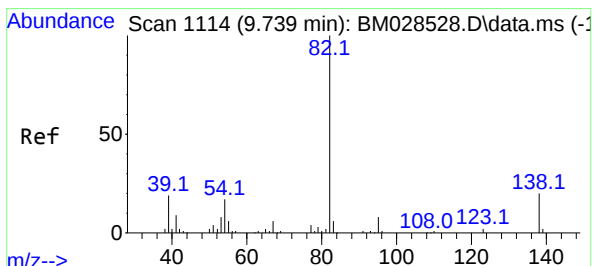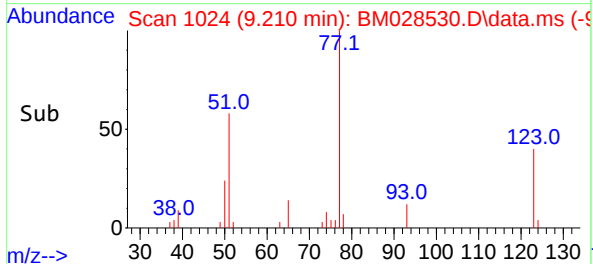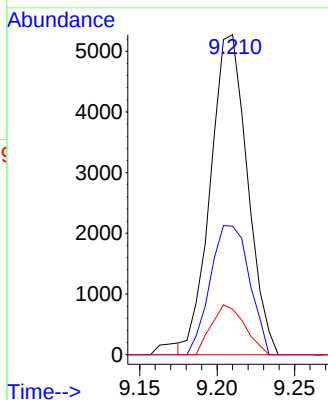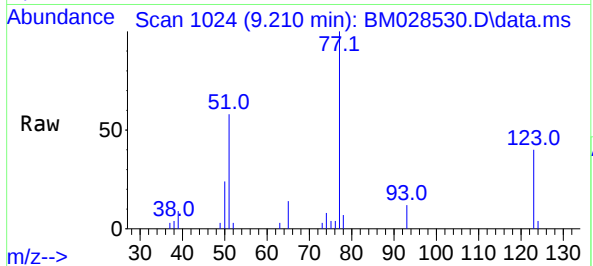

#23
Isophorone
Concen: 3.96 ng/ul
RT: 9.733 min Scan# 1113
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion: 82 Resp: 14574
Ion Ratio Lower Upper
82 100
95 6.0 5.8 8.8
138 19.1 15.2 22.8

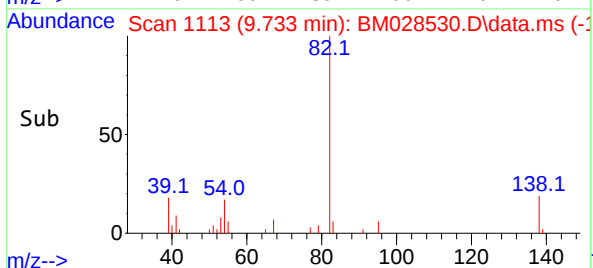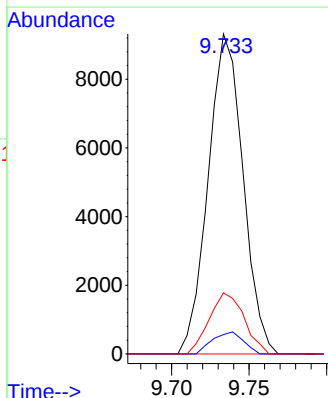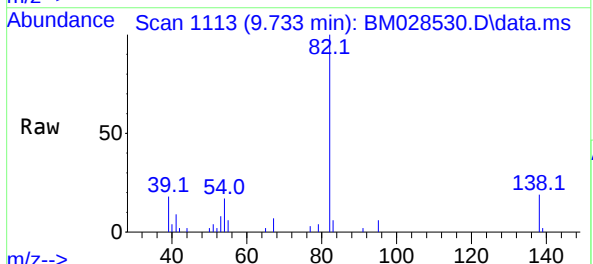







#25
2-Nitrophenol
Concen: 4.32 ng/ul
RT: 9.922 min Scan# 1145
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:139 Resp: 4325
Ion Ratio Lower Upper
139 100
65 51.5 45.2 67.8
109 32.0 24.4 36.6

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM

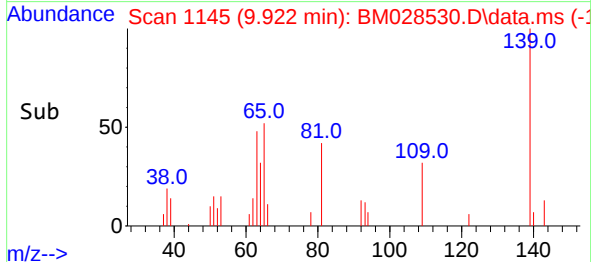

#26
2,4-Dimethylphenol
Concen: 4.05 ng/ul
RT: 9.980 min Scan# 1155
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:107 Resp: 7973
Ion Ratio Lower Upper
107 100
121 51.5 40.6 60.8
122 83.6 66.3 99.5

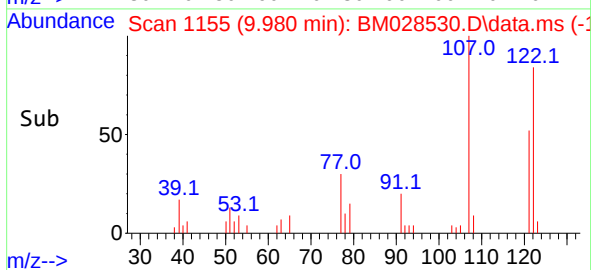







#27
 Bis(2-Chloroethoxy)methane
 Concen: 4.16 ng/ul
 RT: 10.216 min Scan# 1195
 Delta R.T. -0.000 min
 Lab File: BM028530.D
 Acq: 25 Jan 2021 15:42

Tgt Ion: 93	Resp: 9959
Ion Ratio	Lower Upper
93 100	
95 31.8	26.1 39.1
123 11.3	9.3 13.9

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT1-2021-01




Manual Integrations
 APPROVED


mohammad
 1/27/2021 1:07:14 PM

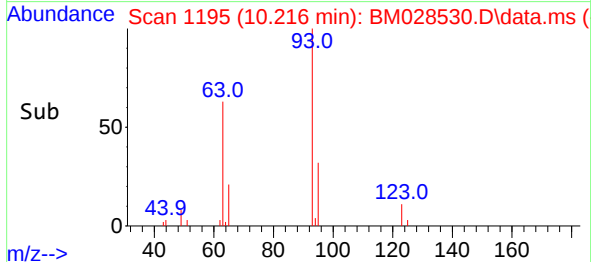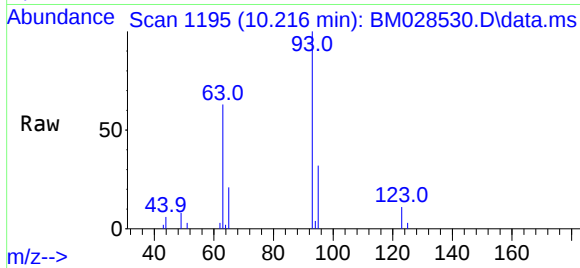


#29
 2,4-Dichlorophenol
 Concen: 4.23 ng/ul
 RT: 10.457 min Scan# 1236
 Delta R.T. -0.000 min
 Lab File: BM028530.D
 Acq: 25 Jan 2021 15:42

Tgt Ion:162	Resp:	7109	
Ion	Ratio	Lower	Upper
162	100		
164	69.6	51.9	77.9
98	34.8	30.1	45.1



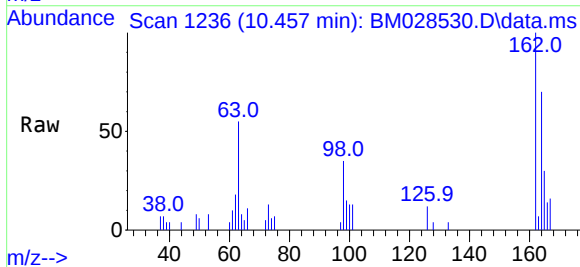





#30
Naphthalene
Concen: 4.11 ng/ul
RT: 10.857 min Scan# 1304
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42





Tgt Ion:128 Resp: 24657
Ion Ratio Lower Upper
128 100
129 11.1 9.0 13.6
127 11.7 10.5 15.7

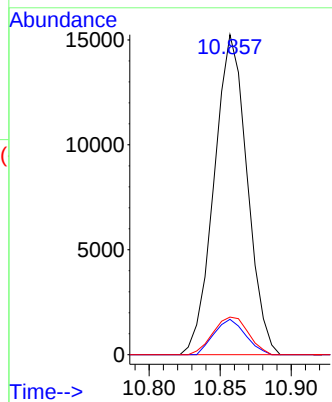

#32
4-Chloroaniline
Concen: 4.24 ng/ul
RT: 10.969 min Scan# 1323
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:127 Resp: 9598
Ion Ratio Lower Upper
127 100
129 31.3 26.1 39.1




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM



#33
Hexachlorobutadiene
Concen: 4.12 ng/ul
RT: 11.133 min Scan# 1351
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:225 Resp: 4700
Ion Ratio Lower Upper
225 100
223 62.9 50.9 76.3
227 68.5 50.7 76.1

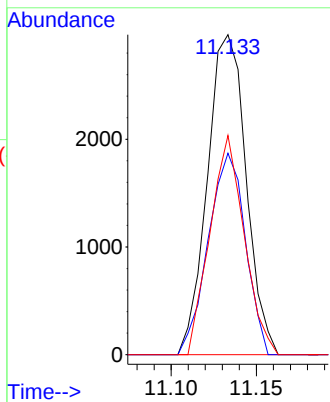


Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM




#34
Caprolactam
Concen: 3.51 ng/ul
RT: 11.751 min Scan# 1456
Delta R.T. 0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:113 Resp: 1737
Ion Ratio Lower Upper
113 100
55 168.4 146.2 219.2
56 126.9 110.6 165.8





#35
4-Chloro-3-methylphenol
Concen: 4.07 ng/ul
RT: 12.086 min Scan# 1513
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

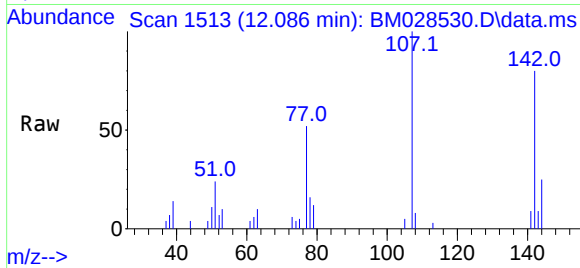


Tgt Ion:107 Resp: 6996
Ion Ratio Lower Upper
107 100
144 24.8 21.0 31.6
142 79.5 64.1 96.1

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM

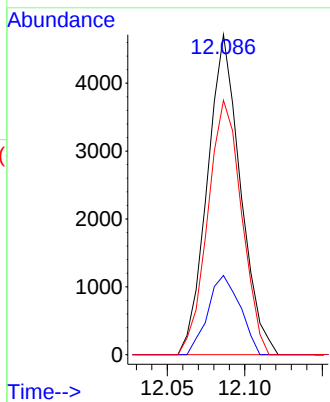


#36
2-Methylnaphthalene
Concen: 4.09 ng/ul
RT: 12.469 min Scan# 1578
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

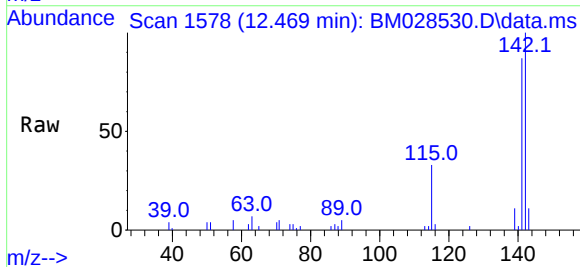

Tgt Ion:142 Resp: 16542
Ion Ratio Lower Upper
142 100
141 86.8 71.3 106.9









#37
1-Methylnaphthalene
Concen: 4.25 ng/ul
RT: 12.680 min Scan# 1614
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:142 Resp: 16534
Ion Ratio Lower Upper
142 100
141 88.5 74.2 111.4

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM

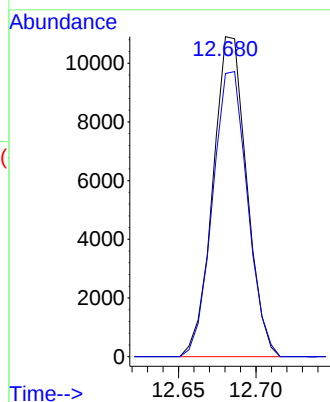


#39
1,2,4,5-Tetrachlorobenzene
Concen: 4.12 ng/ul
RT: 12.833 min Scan# 1640
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:216 Resp: 8332
Ion Ratio Lower Upper
216 100
214 79.9 64.1 96.1
179 22.3 17.8 26.6
108 17.6 14.6 21.8

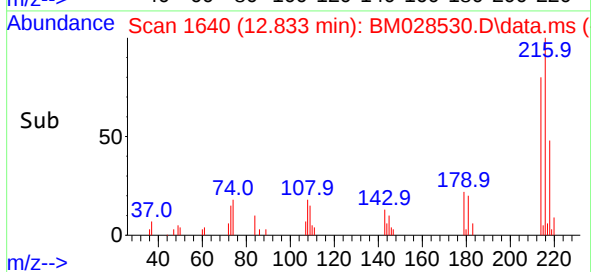





#40
Hexachlorocyclopentadiene
Concen: 3.62 ng/ul
RT: 12.804 min Scan# 1635
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:237 Resp: 3770
Ion Ratio Lower Upper
237 100
235 60.9 50.9 76.3
272 14.1 10.5 15.7




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM




#41
2,4,6-Trichlorophenol
Concen: 3.91 ng/ul
RT: 13.074 min Scan# 1681
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:196 Resp: 4946
Ion Ratio Lower Upper
196 100
198 101.8 75.8 113.8
200 33.0 24.7 37.1





#42
2,4,5-Trichlorophenol
Concen: 3.99 ng/ul
RT: 13.145 min Scan# 1693
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Tgt Ion:196 Resp: 5426
Ion Ratio Lower Upper
196 100
198 107.5 74.2 111.4
200 30.7 24.8 37.2

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM




#43
1,1'-Biphenyl
Concen: 4.08 ng/ul
RT: 13.469 min Scan# 1748
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:154 Resp: 21043
Ion Ratio Lower Upper
154 100
153 39.7 32.7 49.1
76 14.6 10.2 15.4





#44
2-Chloronaphthalene
Concen: 4.10 ng/ul
RT: 13.516 min Scan# 1756
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01



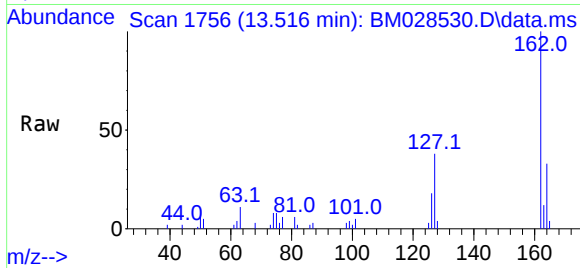


Tgt Ion:162 Resp: 16471


Ion	Ratio	Lower	Upper
162	100		
164	33.4	26.1	39.1
127	37.7	31.8	47.6

Manual Integrations
APPROVED

mohammad
1/27/2021 1:07:14 PM


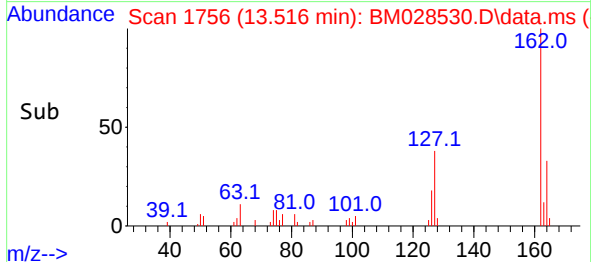



#45
2-Nitroaniline
Concen: 3.73 ng/ul
RT: 13.721 min Scan# 1791
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

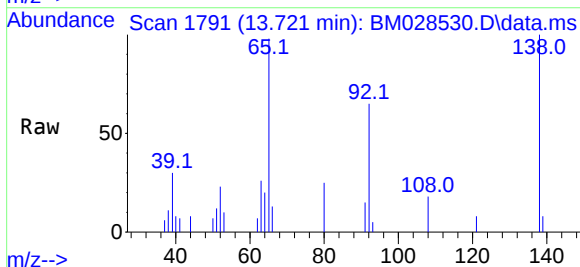

Tgt Ion: 65 Resp: 4134

Ion	Ratio	Lower	Upper
65	100		
92	66.5	51.2	76.8
138	101.7	80.2	120.2





#47

Dimethylphthalate

Concen: 4.18 ng/ul

RT: 14.086 min Scan# 1853

Delta R.T. -0.006 min

Lab File: BM028530.D

Acq: 25 Jan 2021 15:42

Tgt Ion:	163	Resp:	20212
Ion Ratio	Lower	Upper	
163	100		
194	4.1	3.3	4.9
164	10.5	8.7	13.1

Instrument :





BNA_M

ClientSampleId :

MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED

mohammad
1/27/2021 1:07:14 PM



#48

2,6-Dinitrotoluene

Concen: 3.79 ng/ul




RT: 14.216 min Scan# 1875


Delta R.T. -0.000 min

Lab File: BM028530.D


Acq: 25 Jan 2021 15:42

Tgt Ion:	165	Resp:	3617
Ion Ratio	Lower	Upper	
165	100		
89	61.0	46.3	69.5
121	23.9	17.4	26.2

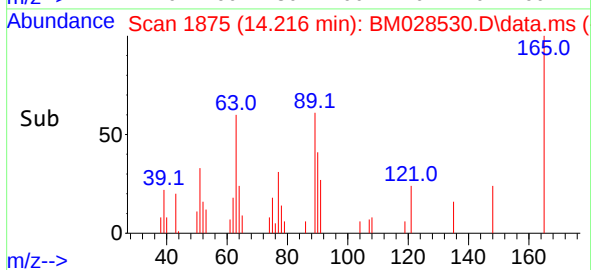



#50
Acenaphthylene
Concen: 4.18 ng/ul
RT: 14.363 min Scan# 1900
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42






Tgt Ion:	152	Resp:	24538
Ion Ratio	Lower	Upper	
152	100		
151	21.4	15.4	23.2
153	12.8	10.2	15.4


Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM

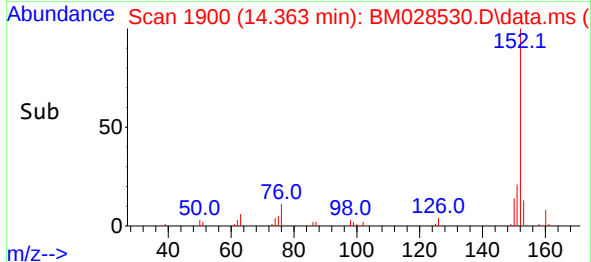


#51
3-Nitroaniline
Concen: 3.89 ng/ul
RT: 14.545 min Scan# 1931
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:	138	Resp:	3381
Ion Ratio	Lower	Upper	
138	100		
108	9.5	8.2	12.4
92	121.9	92.8	139.2





#52
Acenaphthene
Concen: 4.16 ng/ul
RT: 14.698 min Scan# 1957
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42





Tgt Ion:153 Resp: 17623
Ion Ratio Lower Upper
153 100
152 43.5 37.5 56.3
154 89.9 69.1 103.7


Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM




#53
2,4-Dinitrophenol
Concen: 3.19 ng/ul
RT: 14.763 min Scan# 1968
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:184 Resp: 1663
Ion Ratio Lower Upper
184 100
63 67.5 61.0 91.4
154 54.8 49.2 73.8


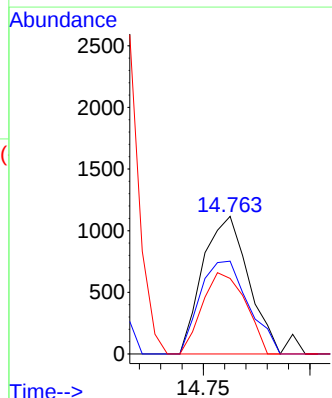






#55
4-Nitrophenol
Concen: 4.15 ng/ul
RT: 14.845 min Scan# 1982
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42





Tgt Ion:109 Resp: 2743
Ion Ratio Lower Upper
109 100
139 142.5 103.4 155.2
65 161.4 104.9 157.3#

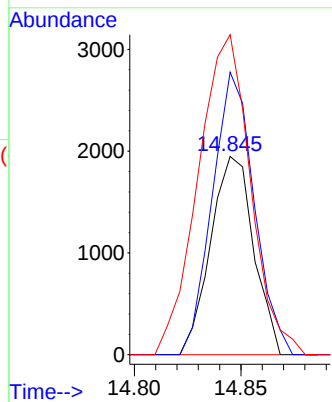

#56
Dibenzofuran
Concen: 4.21 ng/ul
RT: 15.033 min Scan# 2014
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:168 Resp: 23908
Ion Ratio Lower Upper
168 100
139 36.9 29.8 44.6




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM



#57
2,4-Dinitrotoluene
Concen: 3.91 ng/ul
RT: 15.004 min Scan# 2009
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:165 Resp: 5030
Ion Ratio Lower Upper
165 100
63 43.8 39.3 58.9
182 0.0 2.2 3.4#




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM




#58
2,3,4,6-Tetrachlorophenol
Concen: 3.92 ng/ul
RT: 15.257 min Scan# 2052
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:232 Resp: 4328
Ion Ratio Lower Upper
232 100
131 45.8 38.6 57.8
130 0.0 2.1 3.1#
166 30.7 24.2 36.4

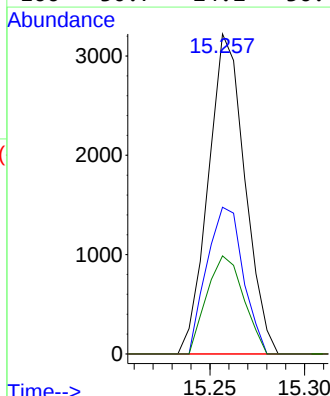



#59
Diethylphthalate
Concen: 3.92 ng/ul
RT: 15.445 min Scan# 2084
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Tgt Ion:149 Resp: 19473
Ion Ratio Lower Upper
149 100
177 20.7 16.9 25.3
150 12.2 9.9 14.9

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM

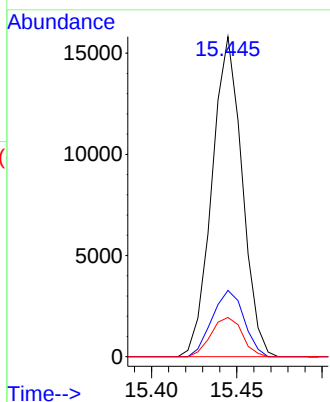


#61
Fluorene
Concen: 4.23 ng/ul
RT: 15.680 min Scan# 2124
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:166 Resp: 19977
Ion Ratio Lower Upper
166 100
165 97.5 77.0 115.4
167 12.6 10.6 16.0





#62
4-Chlorophenyl-phenylether
Concen: 4.19 ng/ul
RT: 15.668 min Scan# 2122
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Tgt Ion:204 Resp: 9874
Ion Ratio Lower Upper
204 100
206 33.5 25.9 38.9
141 58.9 49.0 73.4

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM

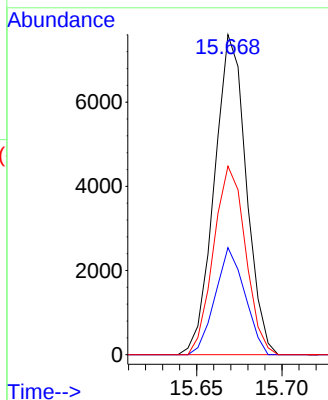


#63
4-Nitroaniline
Concen: 4.44 ng/ul
RT: 15.698 min Scan# 2127
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42



Tgt Ion:138 Resp: 3357
Ion Ratio Lower Upper
138 100
92 53.5 39.8 59.8
108 80.6 60.6 91.0

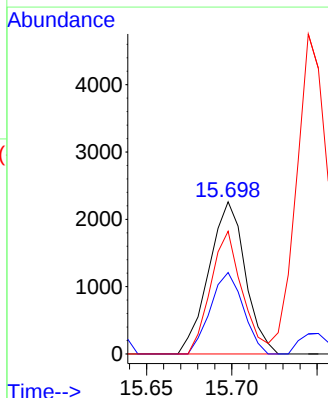







#66
4,6-Dinitro-2-methylphenol
Concen: 3.92 ng/ul
RT: 15.762 min Scan# 2138
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:198 Resp: 3200
Ion Ratio Lower Upper
198 100
182 9.5 3.3 4.9#
77 41.5 20.6 31.0#

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM

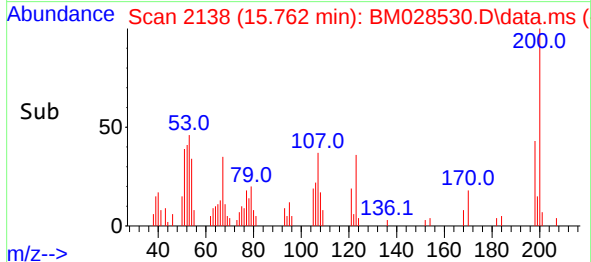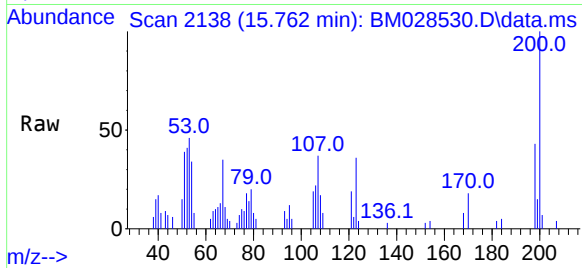


#67
N-Nitrosodiphenylamine
Concen: 4.06 ng/ul
RT: 15.880 min Scan# 2158
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:169 Resp: 16143
Ion Ratio Lower Upper
169 100
168 61.8 53.5 80.3
167 37.3 28.2 42.2



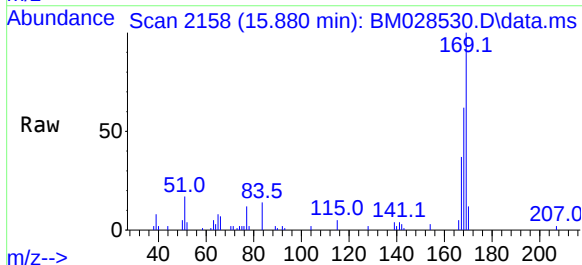





#68
4-Bromophenyl-phenylether
Concen: 3.94 ng/ul
RT: 16.562 min Scan# 2274
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

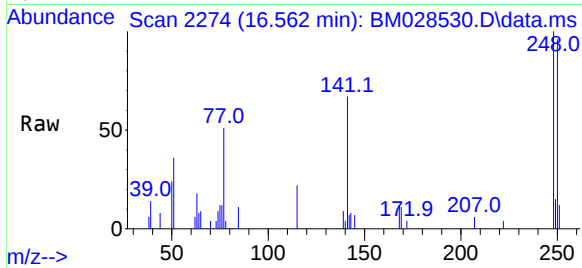



Tgt Ion:248 Resp: 5684
Ion Ratio Lower Upper
248 100
250 96.1 77.9 116.9
141 66.7 60.6 90.8

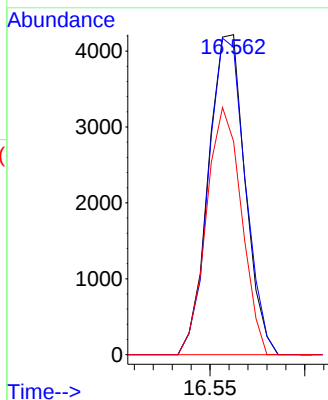

#69
Hexachlorobenzene
Concen: 3.99 ng/ul
RT: 16.674 min Scan# 2293
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

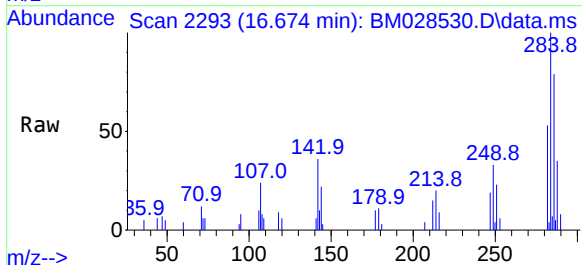


Tgt Ion:284 Resp: 6518
Ion Ratio Lower Upper
284 100
142 33.4 28.1 42.1
249 31.1 23.4 35.2

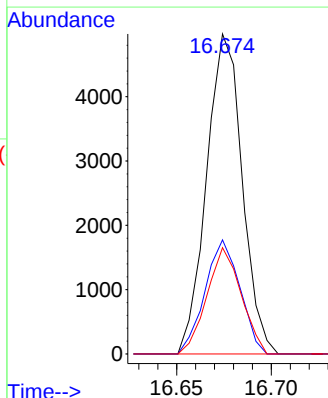


Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM



#70
Atrazine
Concen: 3.80 ng/ul
RT: 16.821 min Scan# 2318
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:200 Resp: 5587
Ion Ratio Lower Upper
200 100
173 27.4 21.5 32.3
215 47.4 37.9 56.9

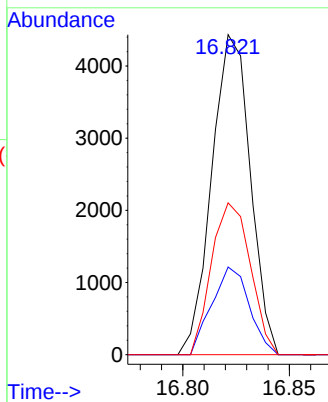


Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM




#71
Pentachlorophenol
Concen: 3.35 ng/ul
RT: 17.015 min Scan# 2351
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:266 Resp: 3091
Ion Ratio Lower Upper
266 100
264 57.7 49.5 74.3
268 61.8 50.6 76.0

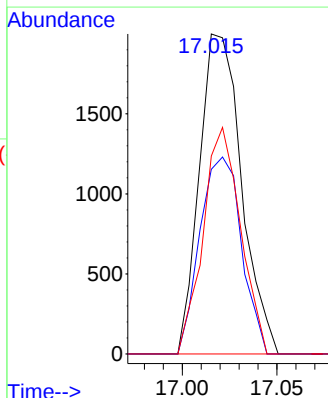



#72
Phenanthrene
Concen: 4.20 ng/ul
RT: 17.409 min Scan# 2418
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Tgt Ion:178 Resp: 30416
Ion Ratio Lower Upper
178 100
179 14.7 12.3 18.5
176 18.8 14.8 22.2

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM

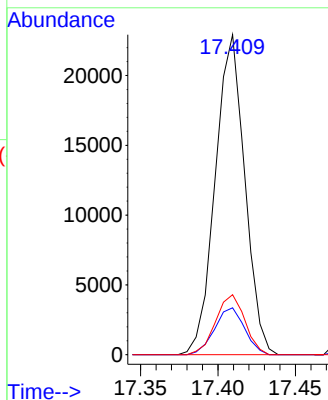


#74
Anthracene
Concen: 4.22 ng/ul
RT: 17.498 min Scan# 2433
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42



Tgt Ion:178 Resp: 31102
Ion Ratio Lower Upper
178 100
179 15.8 12.2 18.4
176 17.5 14.3 21.5

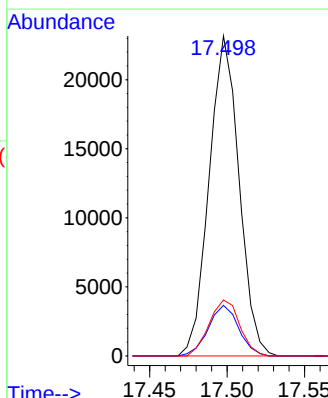







#75
1,2,3,4-Tetrachlorobenzene
Concen: 4.05 ng/uL
RT: 13.439 min Scan# 1743
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:	216	Resp:	8229
Ion Ratio	Lower	Upper	
216	100		
214	81.9	62.6	93.8
218	47.4	38.7	58.1

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM

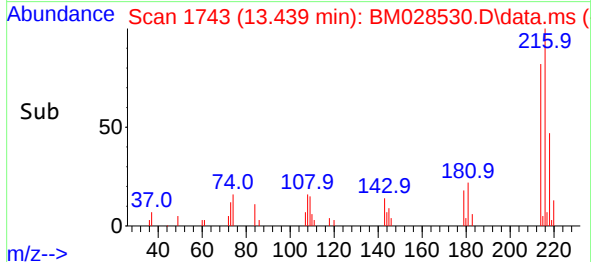

#76
Pentachlorobenzene
Concen: 3.87 ng/uL
RT: 14.951 min Scan# 2000
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42


Tgt Ion:	250	Resp:	7685
Ion Ratio	Lower	Upper	
250	100		
248	65.3	51.2	76.8
252	64.6	49.6	74.4

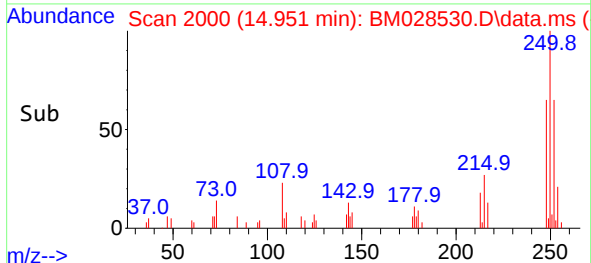



#77
Carbazole
Concen: 4.32 ng/ul
RT: 17.762 min Scan# 2478
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Tgt Ion:167 Resp: 26944
Ion Ratio Lower Upper
167 100
166 20.8 17.1 25.7
139 12.0 10.1 15.1

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM

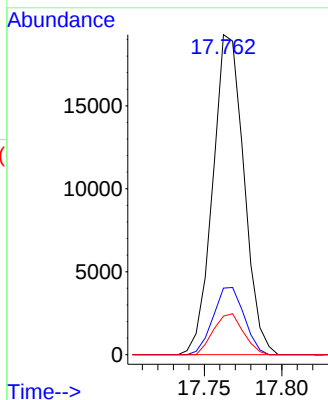


#78
Di-n-butylphthalate
Concen: 3.78 ng/ul
RT: 18.315 min Scan# 2572
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:149 Resp: 32501
Ion Ratio Lower Upper
149 100
150 8.6 7.2 10.8
104 4.9 4.2 6.2

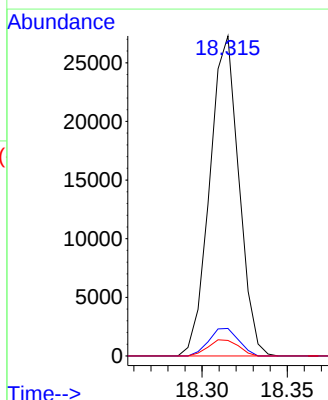



#80
Fluoranthene
Concen: 3.96 ng/ul
RT: 19.403 min Scan# 2757
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Tgt Ion:	202	Resp:	34084
Ion Ratio	Lower	Upper	
202	100		
101	11.5	9.3	13.9
100	9.2	7.4	11.2

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM




#82
Pyrene
Concen: 4.01 ng/ul
RT: 19.762 min Scan# 2818
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42



Tgt Ion:	202	Resp:	35450
Ion Ratio	Lower	Upper	
202	100		
101	14.1	10.9	16.3
100	11.8	9.4	14.2









#83
Butylbenzylphthalate
Concen: 3.82 ng/ul
RT: 20.639 min Scan# 2967
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:	149	Resp:	15303
Ion Ratio	Lower	Upper	
149	100		
91	73.2	58.8	88.2
206	20.5	16.1	24.1

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM




#84
3,3'-Dichlorobenzidine
Concen: 5.11 ng/ul
RT: 21.415 min Scan# 3099
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:	252	Resp:	12043
Ion Ratio	Lower	Upper	
252	100		
254	63.6	52.9	79.3
126	11.9	9.4	14.2


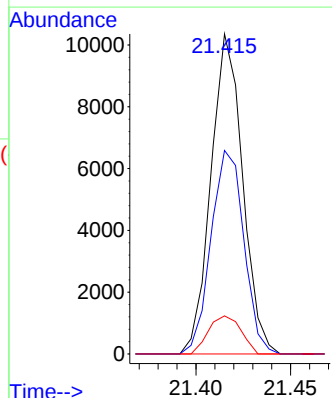






#85
Benzo(a)anthracene
Concen: 4.25 ng/ul
RT: 21.486 min Scan# 3111
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42





Tgt Ion:228 Resp: 33308
Ion Ratio Lower Upper
228 100
229 18.9 15.4 23.2
226 27.1 21.7 32.5



#86
Bis(2-ethylhexyl)phthalate
Concen: 3.71 ng/ul
RT: 21.403 min Scan# 3097
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:149 Resp: 23005
Ion Ratio Lower Upper
149 100
167 26.9 21.4 32.0
279 4.3 3.3 4.9



Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01


Manual Integrations
APPROVED

mohammad
1/27/2021 1:07:14 PM



#87
Chrysene
Concen: 4.25 ng/ul
RT: 21.539 min Scan# 3120
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01



Tgt Ion:228 Resp: 32426
Ion Ratio Lower Upper
228 100
226 28.3 23.2 34.8
229 19.1 15.8 23.6




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM

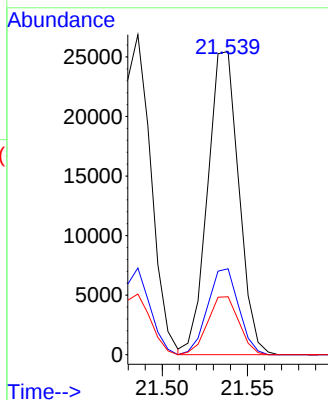

#89
Di-n-octyl phthalate
Concen: 3.67 ng/ul
RT: 22.286 min Scan# 3247
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:149 Resp: 39701

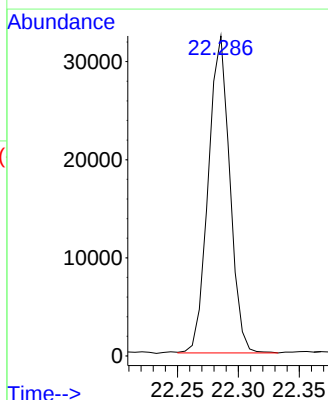







#90
Benzo(b)fluoranthene
Concen: 4.30 ng/ul
RT: 23.086 min Scan# 3383
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:252 Resp: 33911
Ion Ratio Lower Upper
252 100
253 20.5 17.5 26.3
125 12.1 8.7 13.1

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01




Manual Integrations
APPROVED


mohammad
1/27/2021 1:07:14 PM




#91
Benzo(k)fluoranthene
Concen: 4.25 ng/ul m
RT: 23.133 min Scan# 3391
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:252 Resp: 32680
Ion Ratio Lower Upper
252 100
253 24.4 17.8 26.6
125 14.2 9.0 13.6#

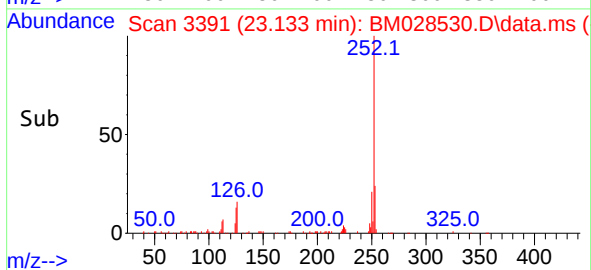




#93
Benzo(a)pyrene
Concen: 4.23 ng/u1
RT: 23.674 min Scan# 3483
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42




Tgt Ion:252 Resp: 30160
Ion Ratio Lower Upper
252 100
253 22.1 17.4 26.2
125 14.8 10.6 15.8




Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED



mohammad
1/27/2021 1:07:14 PM




#94
Indeno(1,2,3-cd)pyrene
Concen: 4.37 ng/u1
RT: 26.085 min Scan# 3893
Delta R.T. -0.000 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42



Tgt Ion:276 Resp: 36801
Ion Ratio Lower Upper
276 100
138 29.1 22.0 33.0
277 24.5 20.4 30.6









#95
Dibenzo(a,h)anthracene
Concen: 4.40 ng/ul
RT: 26.091 min Scan# 3894
Delta R.T. -0.006 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:278 Resp: 31473
Ion Ratio Lower Upper
278 100
139 18.4 13.8 20.8
279 25.0 18.2 27.4

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT1-2021-01

Manual Integrations
APPROVED

mohammad
1/27/2021 1:07:14 PM

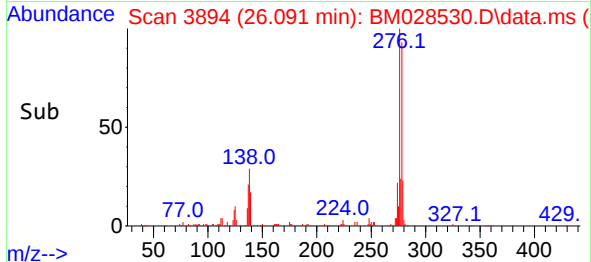

#96
Benzo(g,h,i)perylene
Concen: 4.32 ng/ul
RT: 26.791 min Scan# 4013
Delta R.T. -0.012 min
Lab File: BM028530.D
Acq: 25 Jan 2021 15:42

Tgt Ion:276 Resp: 30650
Ion Ratio Lower Upper
276 100
138 25.0 18.9 28.3
277 23.0 18.3 27.5

