
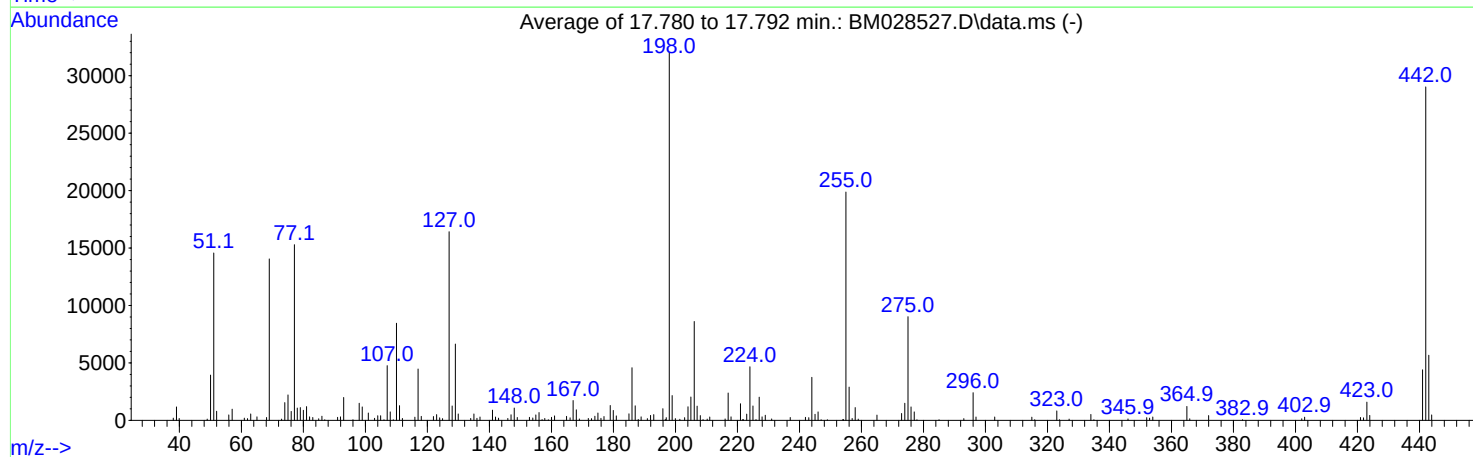


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012521\
 Data File : BM028527.D
 Acq On : 25 Jan 2021 11:39
 Operator : CG/JU
 Sample : DFTPP21
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP021

Integration File: LSCINT.P

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM011921.M
 Title : SVOA CALIBRATION
 Last Update : Mon Jan 25 12:52:04 2021

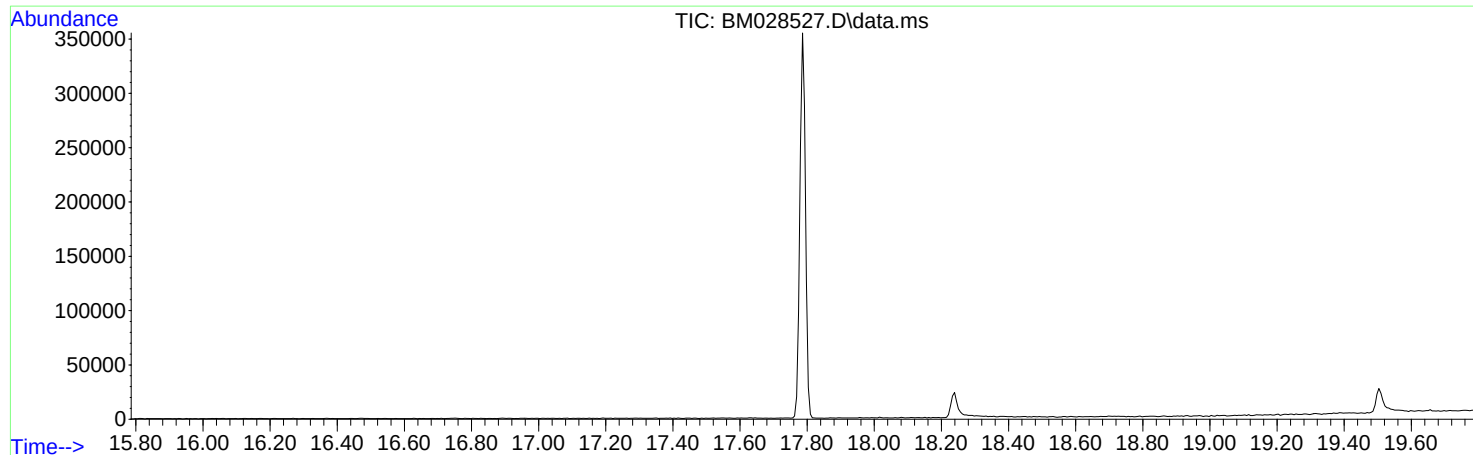

AutoFind: Scans 2481, 2482, 2483; Background Corrected with Scan 2476

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	14567	PASS
68	69	0.00	2	1.8	257	PASS
69	198	0.00	100	43.9	14059	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.3	16423	PASS
197	198	0.00	2	0.7	236	PASS
198	198	100	100	100.0	32021	PASS
199	198	5	9	6.7	2157	PASS
275	198	10	60	28.2	9033	PASS
365	198	1	100	3.8	1218	PASS
441	198	0.01	100	13.7	4399	PASS
442	198	50	100	90.6	29027	PASS
443	442	15	24	19.5	5670	PASS

m/z	Abundance
43.90	476.0
72.90	185.0
207.00	426.0

Instrument :
BNA_M
ClientSampleId :
DFTPP021

m/z	Abundance
38.00	151.0
39.10	1127.0
40.00	161.0
44.00	427.0
48.90	156.0
50.00	3902.0
51.10	14406.0
52.00	771.0
56.00	463.0
57.00	958.0
60.90	174.0
62.00	212.0
63.00	505.0
65.00	271.0
68.10	282.0
69.00	13369.0
73.10	363.0
74.00	1379.0
75.00	2206.0
76.10	723.0
77.10	14631.0
78.00	1012.0
79.00	1070.0
80.00	934.0
81.00	1175.0
82.00	277.0
83.10	267.0
84.90	186.0
85.90	318.0
91.00	249.0
91.90	280.0
93.00	1955.0
96.00	159.0
98.00	1415.0
99.00	1122.0
101.00	649.0
102.90	240.0
104.00	443.0
104.90	361.0
107.00	4455.0
108.00	644.0
110.00	7814.0
111.00	1175.0
111.90	172.0
116.00	258.0
117.00	4253.0
118.00	343.0
121.90	300.0
123.00	528.0
123.90	193.0
127.00	15087.0
128.00	1091.0
129.00	6239.0
129.90	442.0
133.90	180.0
135.00	528.0
135.90	181.0
136.90	254.0
141.00	808.0
142.00	248.0
143.00	155.0
146.00	163.0
147.00	428.0
148.00	950.0
149.00	271.0
152.90	268.0
154.00	167.0
155.00	400.0
156.00	527.0
157.90	166.0
160.00	202.0
161.00	365.0
164.90	250.0
166.00	269.0
167.00	1581.0
168.00	791.0
169.00	156.0
171.90	166.0
174.00	355.0
175.00	543.0
175.90	166.0
177.00	297.0
178.90	1044.0
180.00	889.0
180.90	406.0
185.00	432.0
186.00	3872.0
187.00	976.0
189.00	272.0
190.90	151.0
191.90	391.0
193.00	408.0

Instrument :
BNA_M
ClientSampleId :
DFTPP021

196.00	777.0
197.10	240.0
198.00	26720.0
198.90	1970.0
201.40	150.0
203.00	169.0
204.00	1059.0
205.00	1778.0
206.10	7453.0
207.10	1429.0
208.00	379.0
211.00	235.0
217.00	2118.0
217.90	272.0
221.00	1196.0
221.70	202.0
223.00	450.0
224.00	3818.0
225.00	1103.0
227.00	1653.0
227.90	210.0
228.90	345.0
237.00	196.0
241.90	190.0
243.00	232.0
244.00	3029.0
245.10	392.0
246.00	601.0
255.00	16084.0
256.00	2402.0
258.00	869.0
265.00	419.0
273.00	484.0
274.00	1182.0
275.00	6598.0
276.00	966.0
277.00	573.0
296.00	1901.0
296.90	264.0
303.00	229.0
315.00	160.0
323.00	604.0
334.00	398.0
352.00	169.0
352.90	153.0
354.00	190.0
364.90	959.0
372.00	279.0
402.90	155.0
420.90	180.0
421.90	166.0
423.00	1085.0
424.00	288.0
441.00	2680.0
442.00	18592.0
443.00	3811.0
444.00	293.0

Instrument :
BNA_M
ClientSampleId :
DFTPP021

m/z	Abundance
38.00	259.0
39.00	1411.0
39.90	152.0
43.90	429.0
49.00	177.0
50.00	4750.0
51.10	17344.0
52.00	944.0
56.00	595.0
57.00	1186.0
60.90	245.0
61.90	231.0
63.00	695.0
65.00	355.0
68.10	317.0
69.00	16960.0
73.00	292.0
74.00	1817.0
75.00	2585.0
76.00	959.0
77.10	18304.0
78.00	1290.0
79.00	1357.0
80.00	1025.0
81.00	1312.0
82.00	370.0
83.00	302.0
85.00	221.0
86.00	391.0
86.90	187.0
91.00	358.0
92.00	365.0
93.00	2254.0
98.00	1799.0
99.00	1463.0
100.90	645.0
103.00	310.0
104.00	455.0
104.90	476.0
106.00	159.0
107.00	5657.0
108.00	931.0
109.00	183.0
110.00	10185.0
111.00	1609.0
111.90	194.0
116.00	350.0
117.00	5291.0
118.00	436.0
122.00	438.0
123.00	533.0
124.00	287.0
124.90	217.0
127.00	19376.0
128.00	1507.0
129.00	7874.0
129.90	708.0
133.90	176.0
135.00	580.0
136.00	229.0
136.90	344.0
141.00	1014.0
141.90	320.0
142.90	202.0
145.90	168.0
146.90	598.0
148.00	1299.0
149.00	295.0
152.90	286.0
154.00	255.0
155.00	639.0
156.00	931.0
157.00	218.0
157.90	157.0
159.00	184.0
160.00	345.0
161.00	534.0
164.90	443.0
166.00	186.0
167.00	2039.0
168.00	1155.0
169.00	228.0
171.90	175.0
172.90	268.0
174.00	425.0
175.00	769.0
176.00	220.0
176.90	434.0
179.00	1629.0
179.90	911.0
181.00	428.0
185.00	766.0

Instrument :
BNA_M
ClientSampleId :
DFTPP021

186.00	5330.0
187.00	1492.0
188.00	233.0
189.00	345.0
191.00	293.0
192.00	446.0
193.00	651.0
195.90	1268.0
196.70	248.0
197.10	239.0
198.00	38400.0
199.00	2474.0
199.90	258.0
201.40	160.0
202.90	257.0
204.00	1483.0
205.00	2385.0
206.10	10032.0
207.10	1950.0
208.00	420.0
208.90	201.0
210.20	175.0
211.10	371.0
216.00	218.0
217.00	2832.0
217.90	382.0
221.00	1839.0
223.00	674.0
224.00	5372.0
225.00	1445.0
226.00	202.0
227.00	2438.0
227.90	398.0
229.00	551.0
231.10	238.0
237.00	290.0
242.00	320.0
243.00	286.0
244.00	4453.0
245.00	629.0
246.00	940.0
247.00	160.0
249.00	174.0
254.00	237.0
255.00	23640.0
256.00	3438.0
257.00	262.0
258.00	1280.0
259.00	167.0
265.00	516.0
272.90	675.0
274.00	1728.0
275.00	10934.0
276.00	1338.0
277.00	882.0
285.00	165.0
293.00	237.0
296.00	2728.0
297.00	364.0
303.00	327.0
315.00	402.0
315.90	188.0
323.00	923.0
323.90	169.0
327.00	187.0
334.00	659.0
335.00	180.0
345.90	203.0
352.00	300.0
353.00	236.0
353.90	356.0
365.00	1402.0
365.90	227.0
372.00	455.0
402.00	225.0
402.90	319.0
421.00	283.0
422.00	267.0
423.00	1742.0
423.90	534.0
441.00	5124.0
442.00	32768.0
443.00	6521.0
444.00	530.0

Instrument :
BNA_M
ClientSampleId :
DFTPP021

m/z	Abundance
38.00	159.0
39.00	962.0
39.90	177.0
44.00	440.0
50.10	3161.0
51.10	11950.0
52.00	678.0
55.90	378.0
57.00	805.0
61.00	159.0
63.00	481.0
65.00	303.0
68.10	171.0
69.00	11848.0
73.00	256.0
74.00	1450.0
75.00	1865.0
76.00	639.0
77.10	12954.0
78.00	915.0
79.00	905.0
80.00	675.0
81.00	1090.0
82.00	271.0
83.00	187.0
86.00	380.0
91.00	191.0
92.00	257.0
93.00	1760.0
98.00	1257.0
98.90	926.0
101.00	617.0
104.00	307.0
104.90	366.0
107.00	4190.0
108.00	659.0
110.00	7379.0
111.00	1072.0
112.00	159.0
115.90	230.0
117.00	3871.0
118.00	263.0
121.90	278.0
122.90	460.0
123.90	188.0
124.90	244.0
127.00	14805.0
128.00	1163.0
129.00	5827.0
130.00	526.0
134.00	156.0
135.00	564.0
135.90	158.0
137.00	272.0
141.00	875.0
142.00	302.0
142.90	213.0
146.00	165.0
147.00	428.0
148.00	954.0
149.00	201.0
152.90	245.0
154.00	196.0
154.90	395.0
156.00	589.0
157.80	172.0
160.00	255.0
161.00	291.0
164.90	339.0
166.00	216.0
167.00	1576.0
168.00	802.0
171.90	167.0
173.00	184.0
174.00	303.0
175.00	628.0
176.00	165.0
176.90	266.0
178.90	1203.0
180.00	814.0
181.00	352.0
185.00	509.0
186.00	4538.0
187.00	1355.0
188.90	322.0
192.00	450.0
193.00	461.0
196.00	1003.0
196.90	228.0
198.00	30944.0
198.90	2028.0
200.00	225.0

Instrument :
BNA_M
ClientSampleId :
DFTPP021

202.90	283.0
204.10	1013.0
205.00	1933.0
206.00	8358.0
207.00	1604.0
208.00	443.0
210.30	171.0
211.00	266.0
216.00	177.0
217.00	2187.0
218.00	286.0
221.00	1307.0
221.90	228.0
223.00	500.0
224.00	4807.0
225.00	1199.0
227.00	1954.0
228.00	332.0
229.00	447.0
231.00	159.0
237.00	277.0
242.00	298.0
243.00	194.0
244.00	3757.0
245.00	554.0
246.00	684.0
254.20	223.0
255.00	19912.0
256.00	2843.0
257.00	231.0
258.00	1192.0
258.90	190.0
265.00	438.0
272.90	646.0
274.00	1557.0
275.00	9566.0
276.00	1214.0
277.00	767.0
277.90	157.0
293.00	231.0
296.00	2607.0
297.00	257.0
303.00	330.0
314.90	294.0
323.00	944.0
327.00	159.0
334.00	494.0
346.00	174.0
352.00	243.0
352.90	190.0
354.00	316.0
365.00	1294.0
365.90	184.0
372.00	515.0
382.90	150.0
402.00	206.0
403.00	373.0
421.00	275.0
421.90	250.0
423.00	1925.0
424.00	478.0
441.00	5392.0
442.00	35720.0
443.00	6679.0
443.90	598.0

Instrument :
BNA_M
ClientSampleId :
DFTPP021