
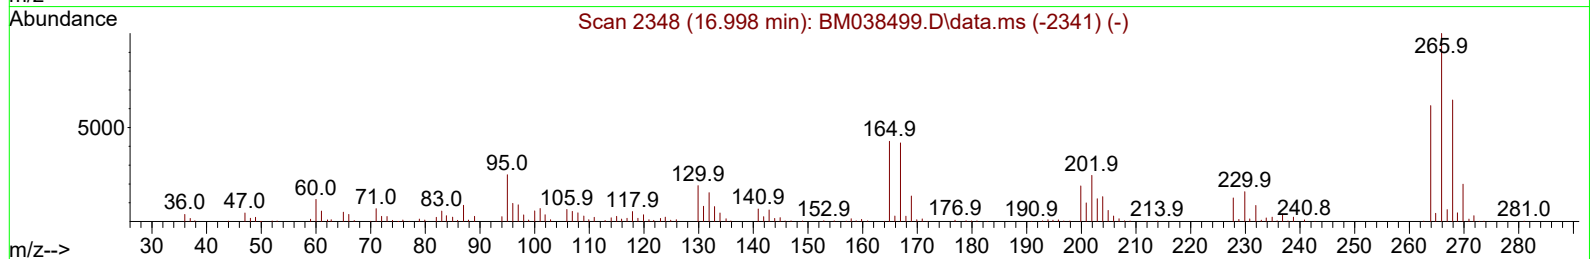
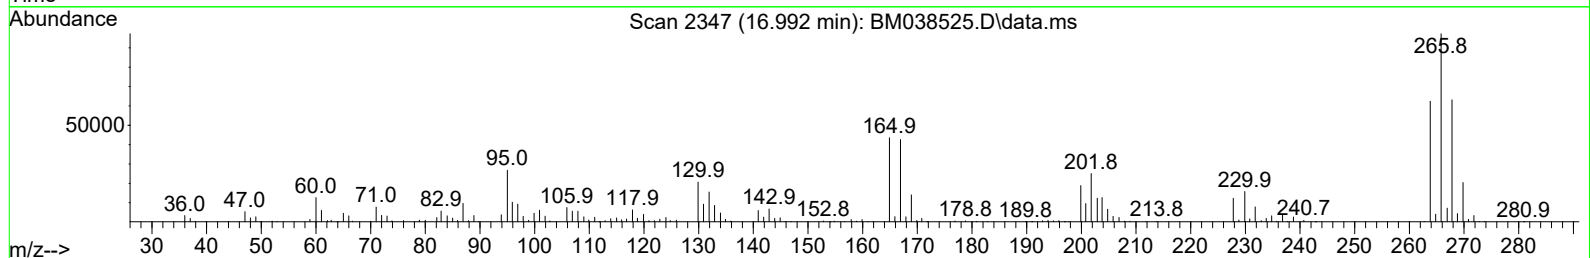


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038525.D
Acq On : 25 Jan 2023 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 03:27:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 21 01:21:49 2023
Response via : Initial Calibration

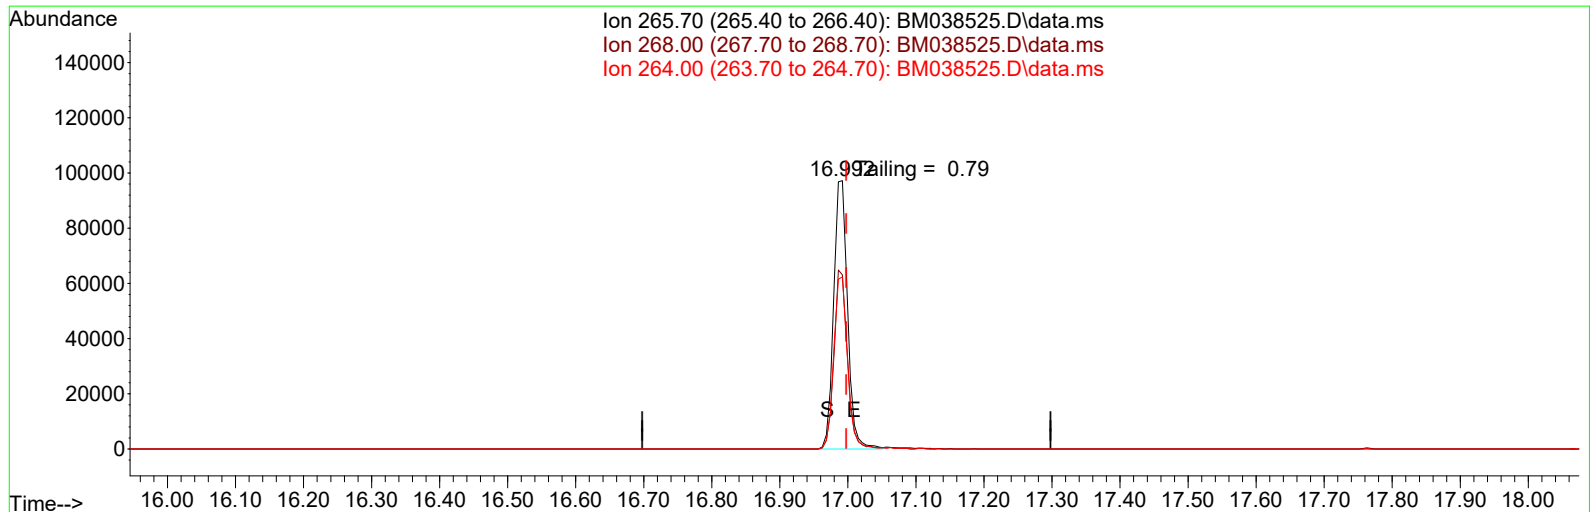

TIC: BM038525.D\data.ms

(70) Pentachlorophenol (C)




16.992min (-0.006) 0.00 ng

response 139160

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.88
264.00	61.70	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
 Data File : BM038525.D
 Acq On : 25 Jan 2023 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 26 03:27:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 21 01:21:49 2023
 Response via : Initial Calibration

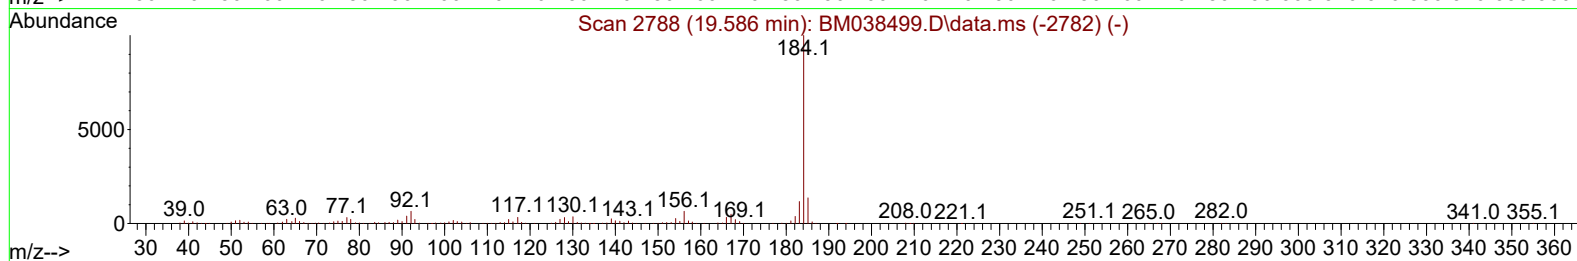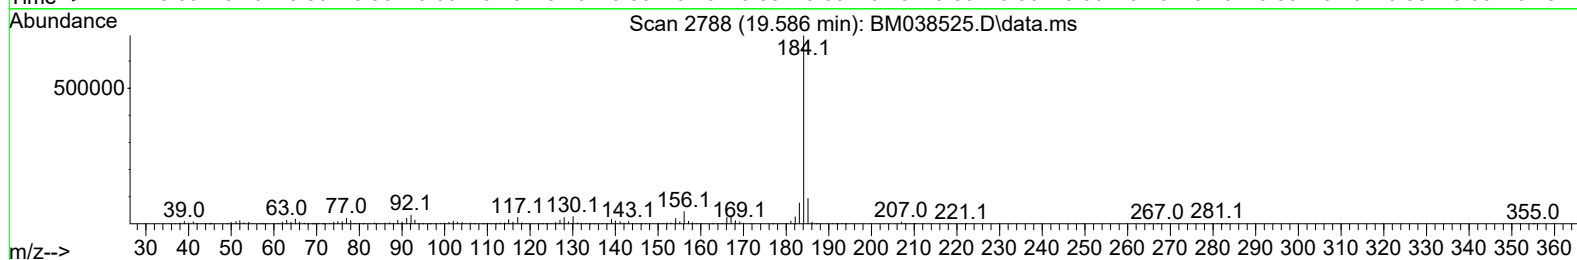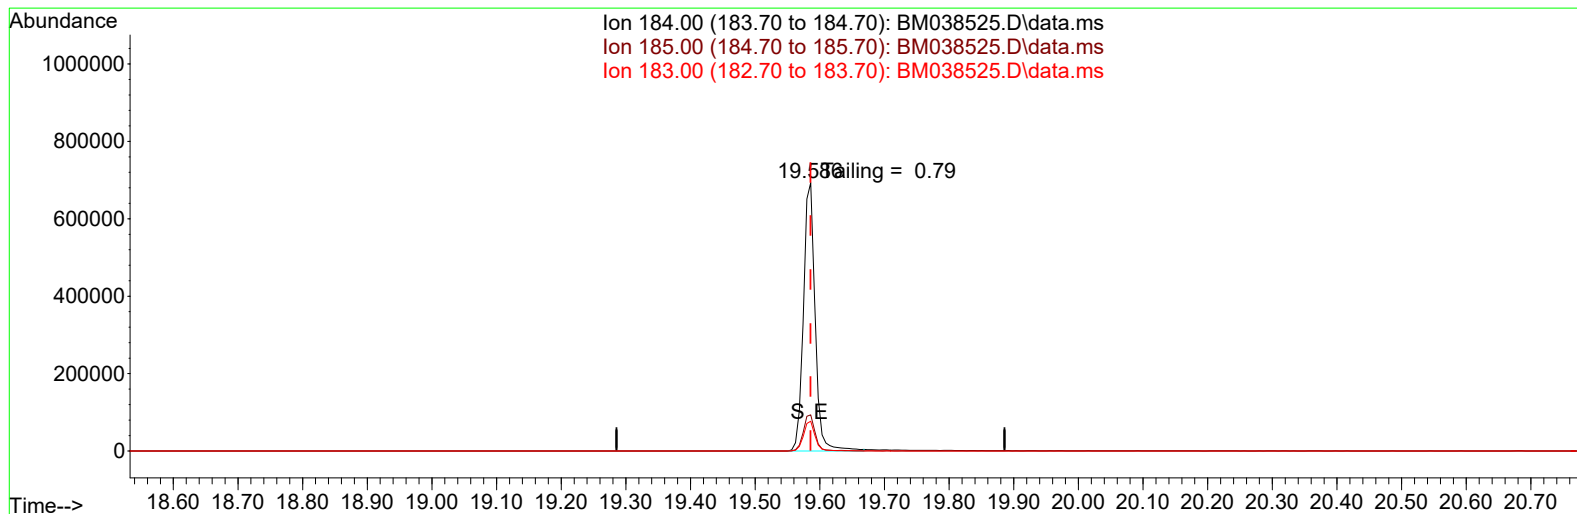

TIC: BM038525.D\data.ms

(77) Benzidine**19.586min (+ 0.000) 720025.19 ng****response 886020**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.47
183.00	11.60	11.11
0.00	0.00	0.00