

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
 Data File : BM038527.D
 Acq On : 25 Jan 2023 11:36
 Operator : CG/JU
 Sample : PB150219BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150219BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038527.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	311	317	326	rBV	770981	1032338	25.75%	4.285%
2	5.522	390	397	413	rBV	2115828	2987043	74.52%	12.400%
3	7.134	662	671	683	rBV	1955304	2959738	73.84%	12.287%
4	7.963	806	812	823	rBV	400101	619300	15.45%	2.571%
5	9.139	1003	1012	1025	rBV	1105125	1756342	43.82%	7.291%
6	10.775	1283	1290	1299	rBV	445945	733265	18.29%	3.044%
7	13.227	1700	1707	1719	rBV	2914977	3922950	97.87%	16.285%
8	14.598	1934	1940	1953	rVB	634596	886978	22.13%	3.682%
9	16.086	2187	2193	2208	rBV	2007600	2695725	67.25%	11.191%
10	17.339	2400	2406	2417	rBV	693702	921563	22.99%	3.826%
11	19.956	2845	2851	2859	rBV	3376453	4008525	100.00%	16.640%
12	21.515	3111	3116	3123	rBV	637591	788275	19.66%	3.272%
13	23.927	3520	3526	3538	rBV2	401580	777115	19.39%	3.226%




Sum of corrected areas: 24089157

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038527.D
Acq On : 25 Jan 2023 11:36
Operator : CG/JU
Sample : PB150219BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150219BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

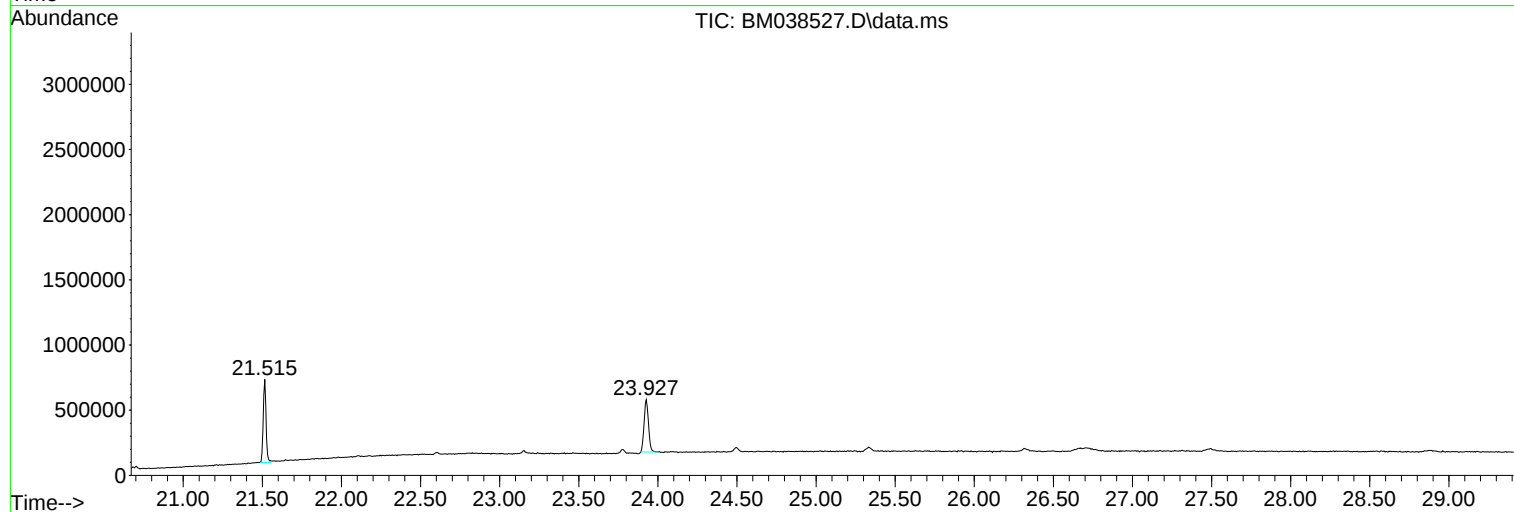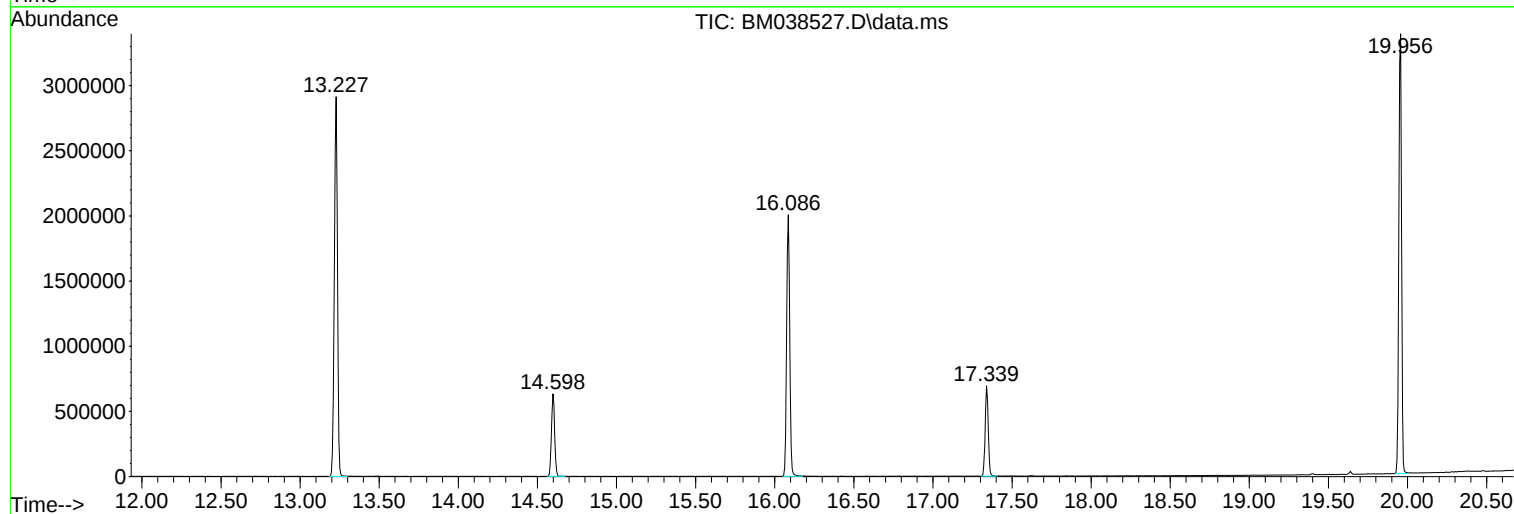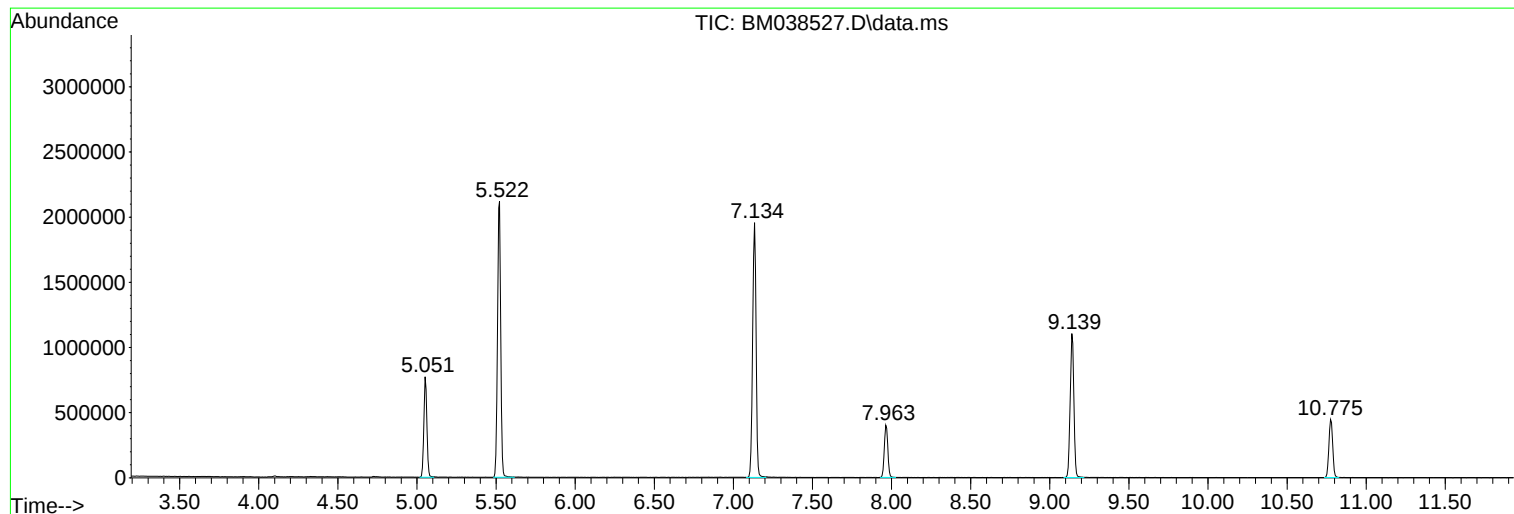

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038527.D
Acq On : 25 Jan 2023 11:36
Operator : CG/JU
Sample : PB150219BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150219BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.051	33.34 ng	1032340	1,4-Dichlorobenzene-d4	7.963

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

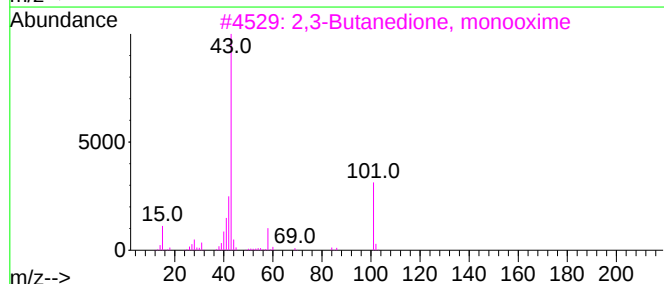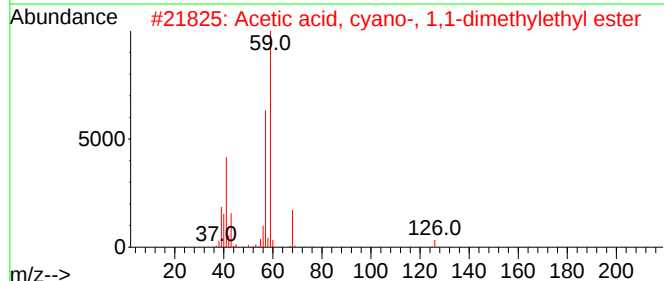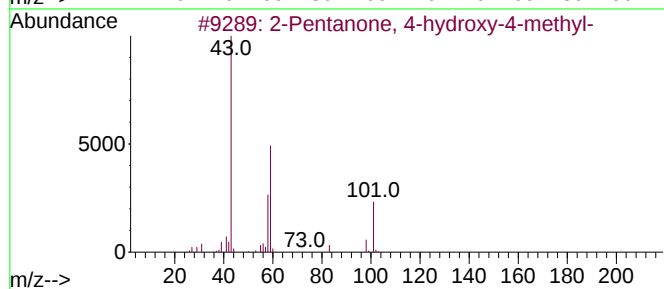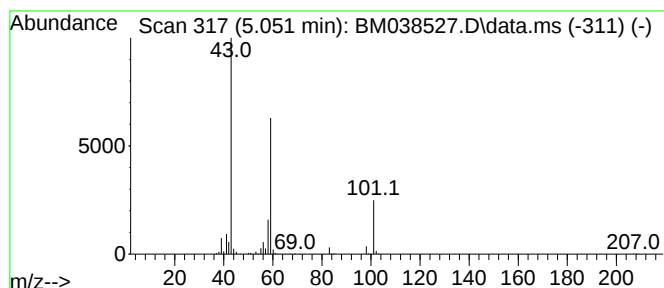

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038527.D
Acq On : 25 Jan 2023 11:36
Operator : CG/JU
Sample : PB150219BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150219BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.051	33.3	ng	1032340	1	7.963	619300	20.0