

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
 Data File : BM038532.D
 Acq On : 25 Jan 2023 15:22
 Operator : CG/JU
 Sample : PB150220BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB150220BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM038532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.052	311	317	328	rBV	501427	686885	24.34%	4.368%
2	5.516	390	396	411	rBV	1442913	1938305	68.68%	12.325%
3	7.128	663	670	681	rBV	1241614	1866798	66.15%	11.871%
4	7.963	805	812	822	rBV	277884	425960	15.09%	2.709%
5	9.139	1004	1012	1029	rBV	663202	1055046	37.39%	6.709%
6	10.775	1283	1290	1300	rBV	286752	464755	16.47%	2.955%
7	13.227	1700	1707	1716	rBV	1582946	2187736	77.52%	13.911%
8	14.598	1934	1940	1950	rBV	390685	531754	18.84%	3.381%
9	16.086	2187	2193	2205	rBV	1182868	1560609	55.30%	9.924%
10	17.339	2400	2406	2413	rBV	437826	569568	20.18%	3.622%
11	19.951	2845	2850	2860	rBV	2436422	2822058	100.00%	17.945%
12	21.515	3111	3116	3124	rBV	572188	708579	25.11%	4.506%
13	23.927	3520	3526	3535	rBV2	461337	908109	32.18%	5.775%




Sum of corrected areas: 15726162

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038532.D
Acq On : 25 Jan 2023 15:22
Operator : CG/JU
Sample : PB150220BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

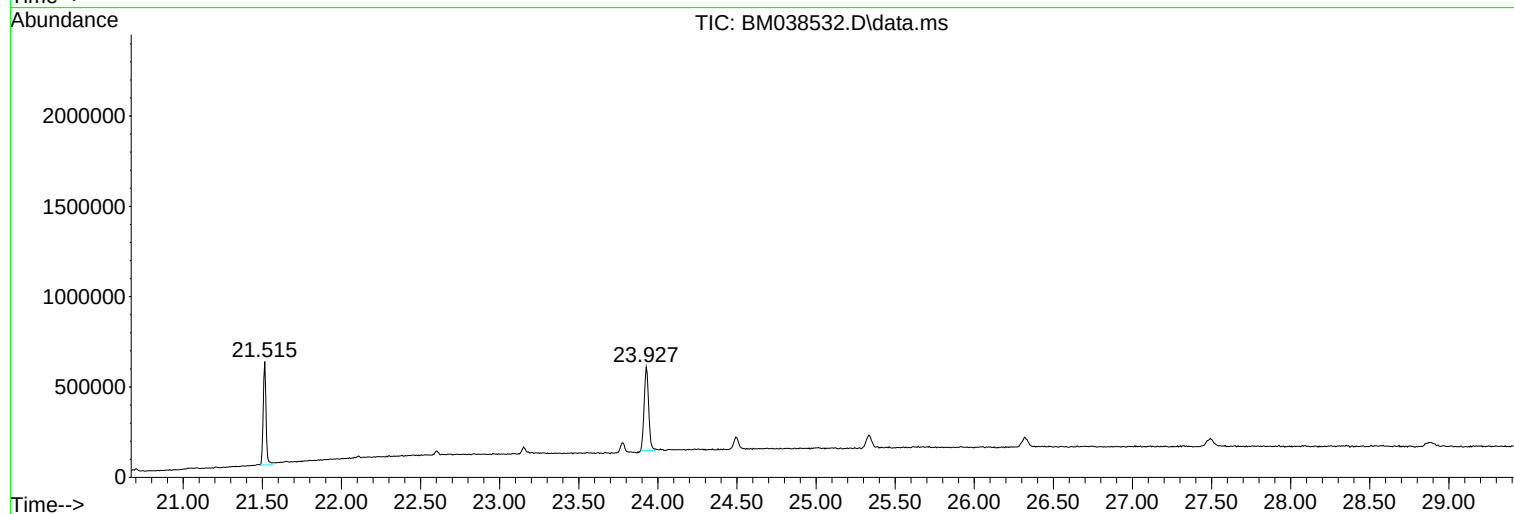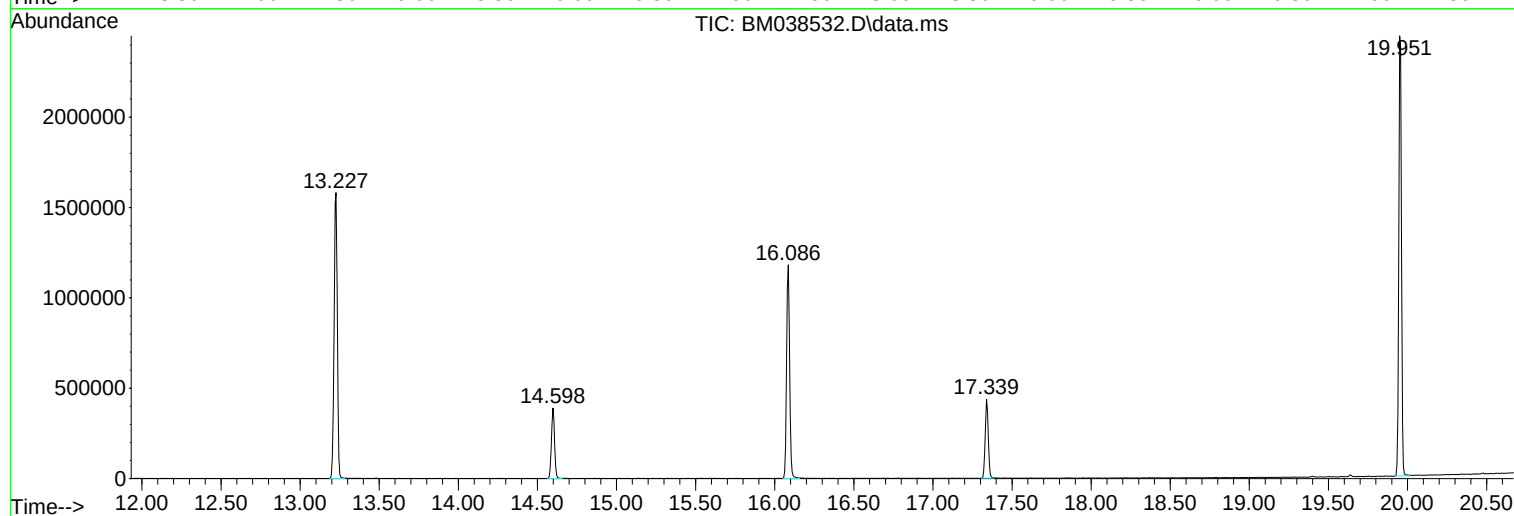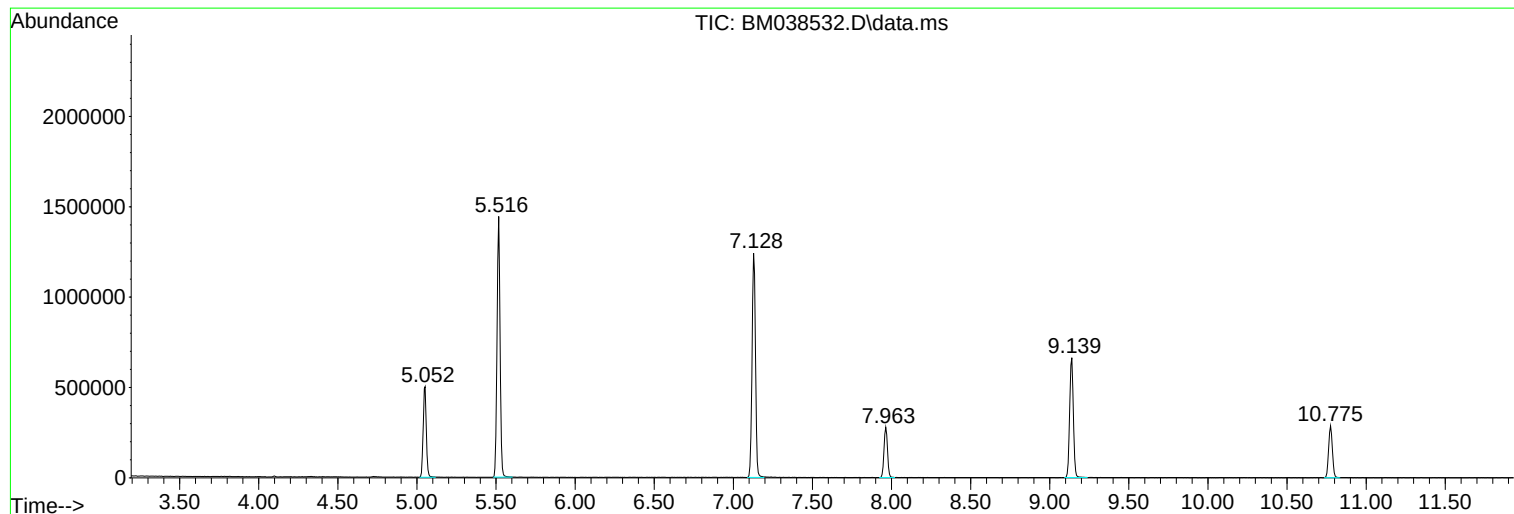

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038532.D
Acq On : 25 Jan 2023 15:22
Operator : CG/JU
Sample : PB150220BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150220BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.052	32.25 ng	686885	1,4-Dichlorobenzene-d4	7.963

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2		2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	17
3		1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
4		5-Hexen-2-one	98	C6H10O	000109-49-9	9
5		Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9

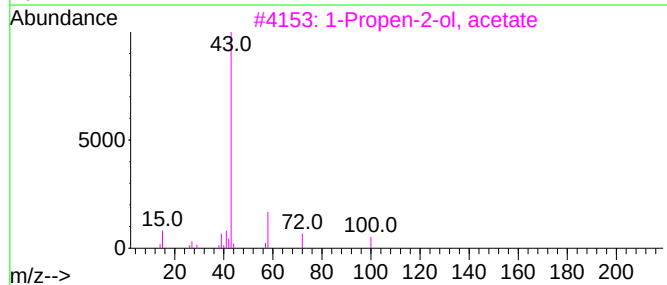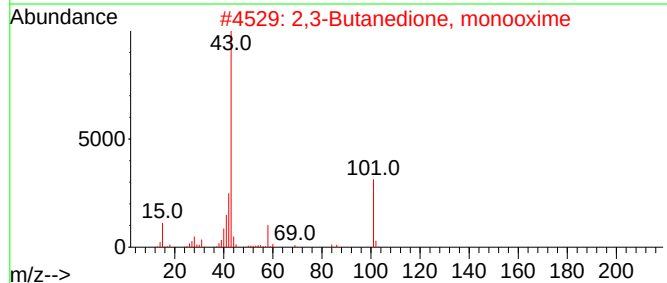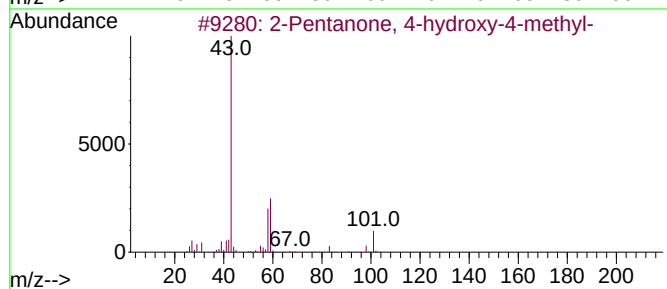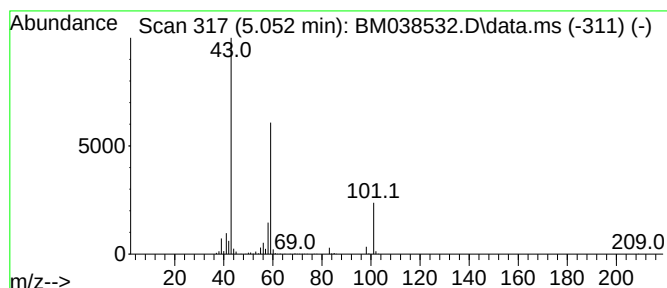

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038532.D
Acq On : 25 Jan 2023 15:22
Operator : CG/JU
Sample : PB150220BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB150220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.052	32.3	ng	686885	1	7.963	425960	20.0