


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038525.D
Acq On : 25 Jan 2023 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jan 21 01:21:49 2023

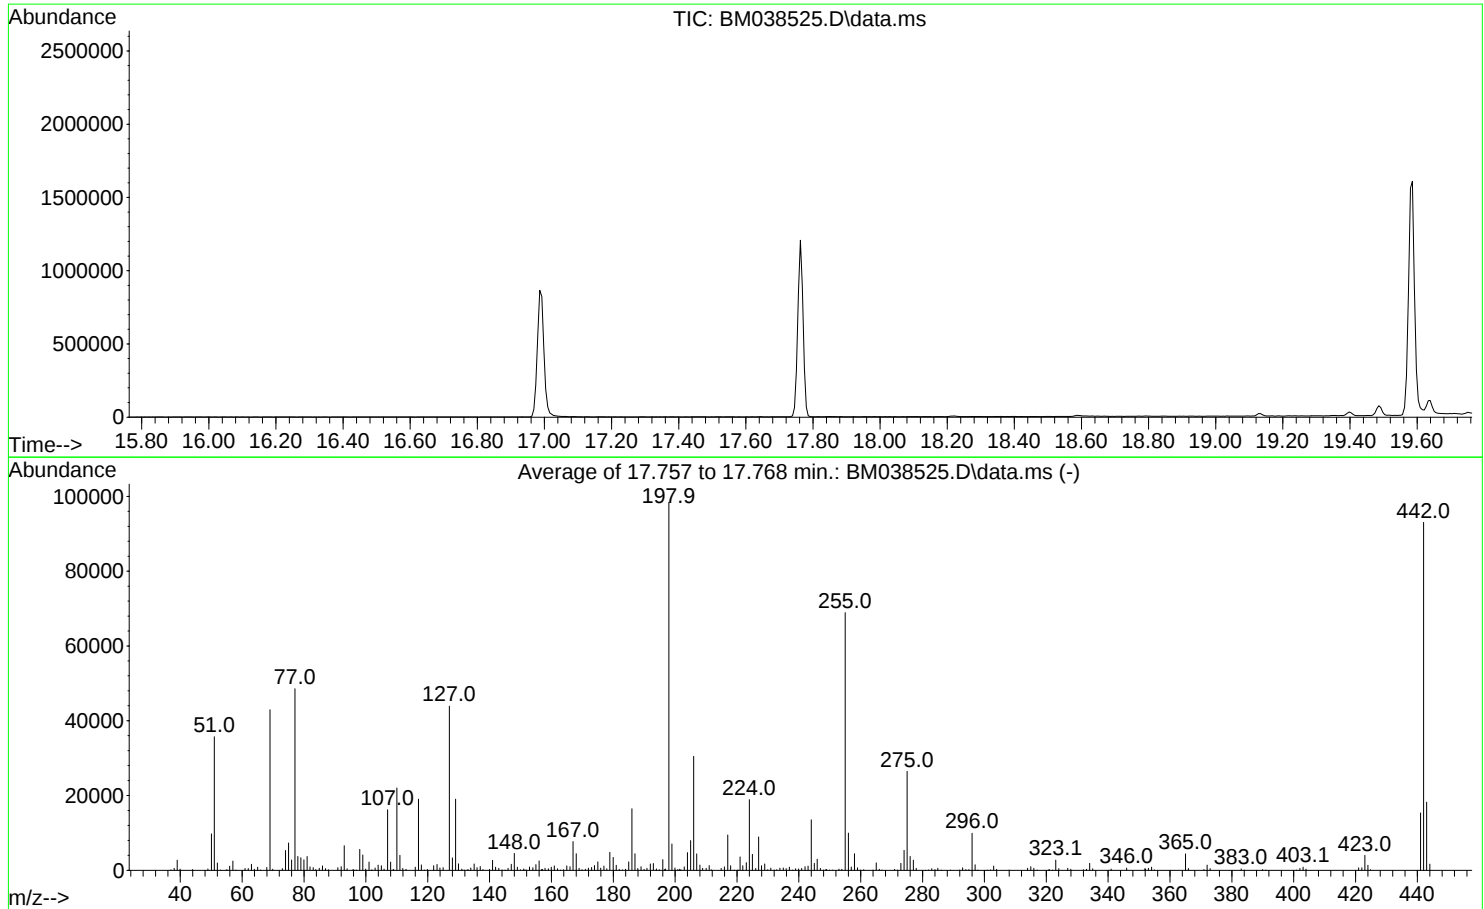




AutoFind: Scans 2477, 2478, 2479; Background Corrected with Scan 2471

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.3	35725	PASS
68	69	0.00	2	1.7	742	PASS
69	198	0.00	100	43.6	42944	PASS
70	69	0.00	2	0.6	277	PASS
127	198	10	80	44.6	43880	PASS
197	198	0.00	2	0.4	379	PASS
198	198	100	100	100.0	98389	PASS
199	198	5	9	7.1	7029	PASS
275	198	10	60	26.9	26485	PASS
365	198	1	100	4.5	4396	PASS
441	198	0.01	100	15.6	15328	PASS
442	442	50	100	100.0	93056	PASS
443	442	15	24	19.6	18195	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
 Data File : BM038525.D
 Acq On : 25 Jan 2023 10:23
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Jan 26 03:27:35 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Jan 21 01:21:49 2023
 Response via : Initial Calibration

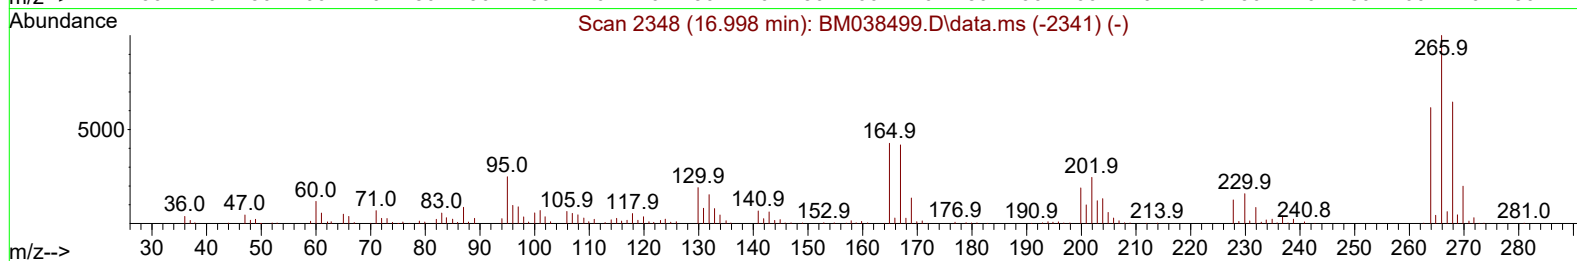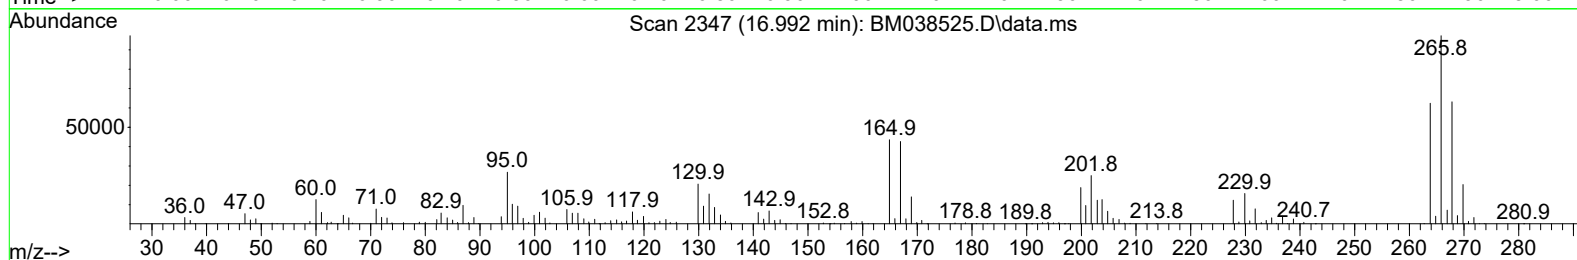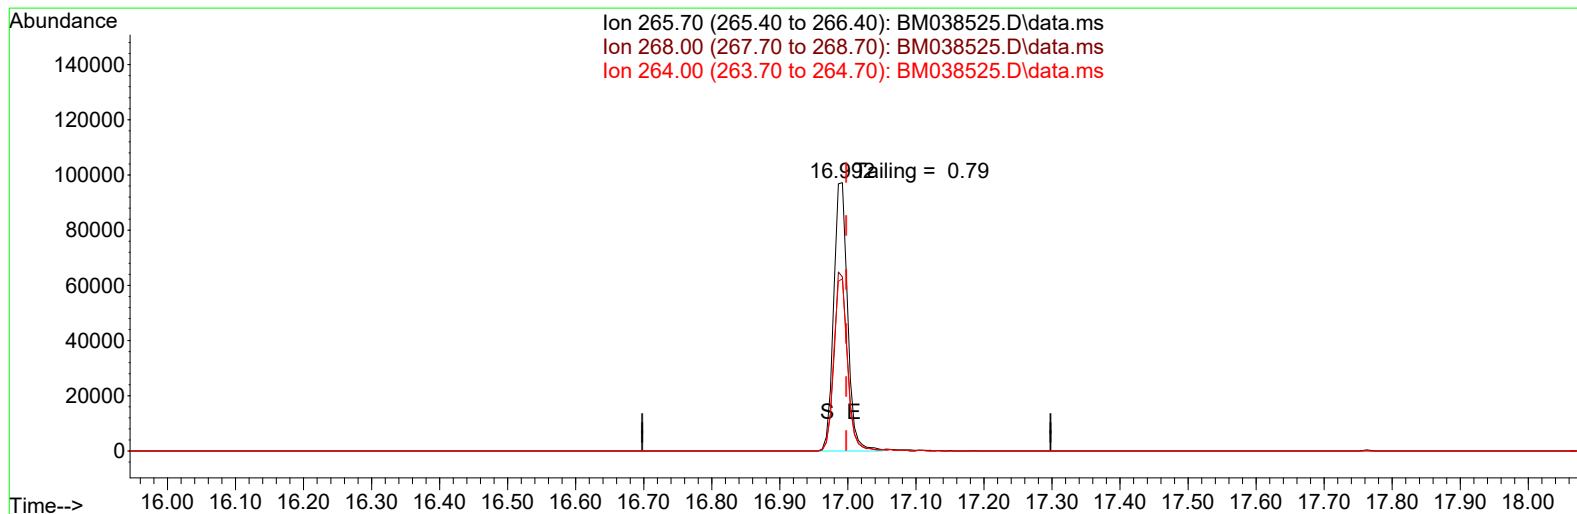

TIC: BM038525.D\data.ms

(70) Pentachlorophenol (C)

16.992min (-0.006) 0.00 ng




response 139160

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.60	64.88
264.00	61.70	64.14
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012523\
Data File : BM038525.D
Acq On : 25 Jan 2023 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Jan 26 03:27:35 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM012023.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Jan 21 01:21:49 2023
Response via : Initial Calibration

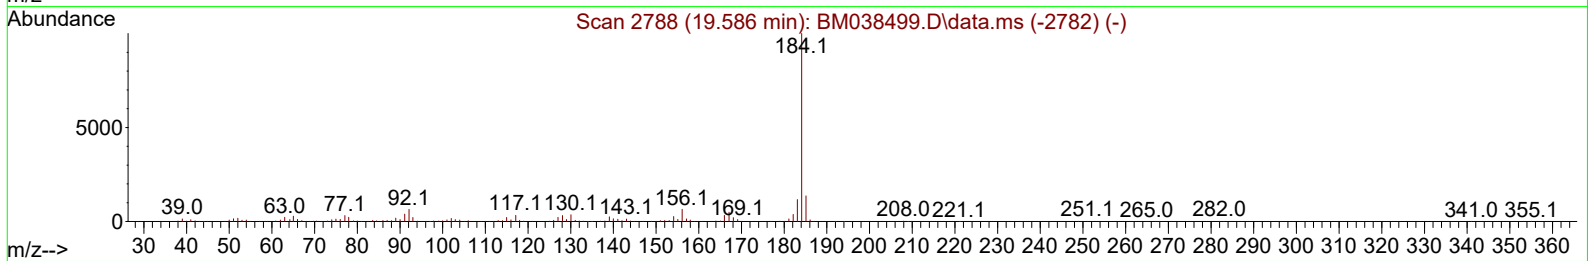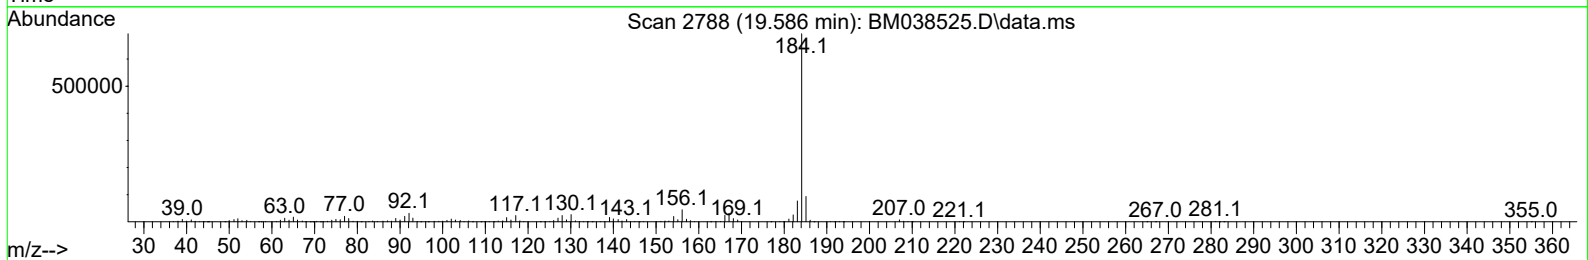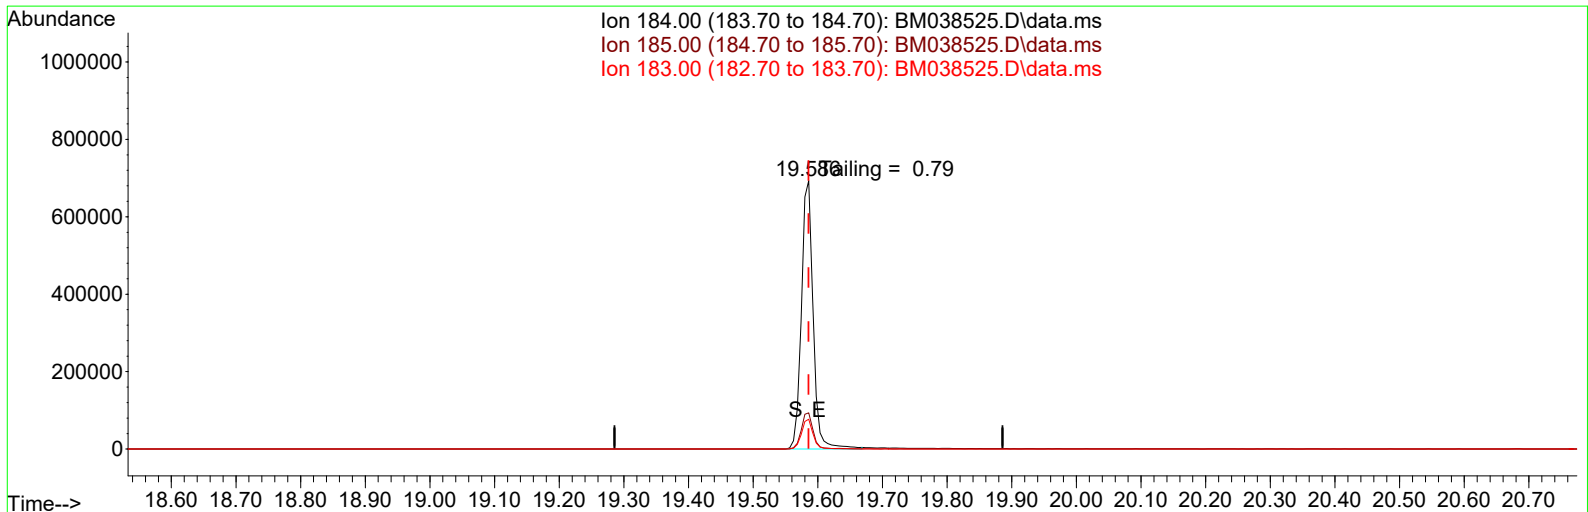

TIC: BM038525.D\data.ms

(77) Benzidine

19.586min (+ 0.000) 720025.19 ng

response 886020

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.60	13.47
183.00	11.60	11.11
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
1/25/2023	BNA_M	<u>BM038525.D</u>
Compound Name	Response	Retention Time
DDT	505790	20.803
DDD	5645	20.415
DDE	0	19.856
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5645	511435	1.10

Instrument :
BNA_M
ClientSampleId :
DFTPP