

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
 Data File : BM033872.D
 Acq On : 26 Jan 2022 16:13
 Operator : CG/JU
 Sample : N1230-05
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q51

Quant Time: Jan 27 01:41:52 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.943	152	1975	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	7231	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.576	164	4230	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	8269	0.400	ng/ul	0.00
17) Chrysene-d12	21.480	240	6428	0.400	ng/ul	# 0.00
23) Perylene-d12	23.875	264	6915	0.400	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	9170	4.441	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.344	152	3466	0.348	ng/ul	0.00
18) Fluoranthene-d10	19.334	212	8348	0.422	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.969	266	309	0.081	ng/ul	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
Data File : BM033872.D
Acq On : 26 Jan 2022 16:13
Operator : CG/JU
Sample : N1230-05
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q51


Quant Time: Jan 27 01:41:52 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

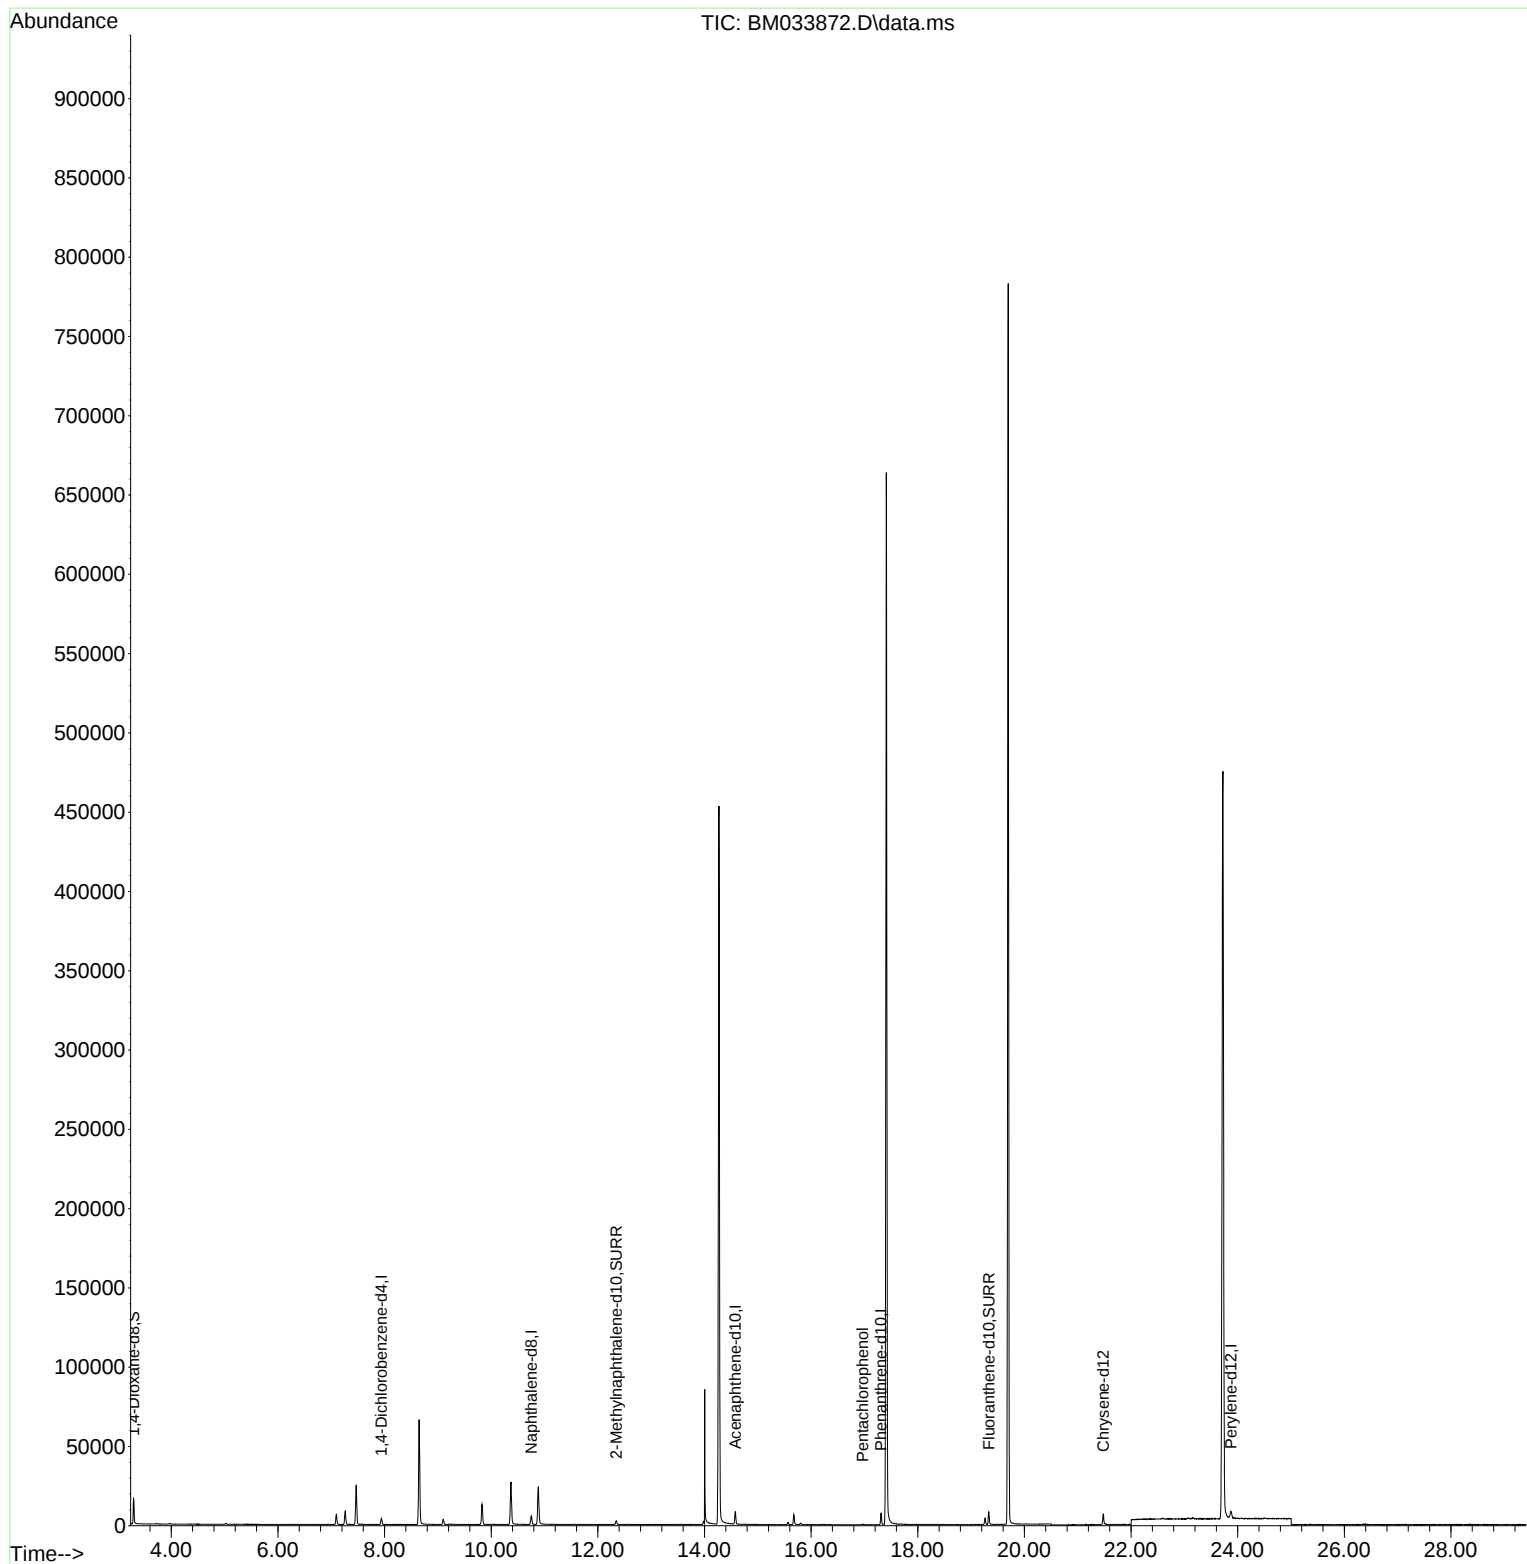

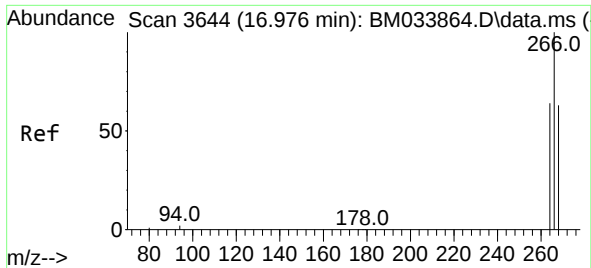

#14
 Pentachlorophenol
 Concen: 0.081 ng/ul
 RT: 16.969 min Scan# 309
 Delta R.T. -0.004 min
 Lab File: BM033872.D
 Acq: 26 Jan 2022 16:13

Instrument :
 BNA_M
 ClientSampleId :
 C0Q51

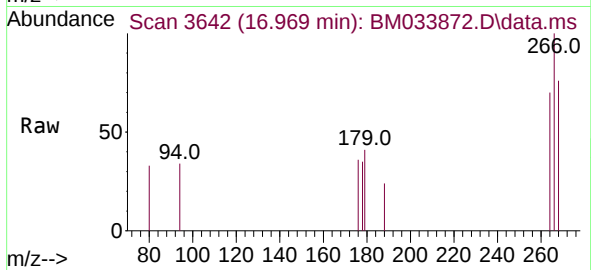

Tgt Ion:	266	Resp:	309
Ion	Ratio	Lower	Upper
266	100		
264	58.6	51.4	77.0
268	58.6	53.1	79.7

