

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
 Data File : BM033875.D
 Acq On : 26 Jan 2022 18:00
 Operator : CG/JU
 Sample : N1230-07
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q20

Quant Time: Jan 27 01:42:24 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.939	152	1717	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136	6245	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.576	164	3705	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	7336	0.400	ng/ul	0.00
17) Chrysene-d12	21.478	240	6000	0.400	ng/ul #	0.00
23) Perylene-d12	23.871	264	7000	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	9294	5.178	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	3469	0.403	ng/ul	0.00
18) Fluoranthene-d10	19.330	212	8401	0.455	ng/ul	0.00
Target Compounds						
					Qvalue	
5) Naphthalene	10.801	128	780	0.045	ng/ul#	81
14) Pentachlorophenol	16.962	266	14663	4.350	ng/ul	97
20) Pyrene	19.723	202	793	0.028	ng/ul#	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
Data File : BM033875.D
Acq On : 26 Jan 2022 18:00
Operator : CG/JU
Sample : N1230-07
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q20

Quant Time: Jan 27 01:42:24 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration




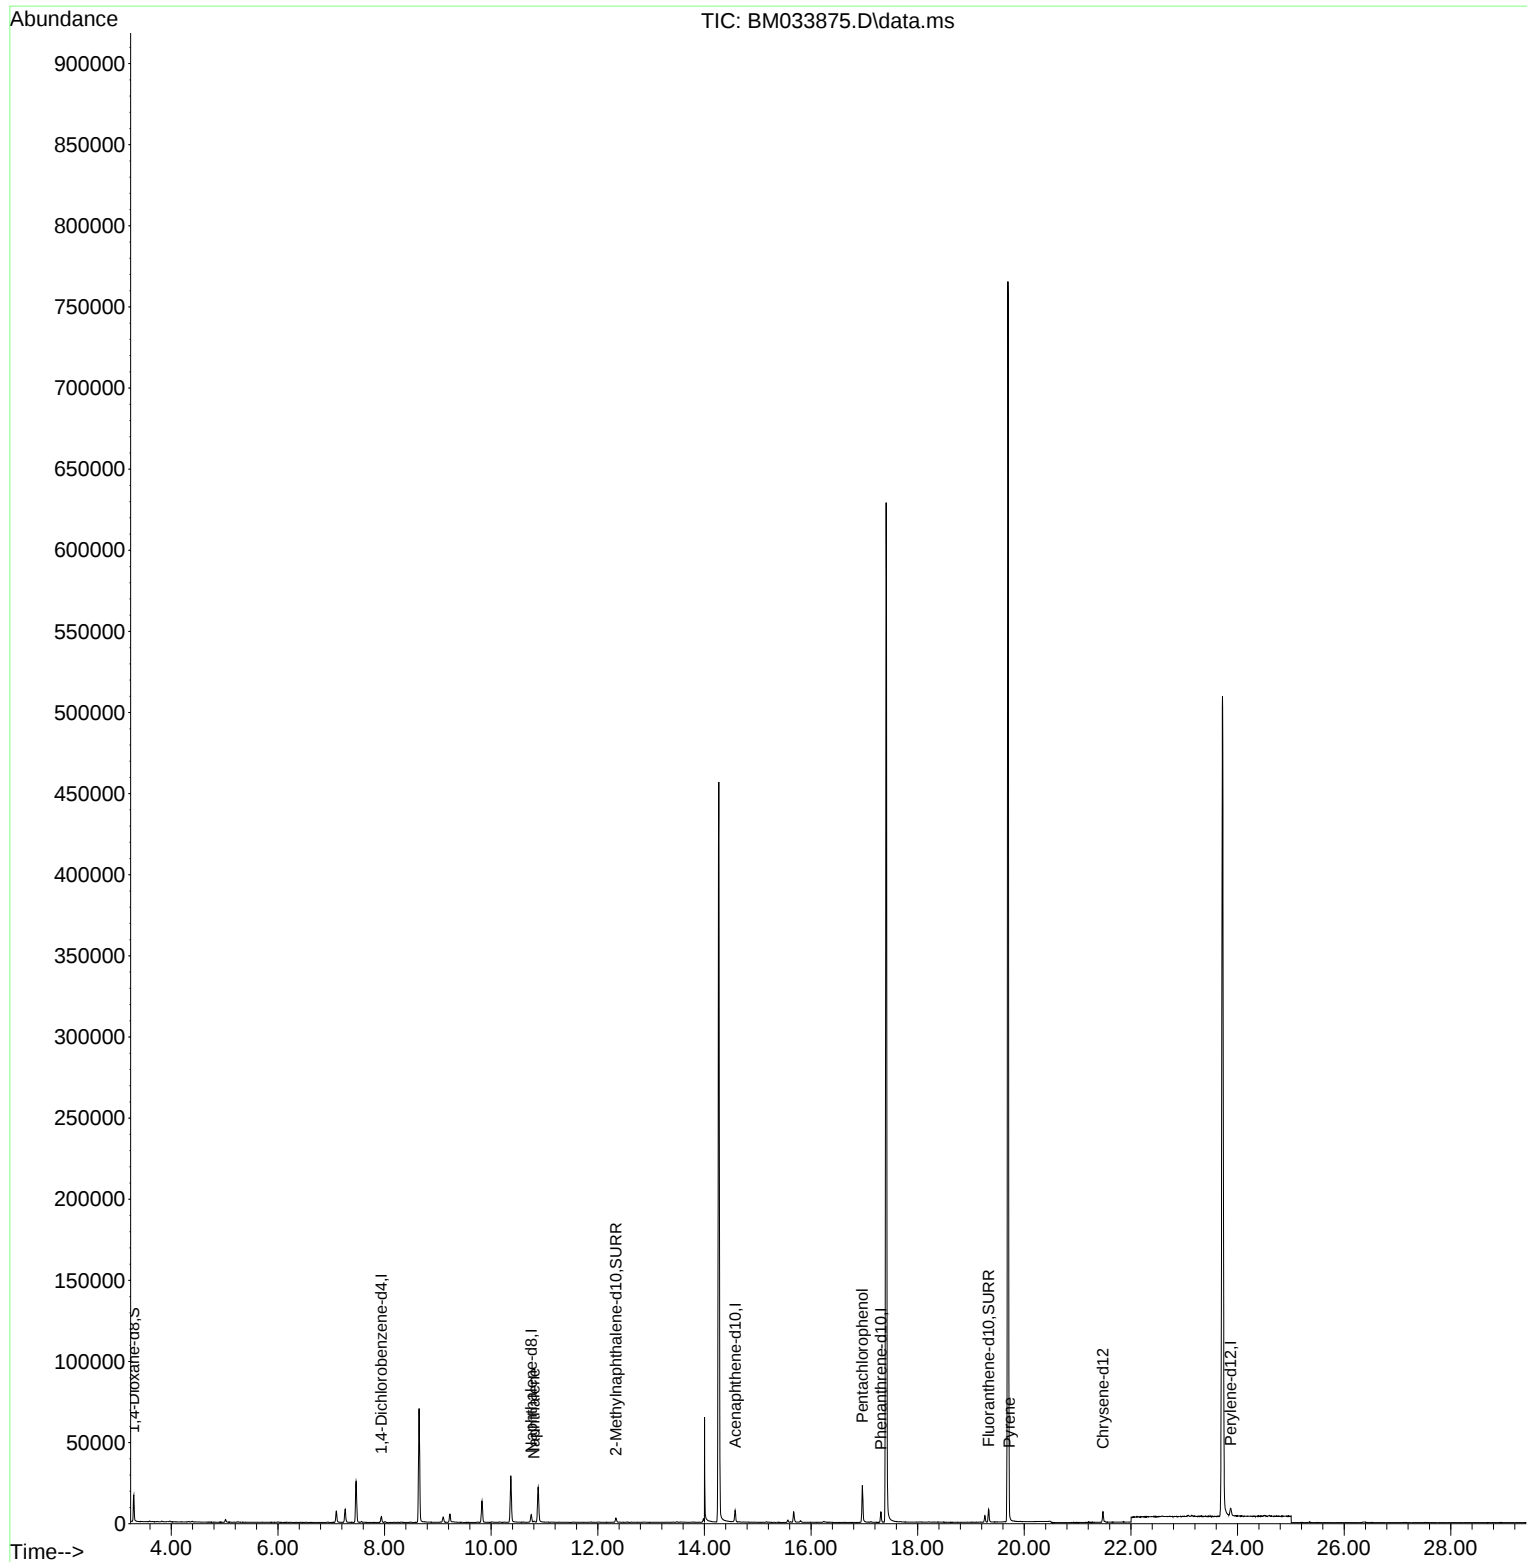


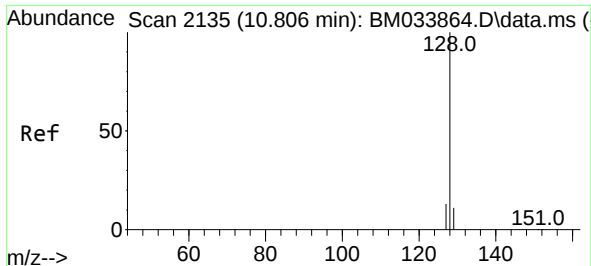

#5
Naphthalene
Concen: 0.045 ng/ul
RT: 10.801 min Scan# 2134
Delta R.T. -0.004 min
Lab File: BM033875.D
Acq: 26 Jan 2022 18:00




Instrument :
BNA_M
ClientSampleId :
C0Q20


Tgt Ion:128 Resp: 780
Ion Ratio Lower Upper
128 100
129 28.2 13.4 20.2#
127 24.6 15.2 22.8#

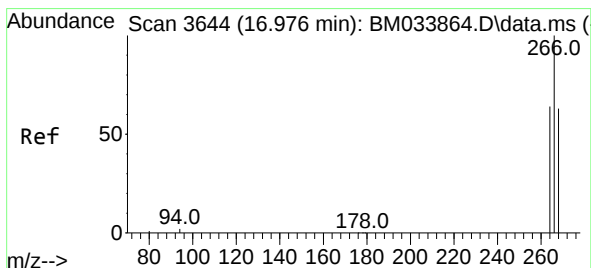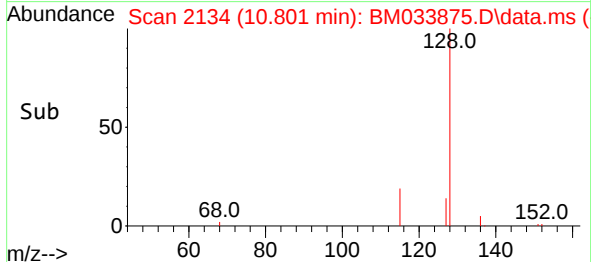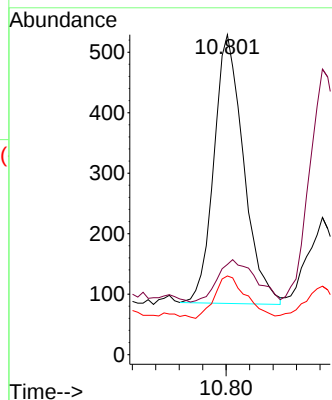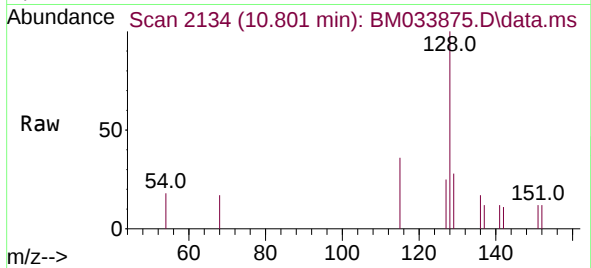

#14
Pentachlorophenol
Concen: 4.350 ng/ul
RT: 16.962 min Scan# 3640
Delta R.T. -0.010 min
Lab File: BM033875.D
Acq: 26 Jan 2022 18:00


Tgt Ion:266 Resp: 14663
Ion Ratio Lower Upper
266 100
264 62.7 51.4 77.0
268 63.4 53.1 79.7

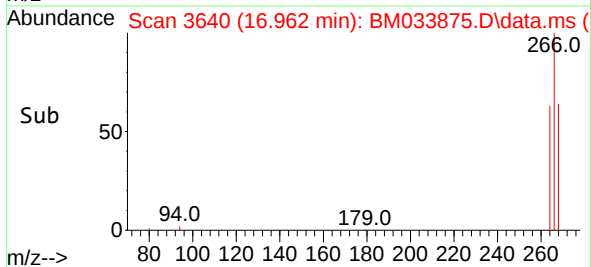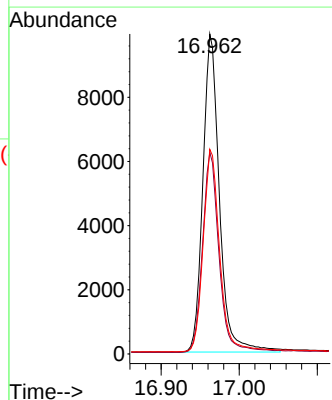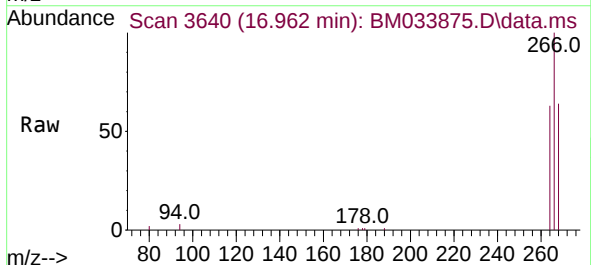

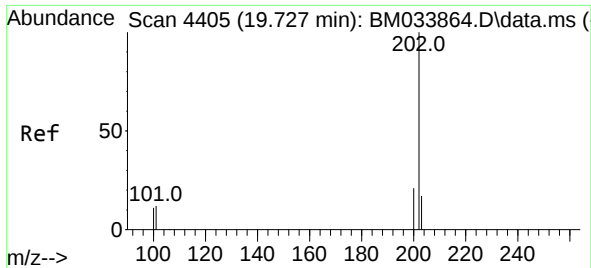

#20
 Pyrene
 Concen: 0.028 ng/ul
 RT: 19.723 min Scan# 44
 Delta R.T. -0.004 min
 Lab File: BM033875.D
 Acq: 26 Jan 2022 18:00

Instrument :
 BNA_M
 ClientSampleId :
 C0Q20

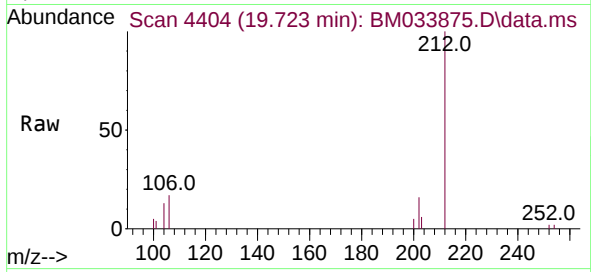

Tgt Ion:	202	Resp:	793
Ion	Ratio	Lower	Upper
202	100		
101	24.8	9.3	13.9#
100	29.2	7.8	11.6#

