

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
 Data File : BM033876.D
 Acq On : 26 Jan 2022 18:35
 Operator : CG/JU
 Sample : N1230-08
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q29

Quant Time: Jan 27 01:42:34 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.939	152	1489	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	5486	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.576	164	3309	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.313	188	6376	0.400	ng/ul	0.00
17) Chrysene-d12	21.477	240	5118	0.400	ng/ul #	0.00
23) Perylene-d12	23.873	264	5717	0.400	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	8711	5.596	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	3721	0.492	ng/ul	0.00
18) Fluoranthene-d10	19.330	212	7923	0.503	ng/ul	0.00
Target Compounds						Qvalue
2) 1,4-Dioxane	3.327	88	162	0.099	ng/ul#	75
14) Pentachlorophenol	16.966	266	1402	0.479	ng/ul	97
16) Anthracene	17.444	178	572	0.030	ng/ul#	74


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
Data File : BM033876.D
Acq On : 26 Jan 2022 18:35
Operator : CG/JU
Sample : N1230-08
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q29

Quant Time: Jan 27 01:42:34 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration




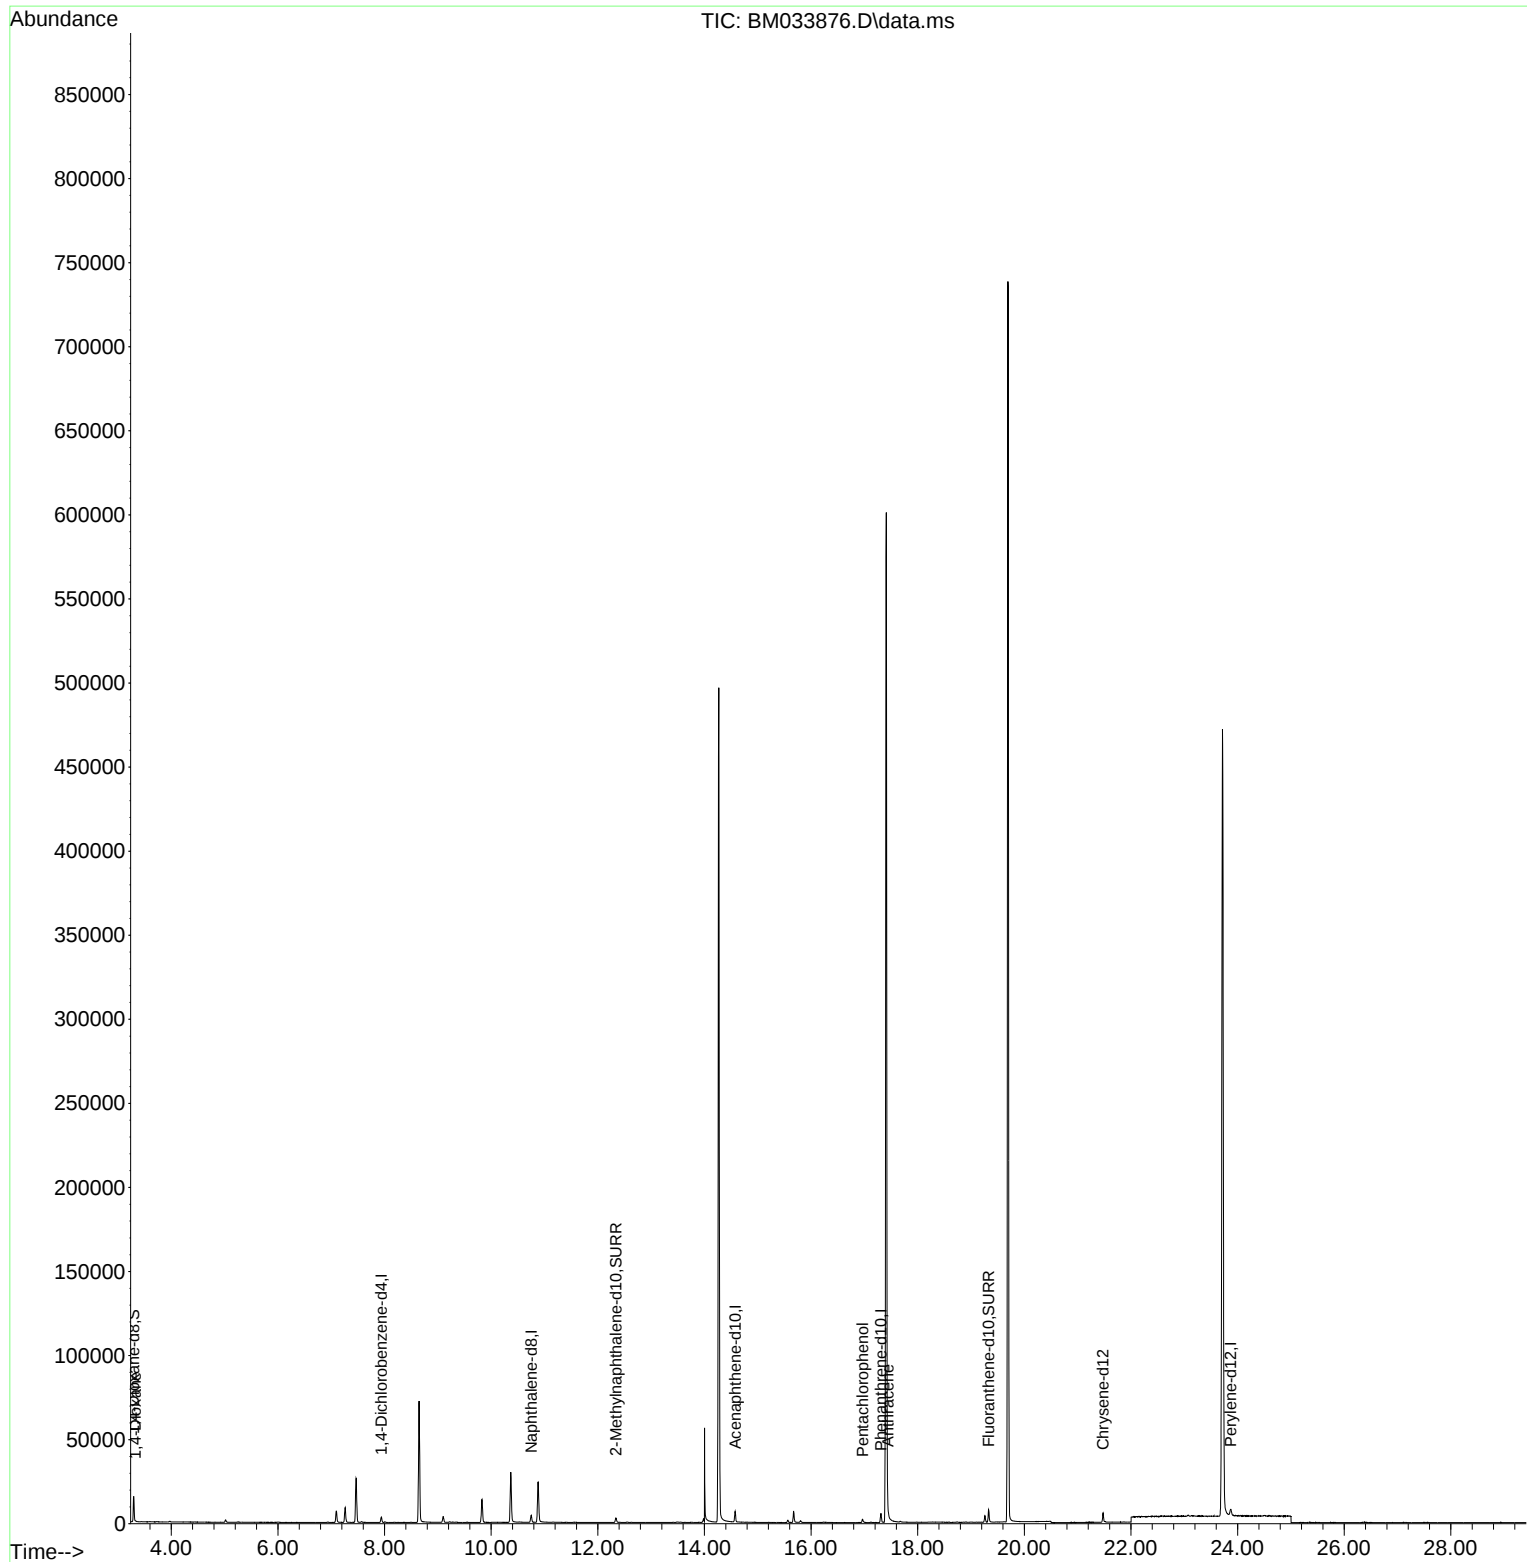


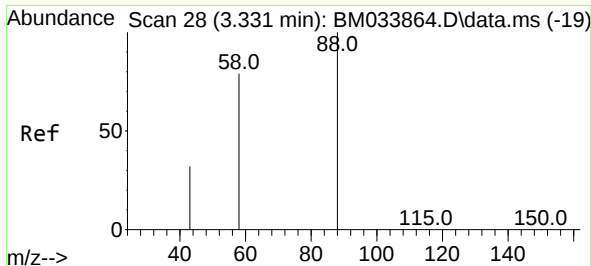

#2
1,4-Dioxane
Concen: 0.099 ng/ul
RT: 3.327 min Scan# 21
Delta R.T. -0.007 min
Lab File: BM033876.D
Acq: 26 Jan 2022 18:35




Instrument :
BNA_M
ClientSampleId :
C0Q29


Tgt Ion: 88 Resp: 162
Ion Ratio Lower Upper
88 100
43 56.9 49.7 74.5
58 32.2 52.5 78.7#

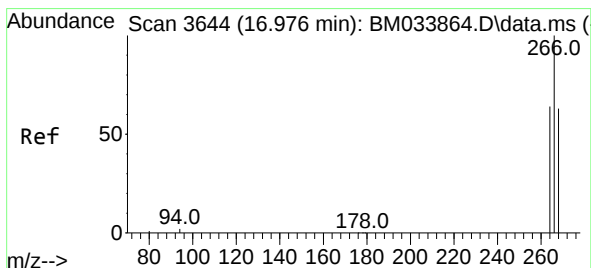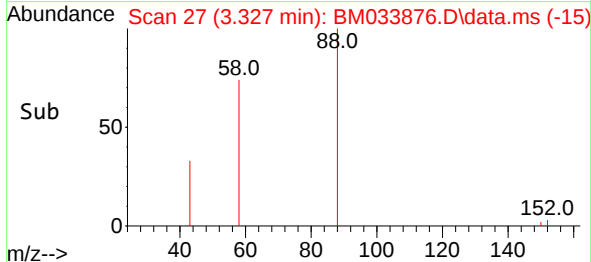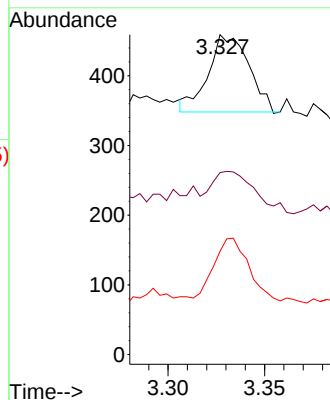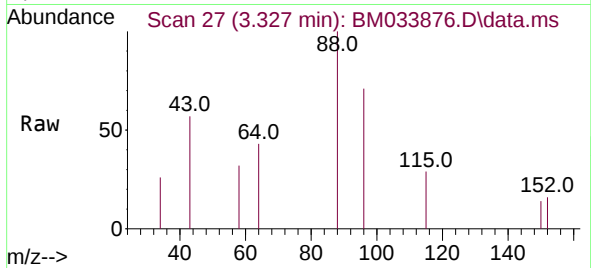

#14
Pentachlorophenol
Concen: 0.479 ng/ul
RT: 16.966 min Scan# 3641
Delta R.T. -0.007 min
Lab File: BM033876.D
Acq: 26 Jan 2022 18:35


Tgt Ion: 266 Resp: 1402
Ion Ratio Lower Upper
266 100
264 62.5 51.4 77.0
268 62.8 53.1 79.7

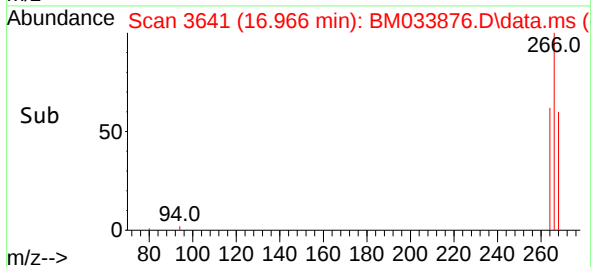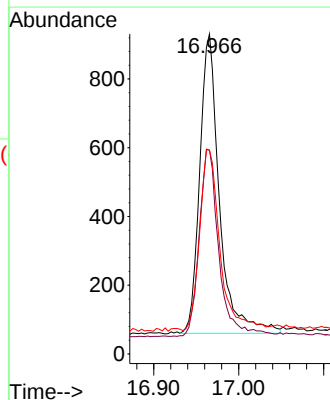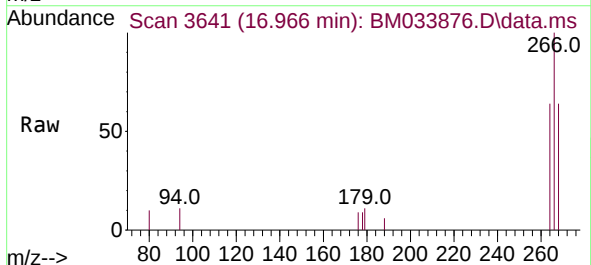

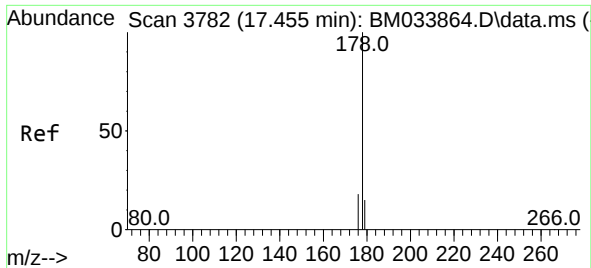

#16
 Anthracene
 Concen: 0.030 ng/ul
 RT: 17.444 min Scan# 31
 Delta R.T. -0.007 min
 Lab File: BM033876.D
 Acq: 26 Jan 2022 18:35

Instrument :
 BNA_M
 ClientSampleId :
 C0Q29

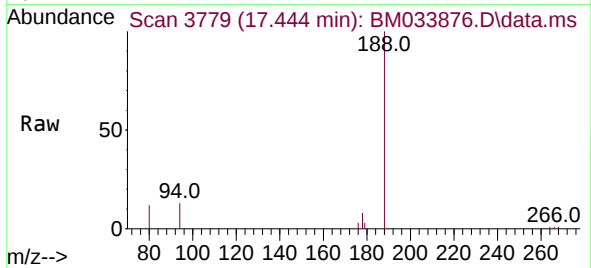

Tgt Ion:178 Resp: 572
 Ion Ratio Lower Upper
 178 100
 179 36.5 16.5 24.7#
 176 32.0 18.3 27.5#

