

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
 Data File : BM033883.D
 Acq On : 26 Jan 2022 23:19
 Operator : CG/JU
 Sample : N1230-17
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q06

Quant Time: Jan 27 02:12:40 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.939	152	1850	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	6589	0.400	ng/ul #	0.00
9) Acenaphthene-d10	14.576	164	3837	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	7434	0.400	ng/ul	-0.01
17) Chrysene-d12	21.472	240	5961	0.400	ng/ul #	-0.01
23) Perylene-d12	23.865	264	6465	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.296	96	9666	4.998	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	3390	0.373	ng/ul	0.00
18) Fluoranthene-d10	19.330	212	7704	0.420	ng/ul	0.00
Target Compounds						Qvalue
12) Fluorene	15.618	166	2541	0.162	ng/ul	99
14) Pentachlorophenol	16.962	266	105339	30.839	ng/ul	97
15) Phenanthrene	17.351	178	520	0.022	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
Data File : BM033883.D
Acq On : 26 Jan 2022 23:19
Operator : CG/JU
Sample : N1230-17
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q06

Quant Time: Jan 27 02:12:40 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration




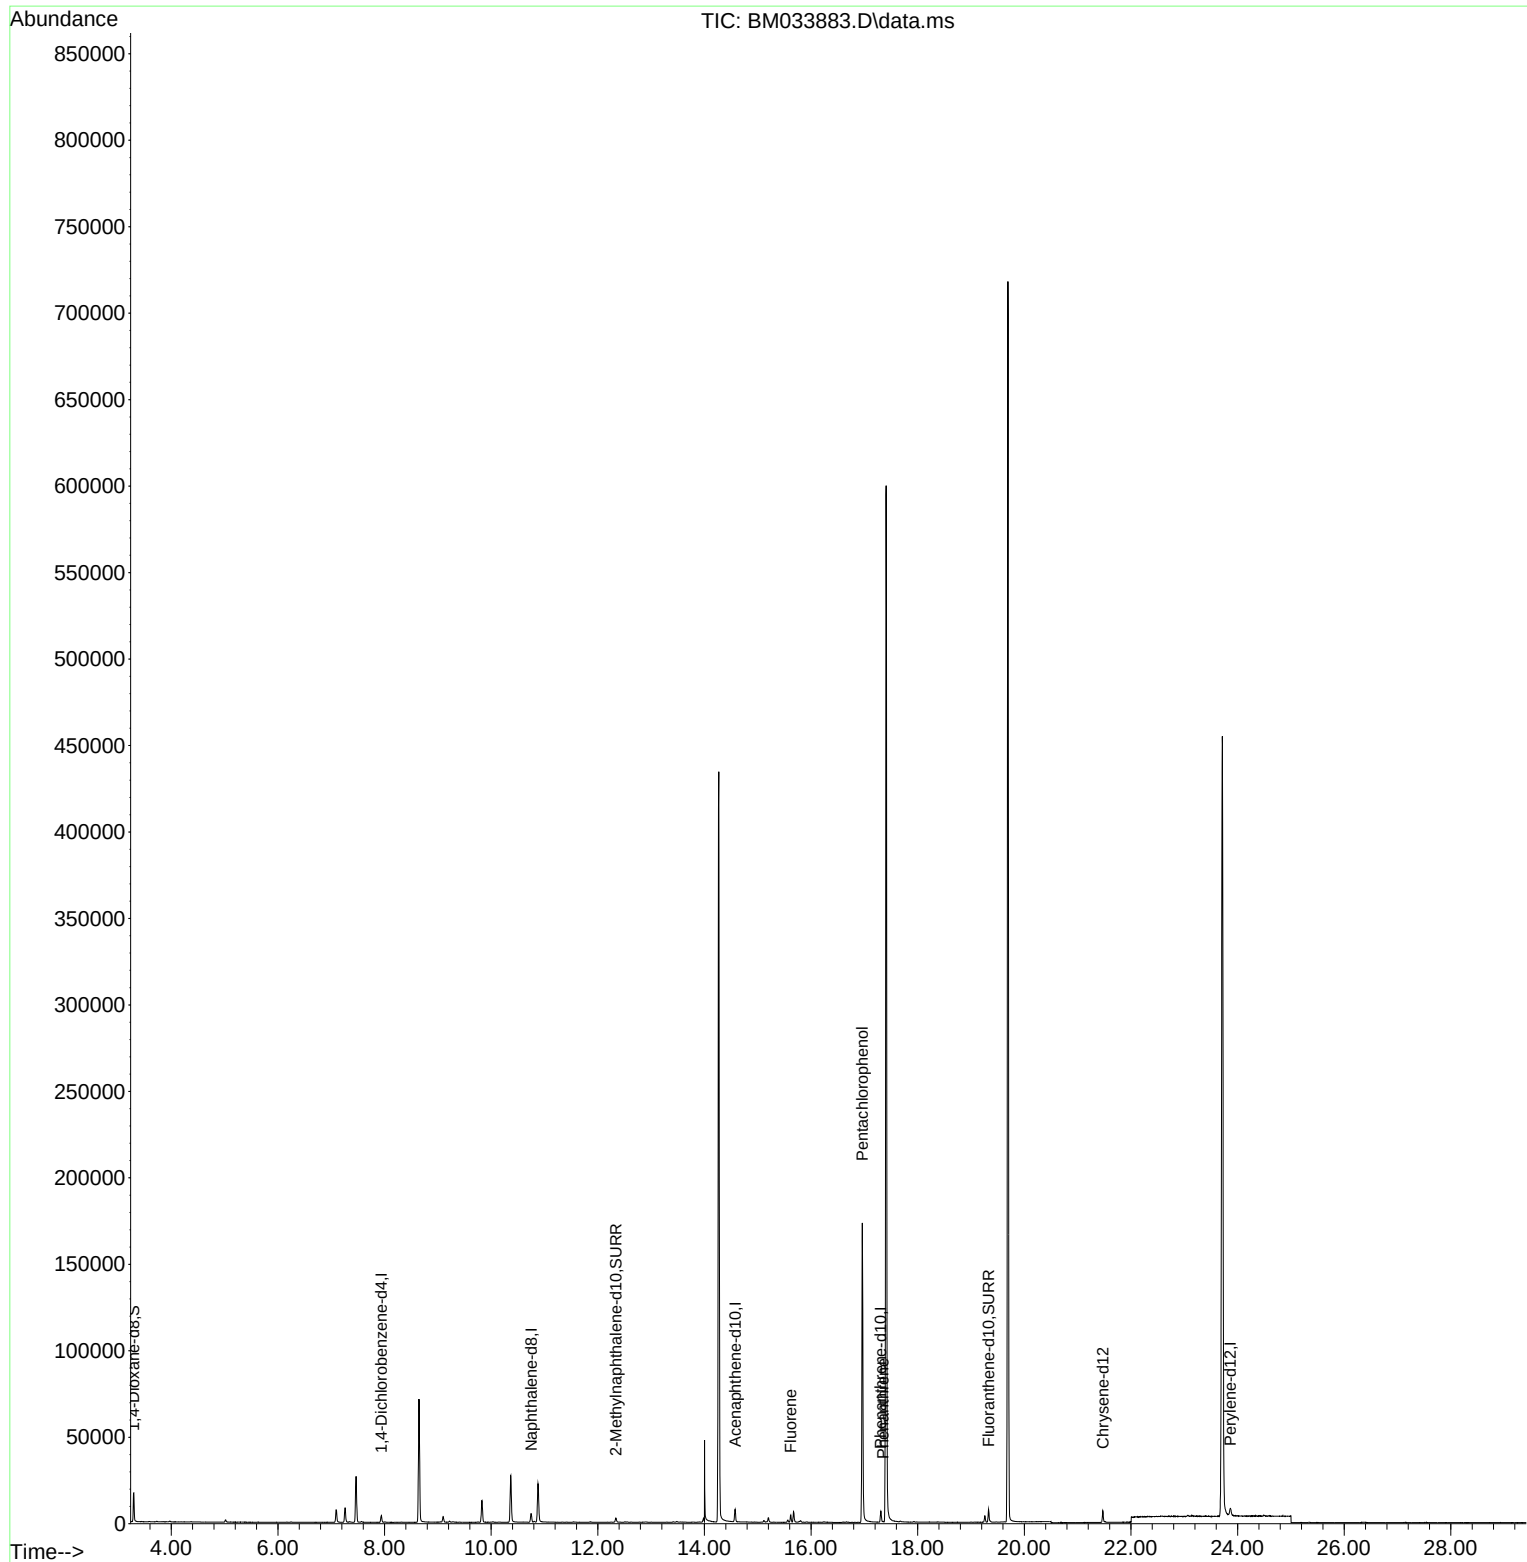


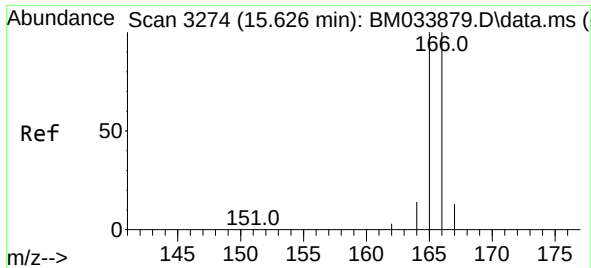

#12
Fluorene
Concen: 0.162 ng/ul
RT: 15.618 min Scan# 31
Delta R.T. -0.008 min
Lab File: BM033883.D
Acq: 26 Jan 2022 23:19




Instrument :
BNA_M
ClientSampleId :
C0Q06


Tgt Ion:166	Resp:	2541
Ion Ratio	Lower	Upper
166	100	
165	101.0	81.1 121.7
167	16.8	14.9 22.3

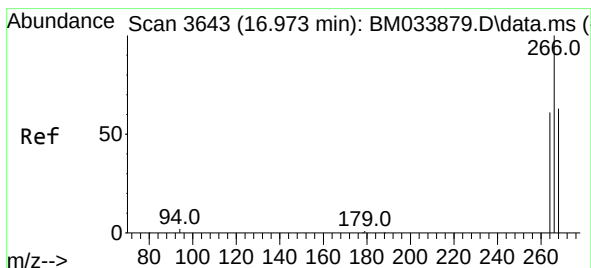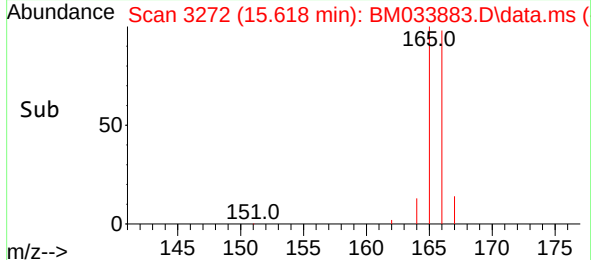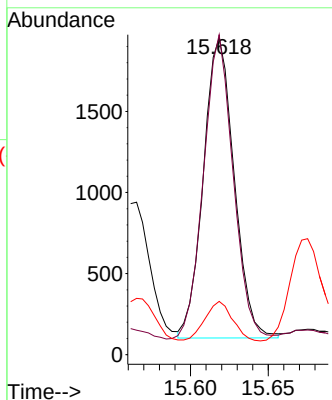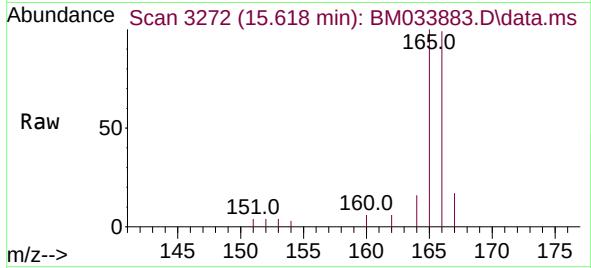

#14
Pentachlorophenol
Concen: 30.839 ng/ul
RT: 16.962 min Scan# 3640
Delta R.T. -0.011 min
Lab File: BM033883.D
Acq: 26 Jan 2022 23:19


Tgt Ion:266	Resp:	105339
Ion Ratio	Lower	Upper
266	100	
264	62.7	51.4 77.0
268	63.7	53.1 79.7

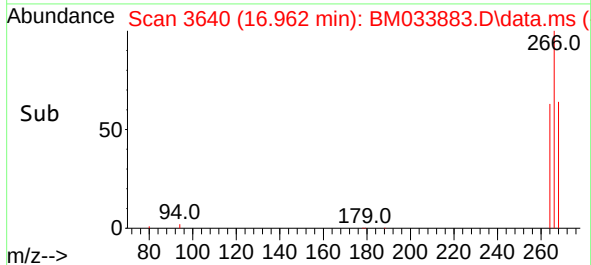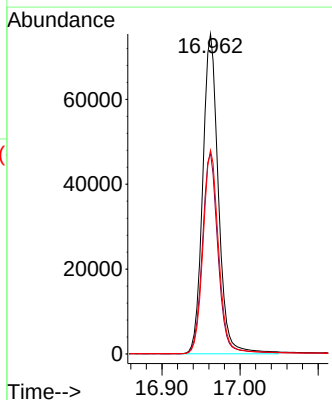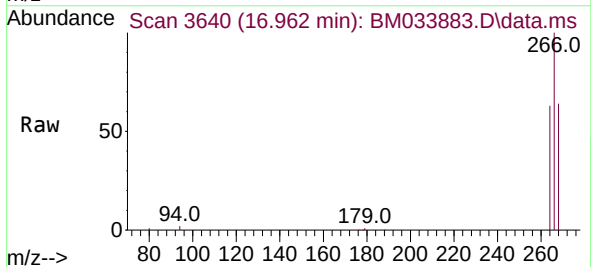

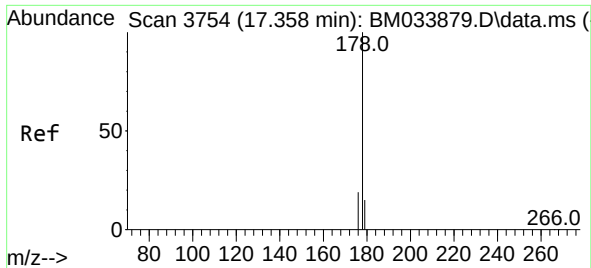

#15
 Phenanthrene
 Concen: 0.022 ng/ul
 RT: 17.351 min Scan# 31
 Delta R.T. -0.007 min
 Lab File: BM033883.D
 Acq: 26 Jan 2022 23:19

Instrument :
 BNA_M
 ClientSampleId :
 C0Q06

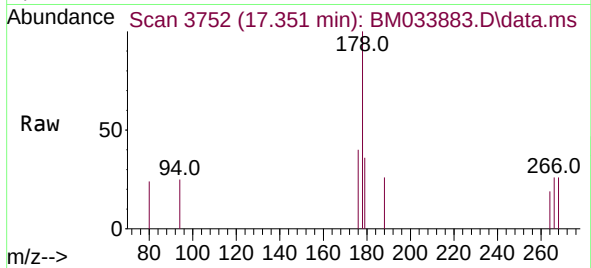

Tgt Ion:178 Resp: 520
 Ion Ratio Lower Upper
 178 100
 179 36.2 15.0 22.6#
 176 39.7 17.9 26.9#

