

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
 Data File : BM033885.D
 Acq On : 27 Jan 2022 00:30
 Operator : CG/JU
 Sample : N1230-19
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q21

Quant Time: Jan 27 02:13:04 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.939	152	1800	0.400	ng/ul	0.00
4) Naphthalene-d8	10.752	136	6474	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.572	164	3683	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.309	188	7223	0.400	ng/ul	-0.01
17) Chrysene-d12	21.473	240	5775	0.400	ng/ul	# 0.00
23) Perylene-d12	23.863	264	6313	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	9090	4.831	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	3344	0.375	ng/ul	0.00
18) Fluoranthene-d10	19.330	212	7357	0.414	ng/ul	0.00
Target Compounds						
						Qvalue
14) Pentachlorophenol	16.962	266	1112	0.335	ng/ul	99
15) Phenanthrene	17.351	178	742	0.032	ng/ul#	76


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
Data File : BM033885.D
Acq On : 27 Jan 2022 00:30
Operator : CG/JU
Sample : N1230-19
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q21

Quant Time: Jan 27 02:13:04 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration




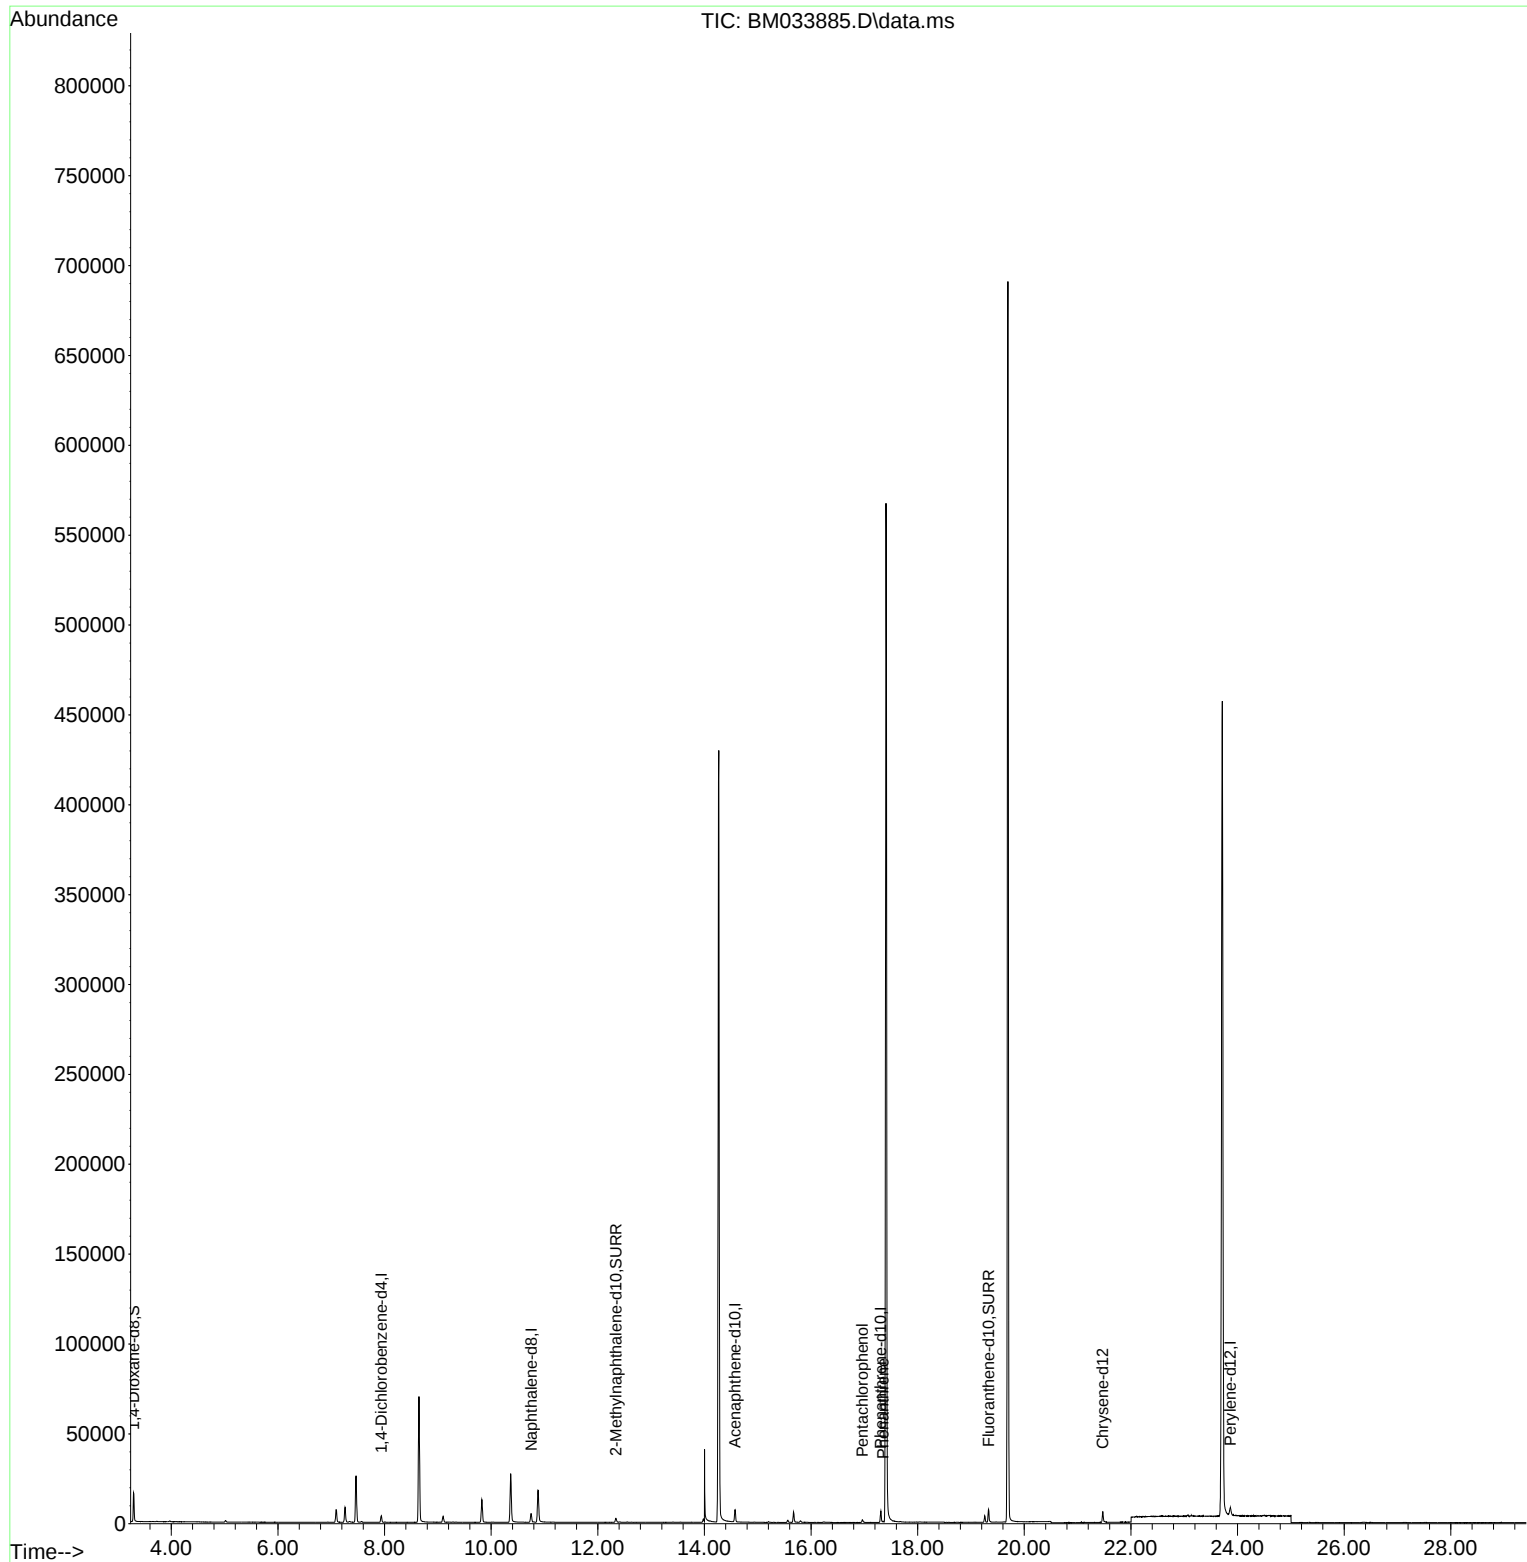


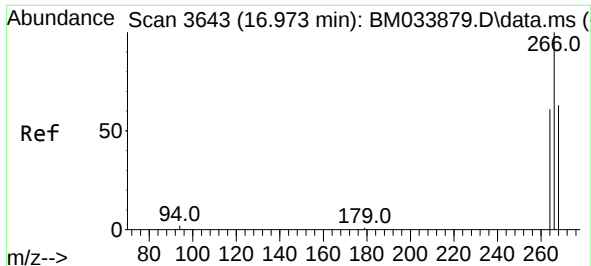

#14
 Pentachlorophenol
 Concen: 0.335 ng/ul
 RT: 16.962 min Scan# 3
 Delta R.T. -0.010 min
 Lab File: BM033885.D
 Acq: 27 Jan 2022 00:30

Instrument :
 BNA_M
 ClientSampleId :
 C0Q21

Tgt Ion:266 Resp: 1112
 Ion Ratio Lower Upper
 266 100
 264 63.7 51.4 77.0
 268 64.9 53.1 79.7

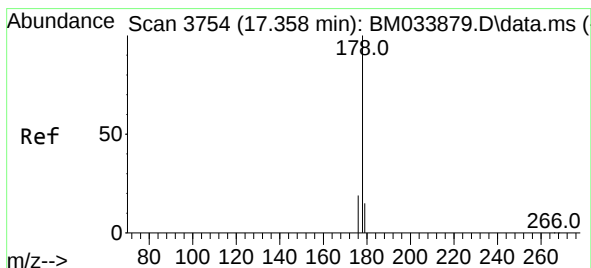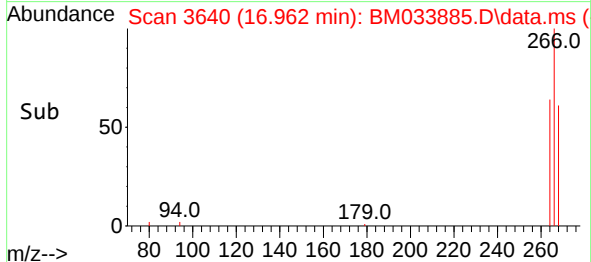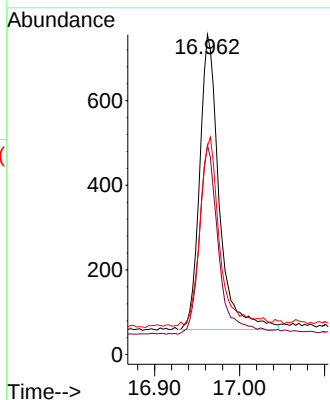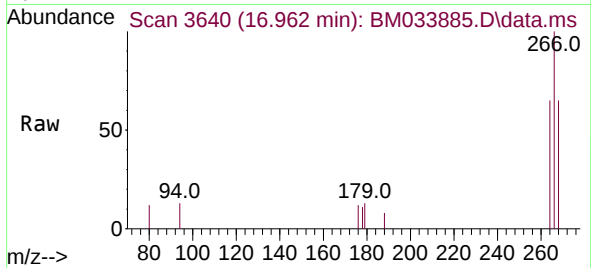

#15
 Phenanthrene
 Concen: 0.032 ng/ul
 RT: 17.351 min Scan# 3752
 Delta R.T. -0.007 min
 Lab File: BM033885.D
 Acq: 27 Jan 2022 00:30

Tgt Ion:178 Resp: 742
 Ion Ratio Lower Upper
 178 100
 179 31.6 15.0 22.6#
 176 32.0 17.9 26.9#

