

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
 Data File : BM033889.D
 Acq On : 27 Jan 2022 02:52
 Operator : CG/JU
 Sample : N1230-16
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q60

Quant Time: Jan 27 04:25:15 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.939	152	1723	0.400	ng/ul	0.00
4) Naphthalene-d8	10.751	136	6043	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.576	164	3433	0.400	ng/ul	0.00
13) Phenanthrene-d10	17.309	188	6506	0.400	ng/ul	-0.01
17) Chrysene-d12	21.472	240	5153	0.400	ng/ul	#-0.01
23) Perylene-d12	23.863	264	5986	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	9306	5.166	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	3002	0.361	ng/ul	0.00
18) Fluoranthene-d10	19.330	212	6646	0.419	ng/ul	0.00
Target Compounds						Qvalue
14) Pentachlorophenol	16.965	266	117	0.039	ng/ul	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
Data File : BM033889.D
Acq On : 27 Jan 2022 02:52
Operator : CG/JU
Sample : N1230-16
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q60


Quant Time: Jan 27 04:25:15 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

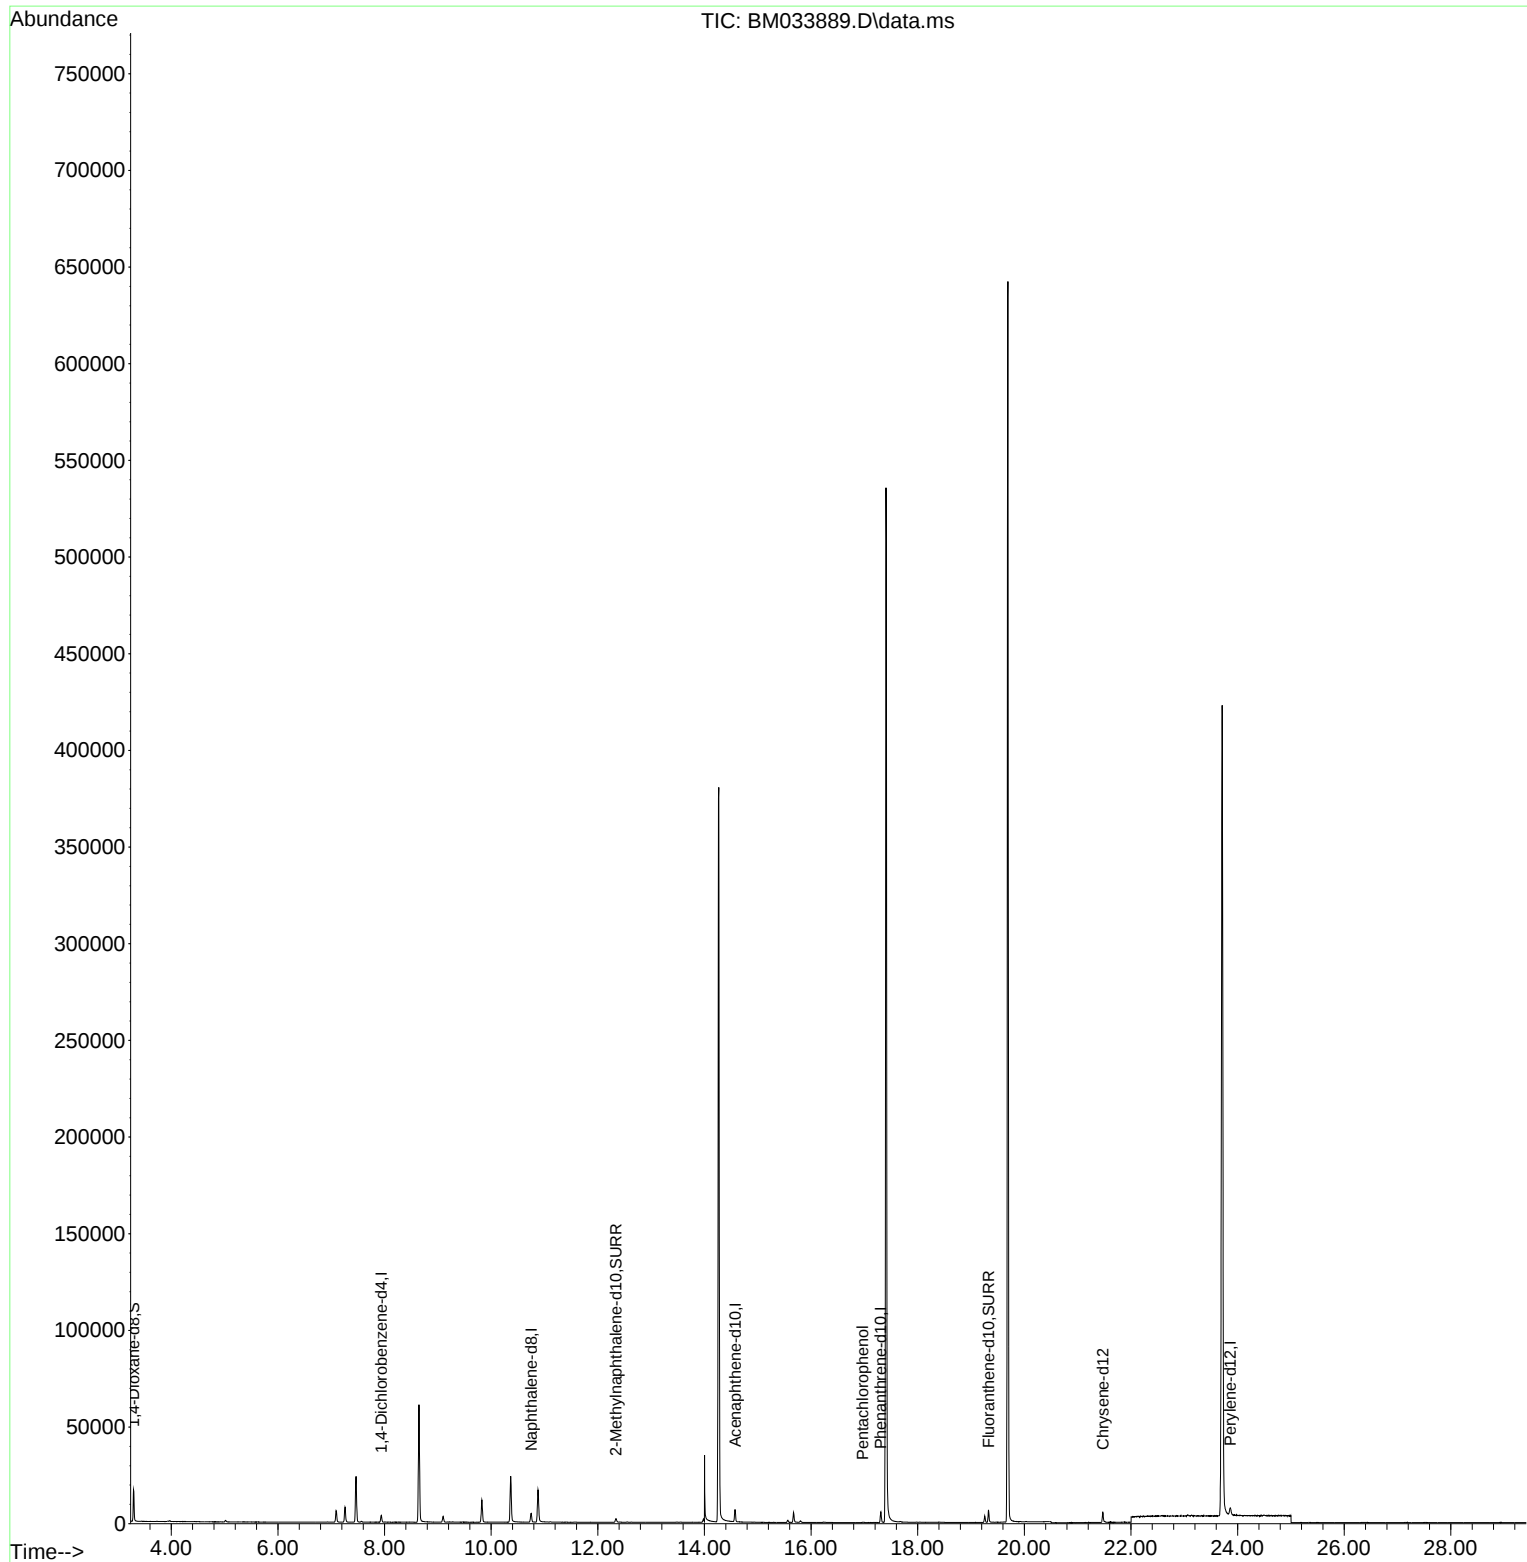

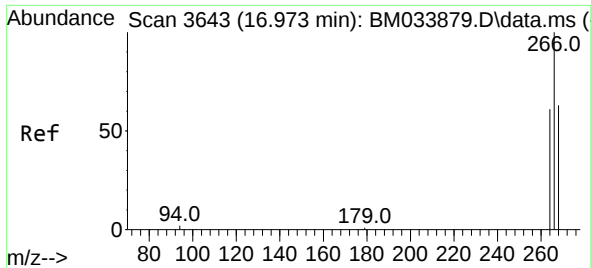

#14
 Pentachlorophenol
 Concen: 0.039 ng/ul
 RT: 16.965 min Scan# 30
 Delta R.T. -0.007 min
 Lab File: BM033889.D
 Acq: 27 Jan 2022 02:52

Instrument :
 BNA_M
 ClientSampleId :
 C0Q60

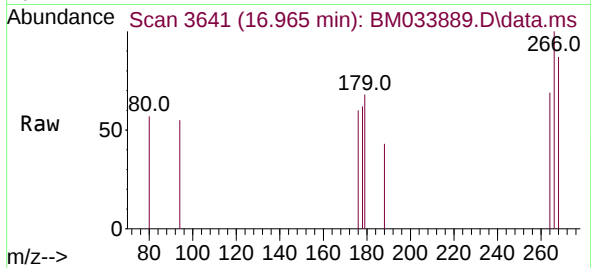

Tgt Ion: 266 Resp: 117

Ion	Ratio	Lower	Upper
266	100		
264	59.8	51.4	77.0
268	70.1	53.1	79.7

