

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
 Data File : BM033901.D
 Acq On : 27 Jan 2022 14:19
 Operator : CG/JU
 Sample : N1230-07DL 5X
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q20DL

Quant Time: Jan 28 01:50:43 2022
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jan 24 15:20:03 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.936	152	2077	0.400	ng/ul	0.00
4) Naphthalene-d8	10.747	136	7377	0.400	ng/ul	# 0.00
9) Acenaphthene-d10	14.572	164	3802	0.400	ng/ul	-0.01
13) Phenanthrene-d10	17.309	188	7284	0.400	ng/ul	-0.01
17) Chrysene-d12	21.475	240	5602	0.400	ng/ul	# 0.00
23) Perylene-d12	23.868	264	5960	0.400	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.292	96	2442	1.125	ng/ul	0.00
6) 2-Methylnaphthalene-d10	12.339	152	877	0.086	ng/ul	0.00
18) Fluoranthene-d10	19.330	212	1760	0.102	ng/ul	0.00
Target Compounds						
14) Pentachlorophenol	16.962	266	2603	0.778	ng/ul	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM012622\
Data File : BM033901.D
Acq On : 27 Jan 2022 14:19
Operator : CG/JU
Sample : N1230-07DL 5X
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q20DL


Quant Time: Jan 28 01:50:43 2022
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-SIM-BM012422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 24 15:20:03 2022
Response via : Initial Calibration

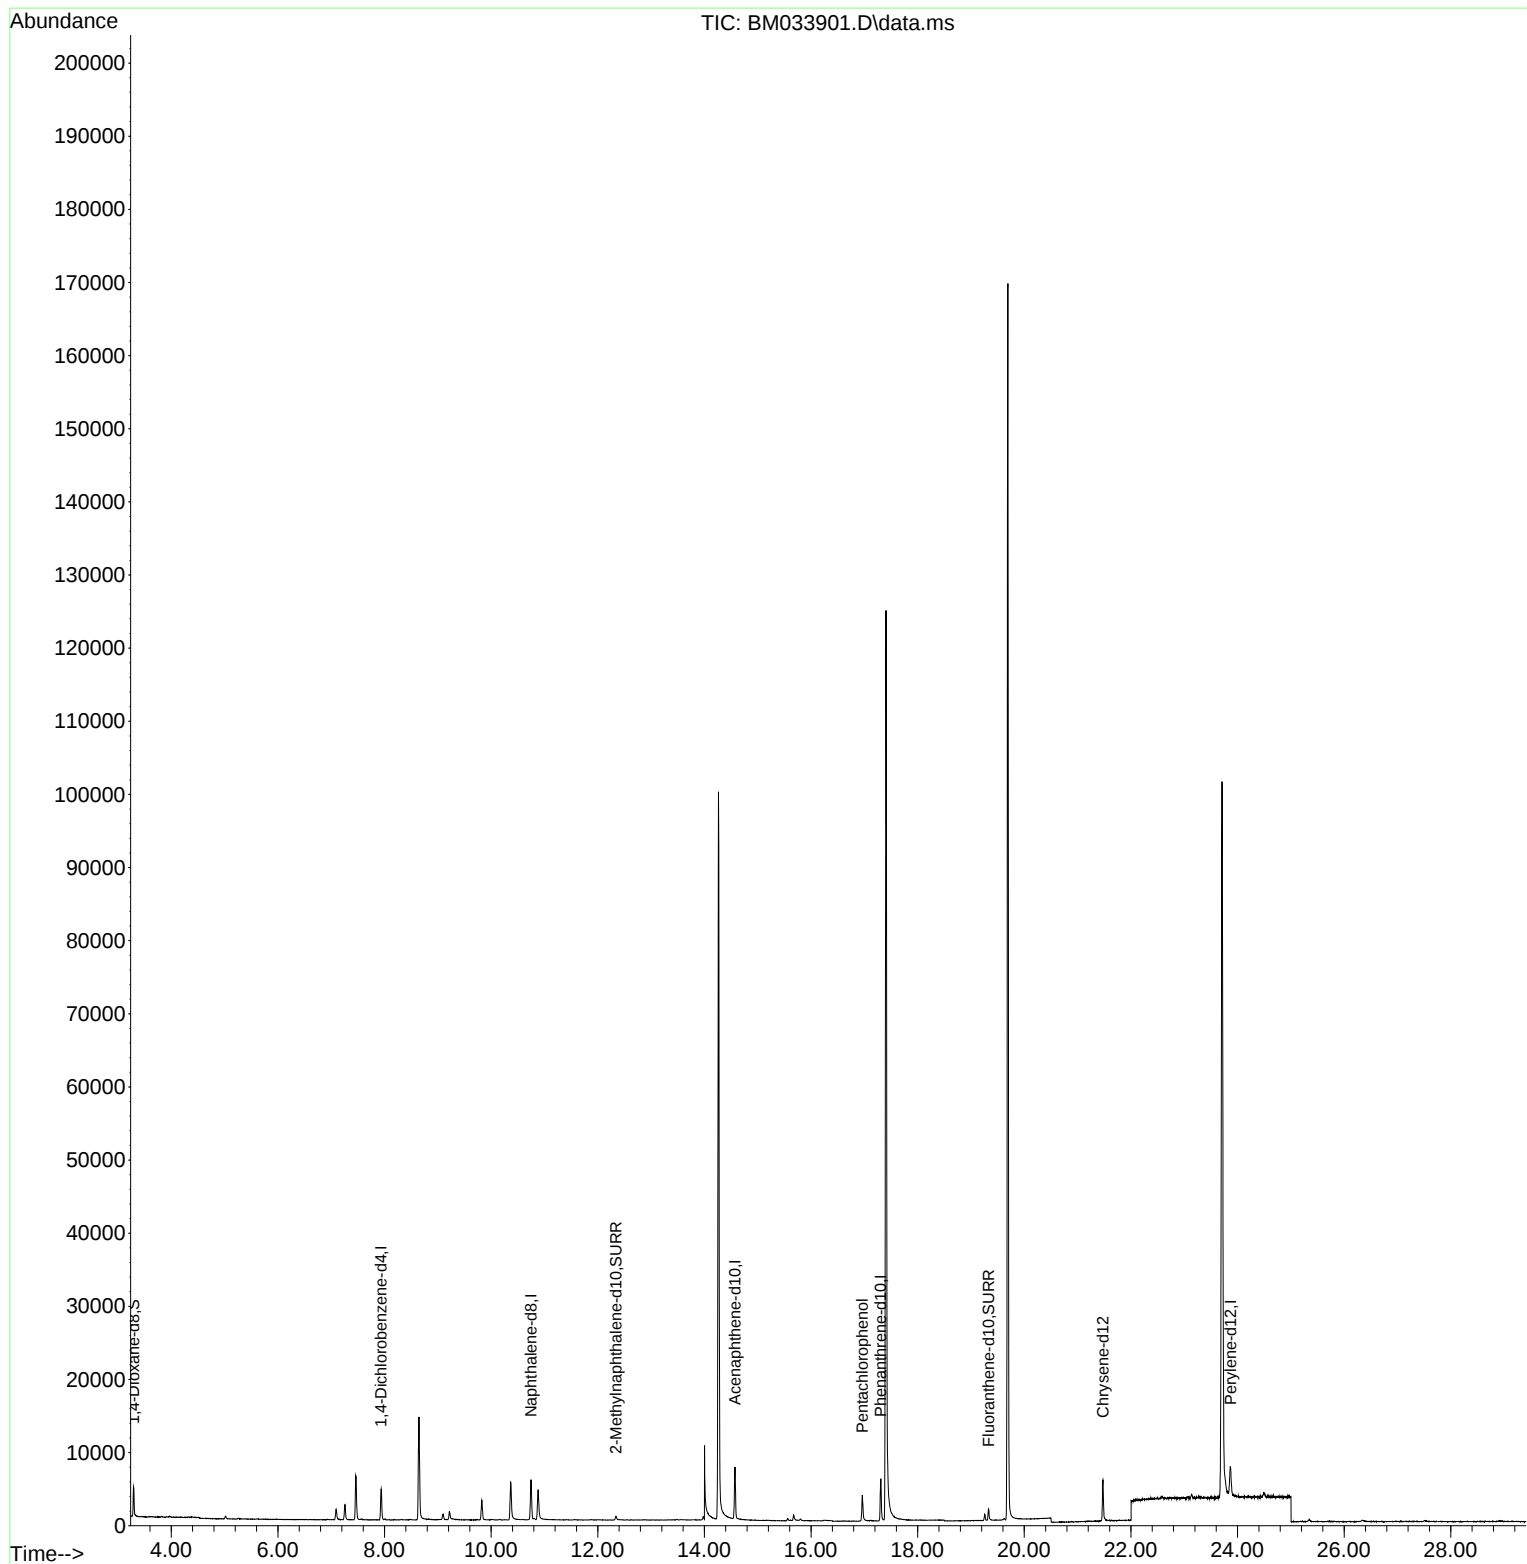

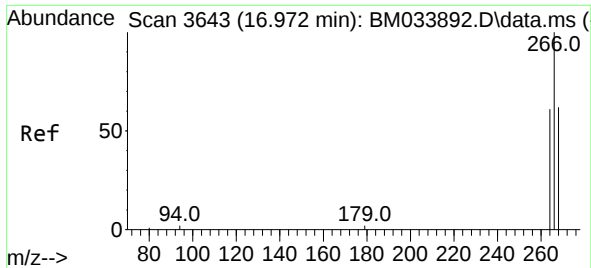

#14
 Pentachlorophenol
 Concen: 0.778 ng/ul
 RT: 16.962 min Scan# 30
 Delta R.T. -0.010 min
 Lab File: BM033901.D
 Acq: 27 Jan 2022 14:19

Instrument :
 BNA_M
 ClientSampleId :
 C0Q20DL

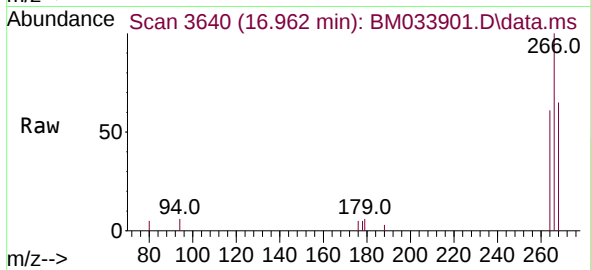

Tgt Ion:266	Resp:	2603
Ion	Ratio	Lower Upper
266	100	
264	63.5	51.4 77.0
268	65.2	53.1 79.7

