




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033937.D
Acq On : 01 Feb 2022 13:46
Operator : CG/JU
Sample : N1273-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:58:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

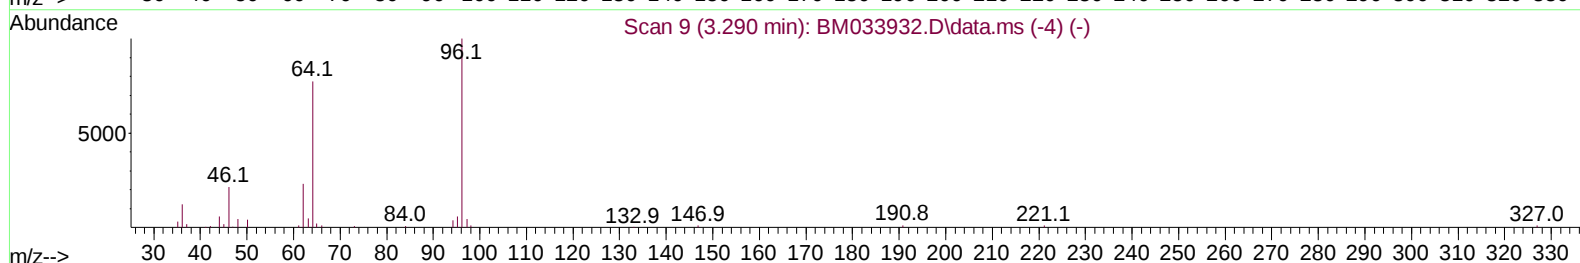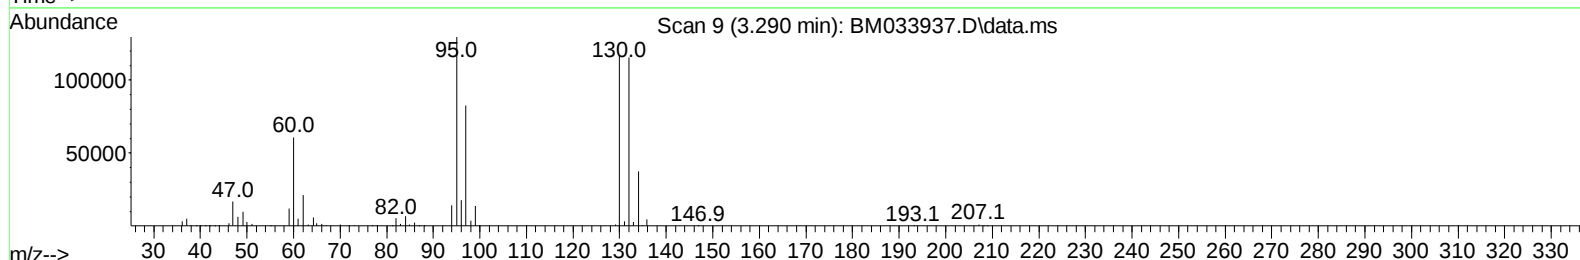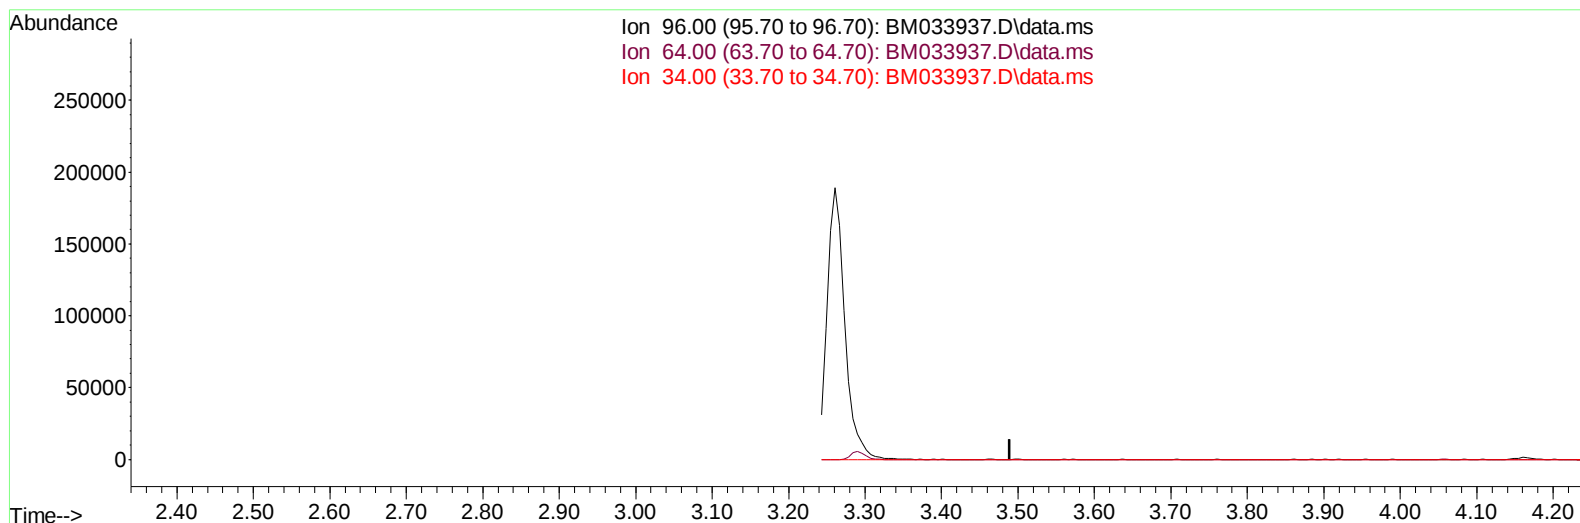

TIC: BM033937.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.290min (-3.290) 0.00 ng/uL

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	74.20	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033937.D
 Acq On : 01 Feb 2022 13:46
 Operator : CG/JU
 Sample : N1273-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:58:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

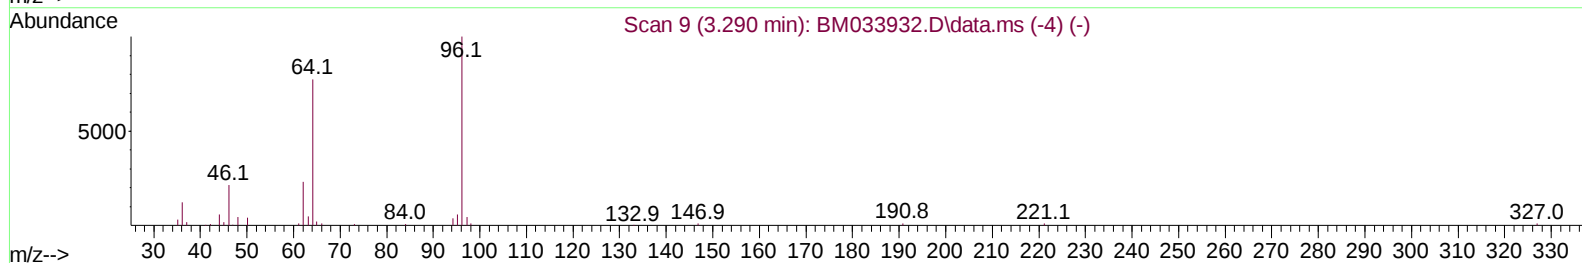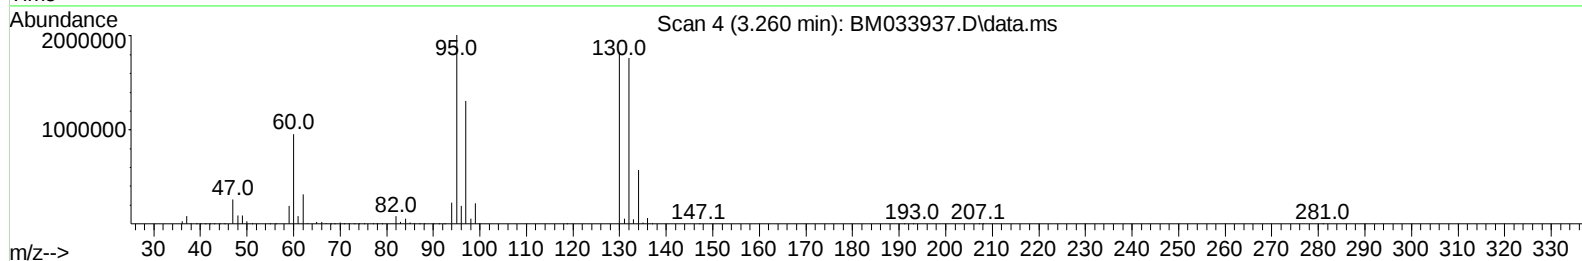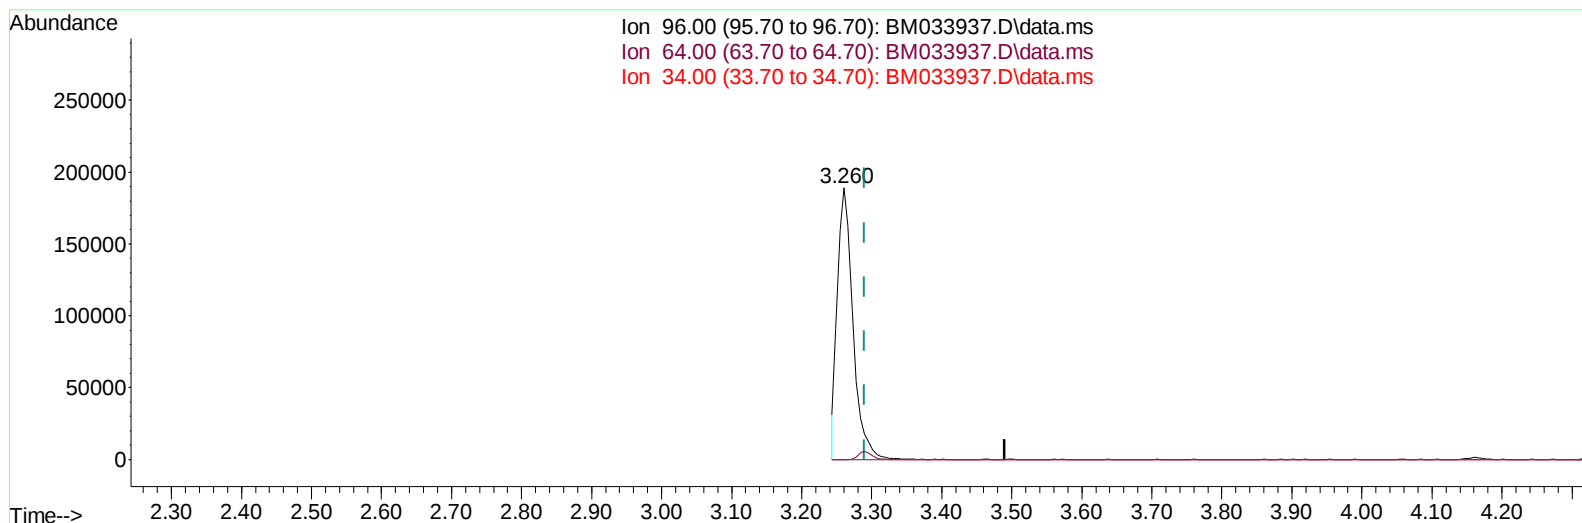

TIC: BM033937.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.260min (-0.030) 117.77 ng/uL m

response 293715

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033937.D
 Acq On : 01 Feb 2022 13:46
 Operator : CG/JU
 Sample : N1273-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:58:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

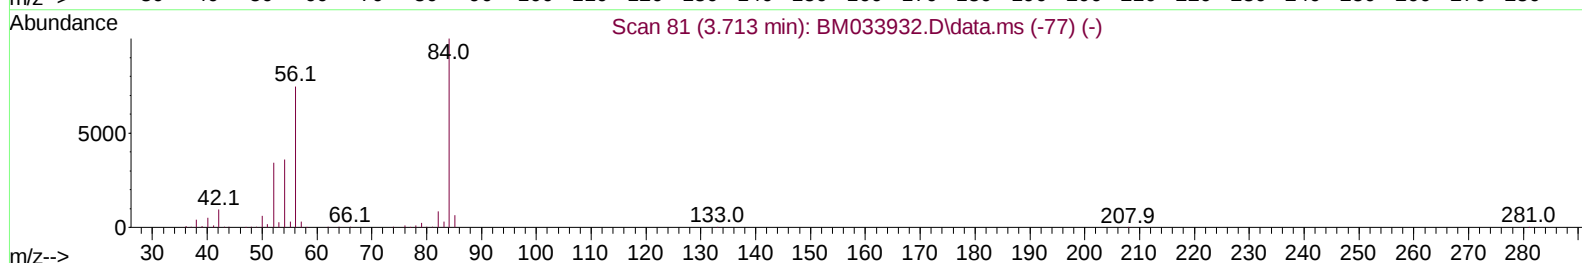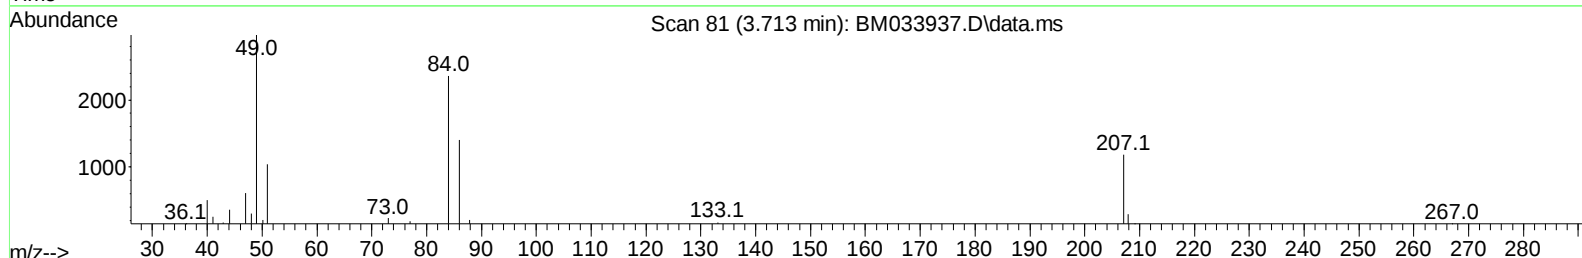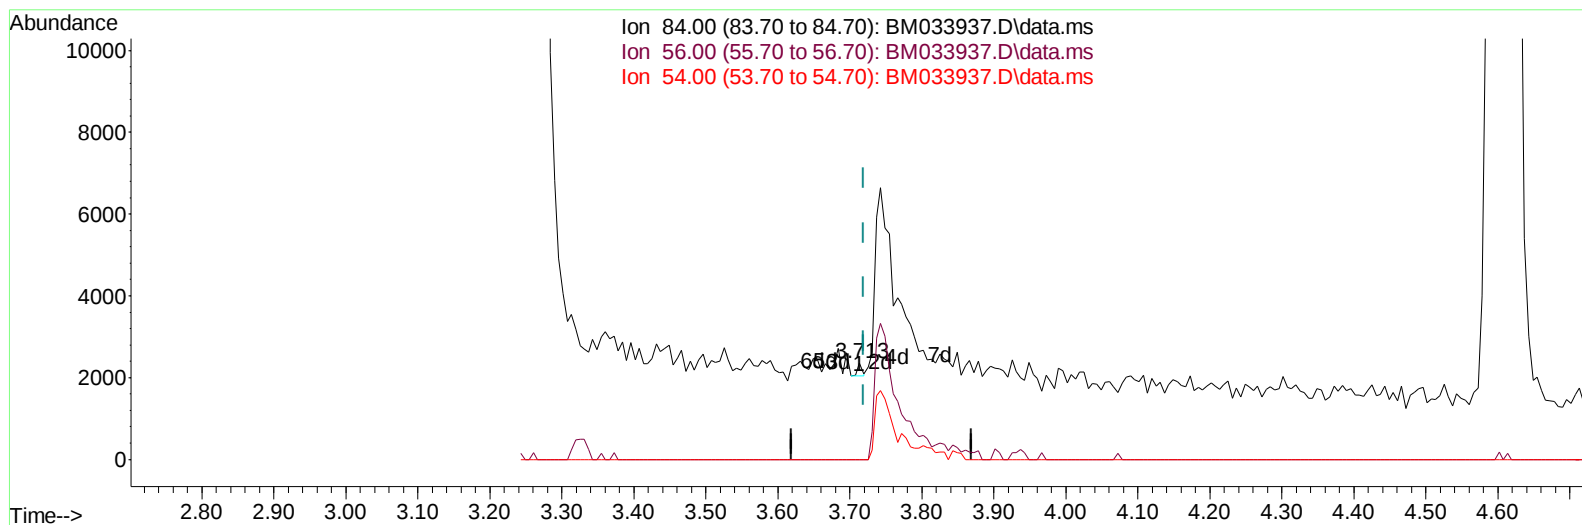

TIC: BM033937.D\data.ms

(4) Pyridine-d5 (S)

3.713min (-0.006) 0.02 ng/u1

response 140

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	80.70	0.00#
54.00	42.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033937.D
 Acq On : 01 Feb 2022 13:46
 Operator : CG/JU
 Sample : N1273-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:58:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

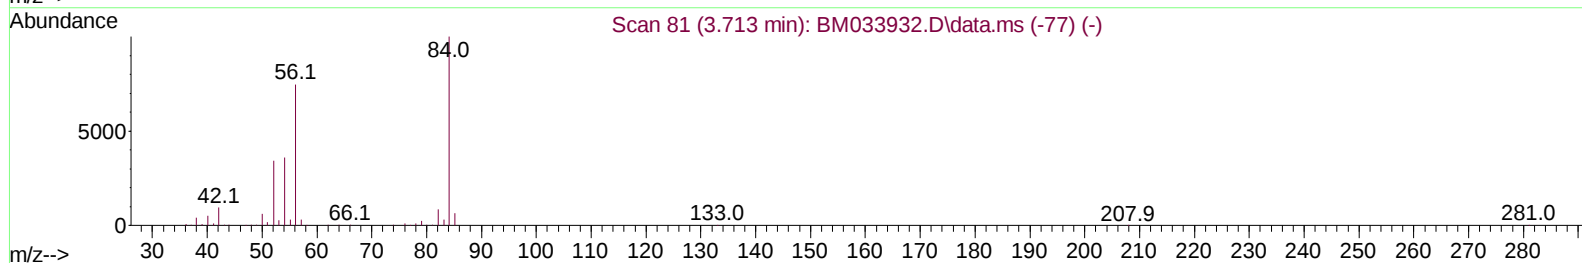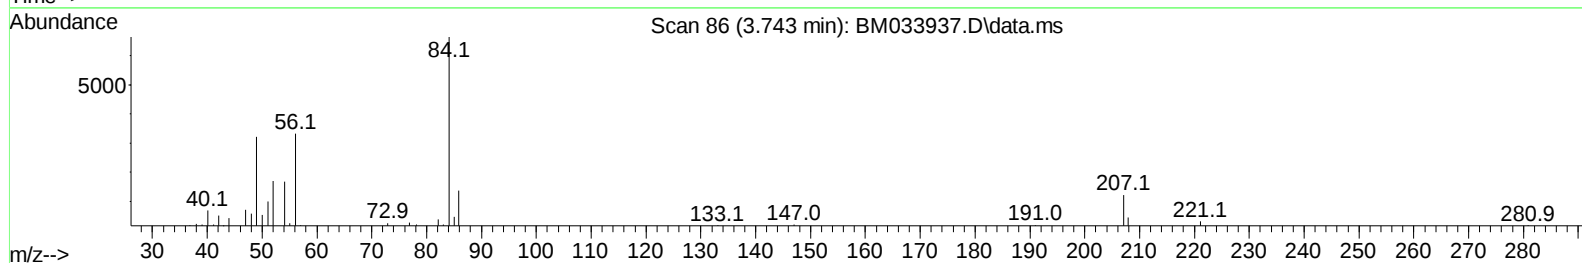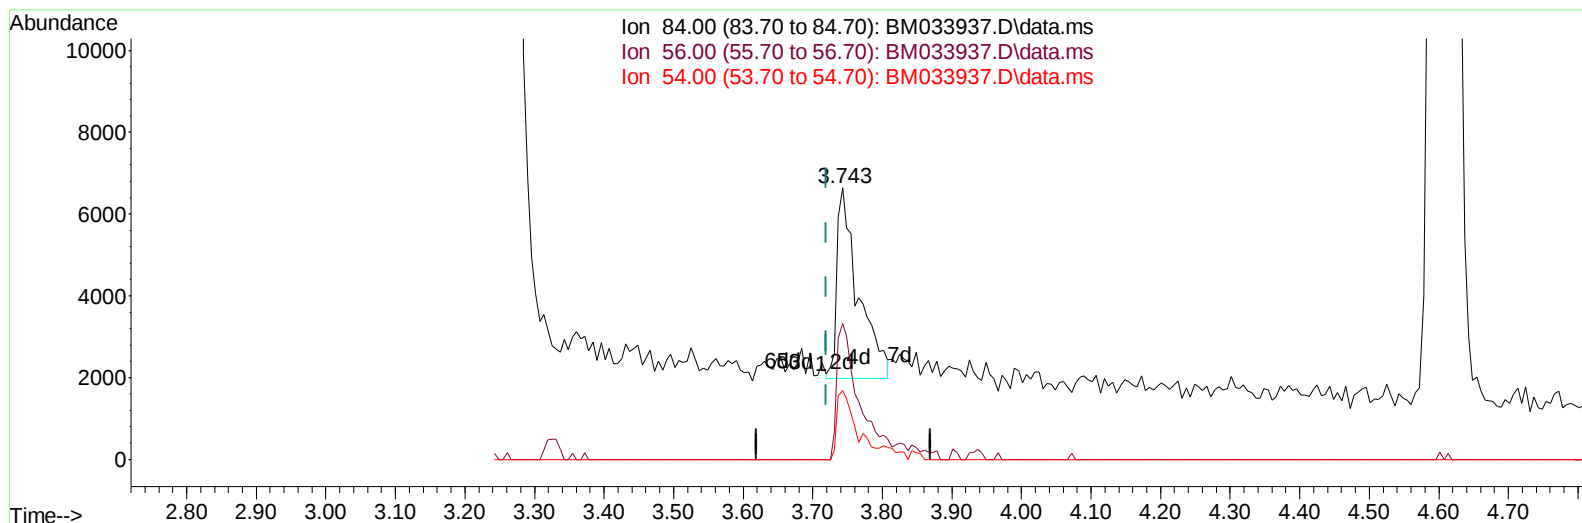

TIC: BM033937.D\data.ms

(4) Pyridine-d5 (S)

3.743min (+ 0.024) 1.42 ng/u1 m

response 9855

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	80.70	50.05#
54.00	42.60	25.26#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033937.D
Acq On : 01 Feb 2022 13:46
Operator : CG/JU
Sample : N1273-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:58:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

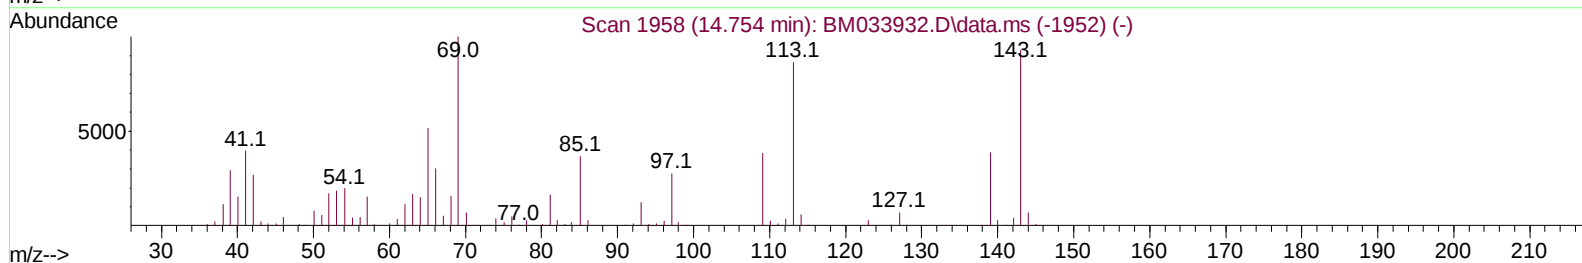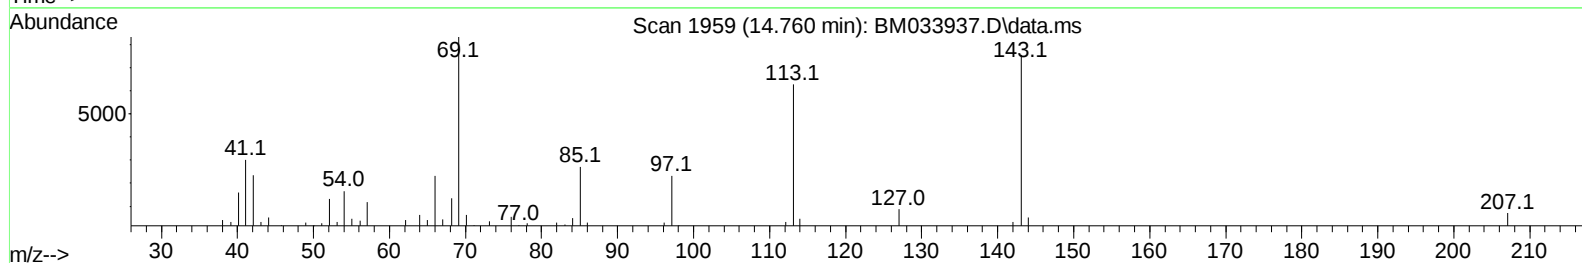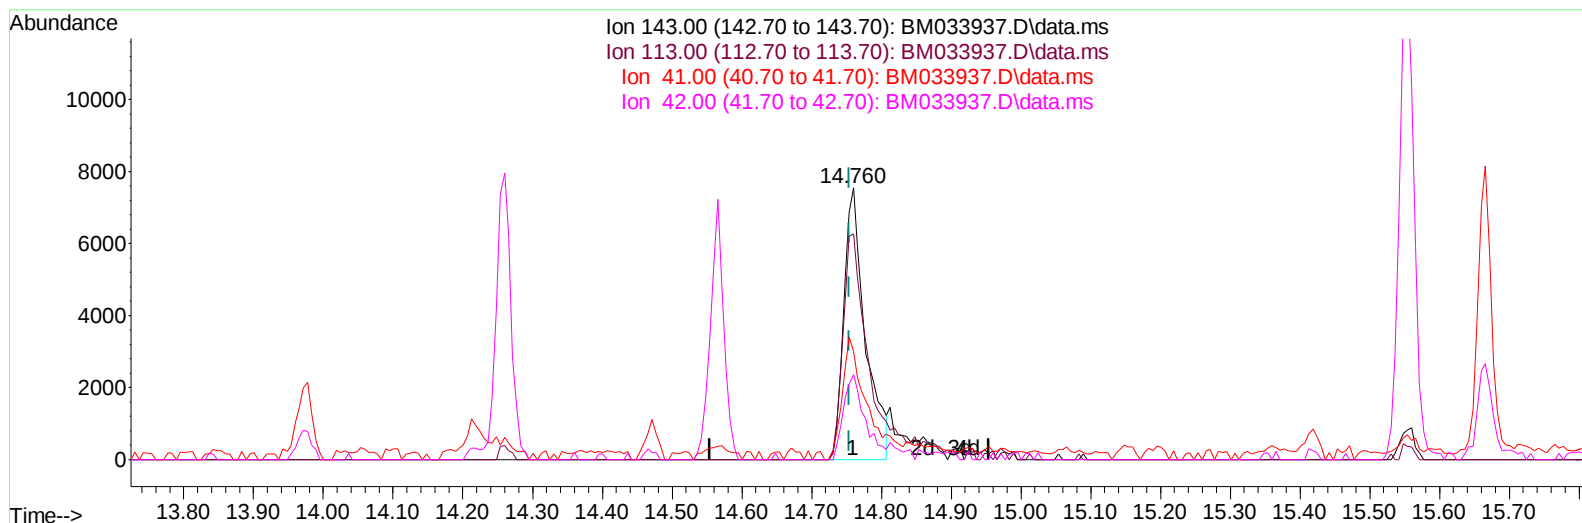

TIC: BM033937.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.760min (+ 0.006) 4.57 ng/u1

response 16074

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	83.10#
41.00	57.20	39.86#
42.00	39.50	31.19#




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033937.D
Acq On : 01 Feb 2022 13:46
Operator : CG/JU
Sample : N1273-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL5

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:58:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

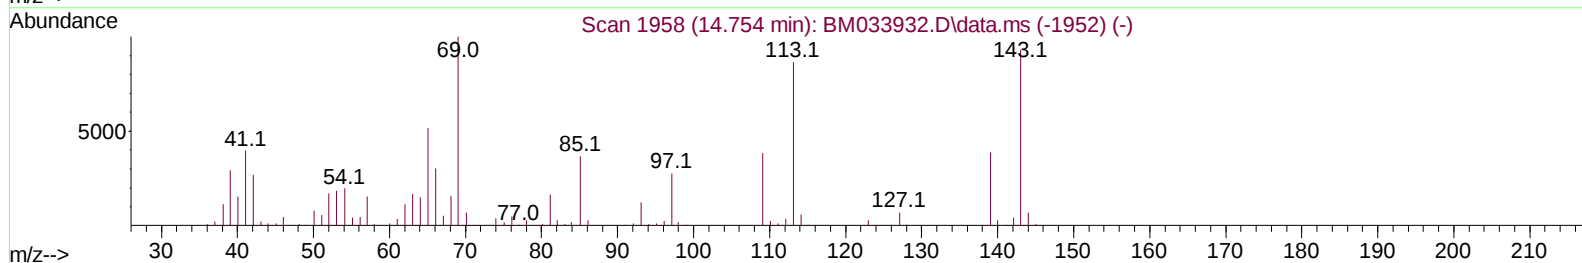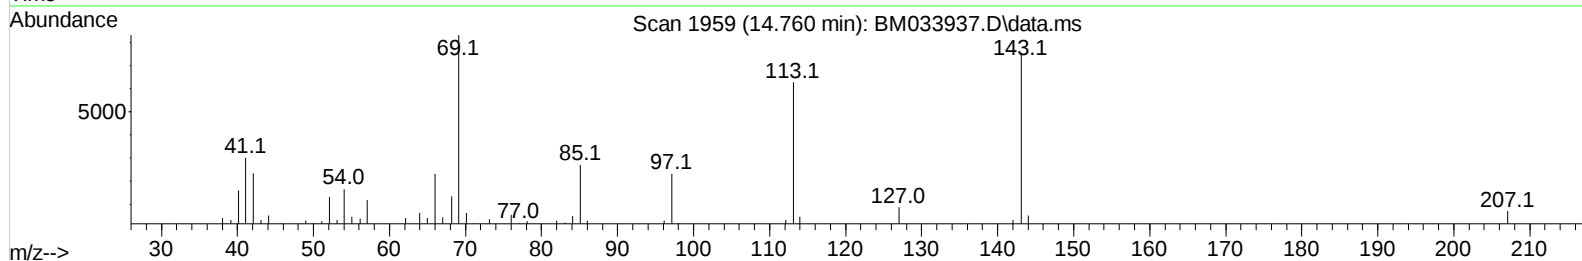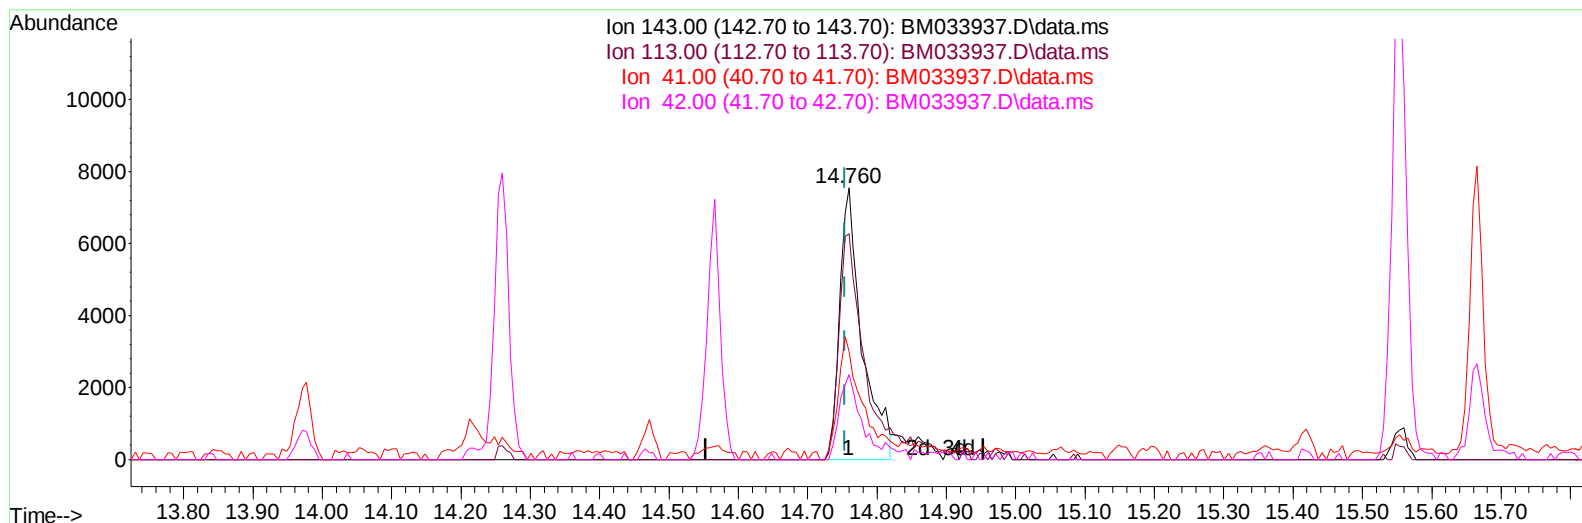

TIC: BM033937.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.760min (+ 0.006) 4.78 ng/ul m

response 16827

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	83.10#
41.00	57.20	39.86#
42.00	39.50	31.19#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033937.D
 Acq On : 01 Feb 2022 13:46
 Operator : CG/JU
 Sample : N1273-17
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 01 23:58:50 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	98358	20.000	ng/ul	0.00
20) Naphthalene-d8	10.742	136	425794	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.566	164	275683	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.301	188	528750	20.000	ng/ul	0.00
79) Chrysene-d12	21.465	240	390571	20.000	ng/ul	0.00
88) Perylene-d12	23.853	264	386261	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	293715m	117.772	ng/uL	-0.03
4) Pyridine-d5	3.743	84	9855m	1.416	ng/ul	0.02
7) Phenol-d5	7.084	99	55863	6.779	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	190547	37.930	ng/ul	0.00
11) 2-Chlorophenol-d4	7.454	132	189314	28.676	ng/ul	0.00
15) 4-Methylphenol-d8	8.637	113	111277	17.042	ng/ul	0.00
21) Nitrobenzene-d5	9.089	128	124205	36.354	ng/ul	0.00
24) 2-Nitrophenol-d4	9.819	143	130769	35.443	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	203459	30.473	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131	45166	4.899	ng/ul	0.00
46) Dimethylphthalate-d6	13.977	166	800910	38.877	ng/ul	0.00
49) Acenaphthylene-d8	14.260	160	874608	34.657	ng/ul	0.00
54) 4-Nitrophenol-d4	14.760	143	16827m	4.781	ng/ul	0.00
60) Fluorene-d10	15.554	176	661972	38.483	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.666	200	114165	34.393	ng/ul	0.00
73) Anthracene-d10	17.401	188	1051769	41.536	ng/ul	0.00
81) Pyrene-d10	19.683	212	1061392	46.030	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.700	264	892607	43.997	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.325	88	156532	57.517	ng/uL#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033937.D
Acq On : 01 Feb 2022 13:46
Operator : CG/JU
Sample : N1273-17
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL5

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 01 23:58:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

