




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033939.D
Acq On : 01 Feb 2022 14:58
Operator : CG/JU
Sample : N1328-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HM1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 01 23:59:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

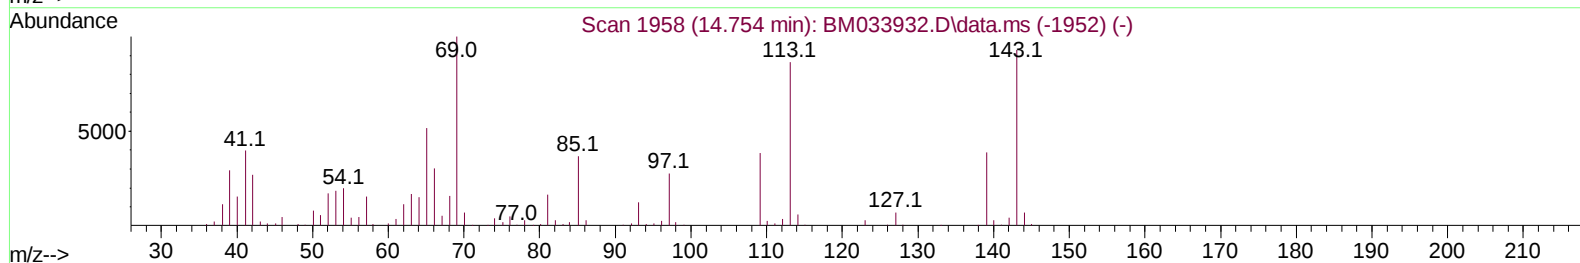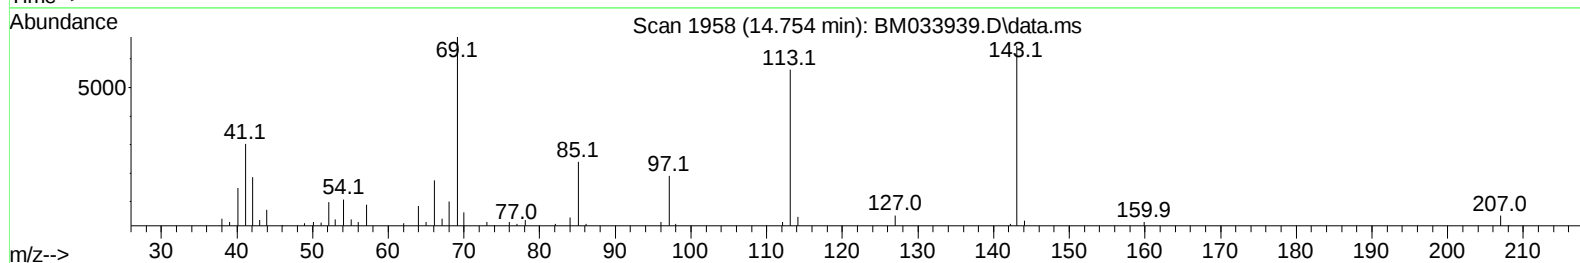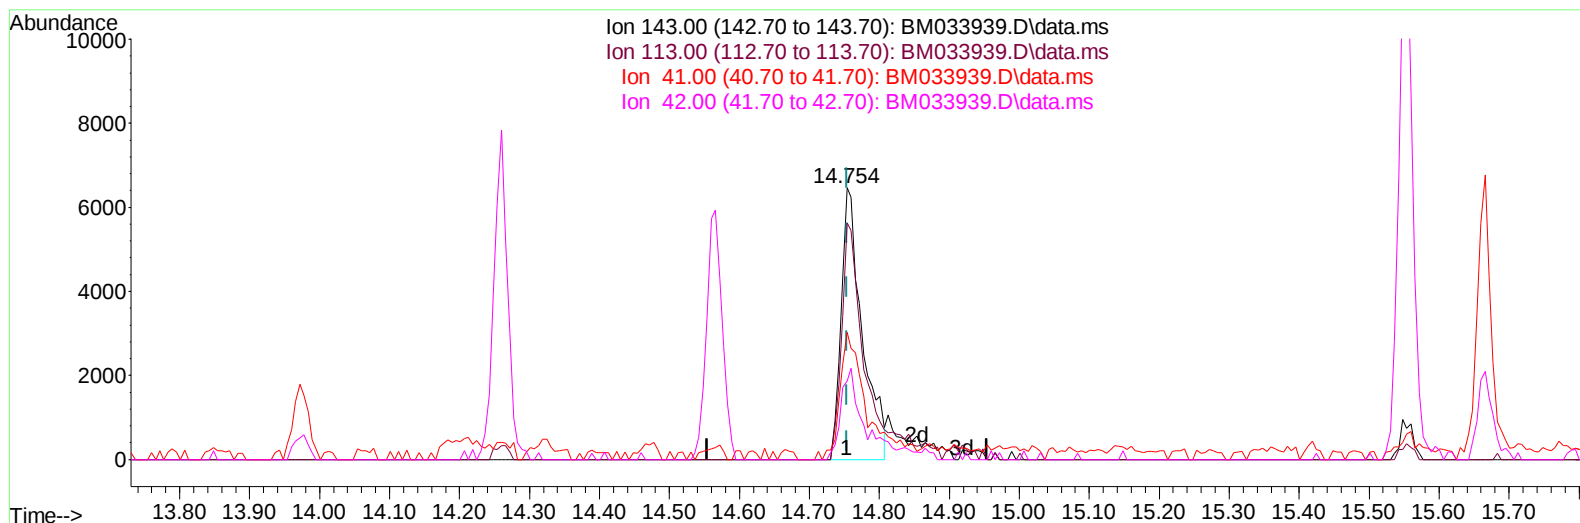

TIC: BM033939.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.754min (+ 0.000) 4.00 ng/u1

response 13449

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	87.12
41.00	57.20	46.83
42.00	39.50	28.88#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033939.D
 Acq On : 01 Feb 2022 14:58
 Operator : CG/JU
 Sample : N1328-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHM1

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:59:09 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	99525	20.000	ng/ul	0.00
20) Naphthalene-d8	10.742	136	420646	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.566	164	263417	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.301	188	497877	20.000	ng/ul	0.00
79) Chrysene-d12	21.465	240	386432	20.000	ng/ul	0.00
88) Perylene-d12	23.853	264	403066	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	8216	3.256	ng/uL	0.00
4) Pyridine-d5	3.725	84	53168	7.548	ng/ul	0.00
7) Phenol-d5	7.084	99	51984	6.235	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	171207	33.681	ng/ul	0.00
11) 2-Chlorophenol-d4	7.454	132	169492	25.373	ng/ul	0.00
15) 4-Methylphenol-d8	8.637	113	100334	15.186	ng/ul	0.00
21) Nitrobenzene-d5	9.090	128	109562	32.461	ng/ul	0.00
24) 2-Nitrophenol-d4	9.819	143	114715	31.473	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	183239	27.781	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131	231127	25.375	ng/ul	0.00
46) Dimethylphthalate-d6	13.977	166	693178	35.215	ng/ul	0.00
49) Acenaphthylene-d8	14.260	160	793014	32.887	ng/ul	0.00
54) 4-Nitrophenol-d4	14.754	143	14260m	4.240	ng/ul	0.00
60) Fluorene-d10	15.554	176	575660	35.024	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.666	200	92734	29.669	ng/ul	0.00
73) Anthracene-d10	17.401	188	892536	37.433	ng/ul	0.00
81) Pyrene-d10	19.683	212	918933	40.279	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.700	264	820035	38.735	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.325	88	34175	12.410	ng/ul#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033939.D
Acq On : 01 Feb 2022 14:58
Operator : CG/JU
Sample : N1328-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HM1

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 01 23:59:09 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

