




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033940.D
 Acq On : 01 Feb 2022 15:34
 Operator : CG/JU
 Sample : N1273-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL8

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:59:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

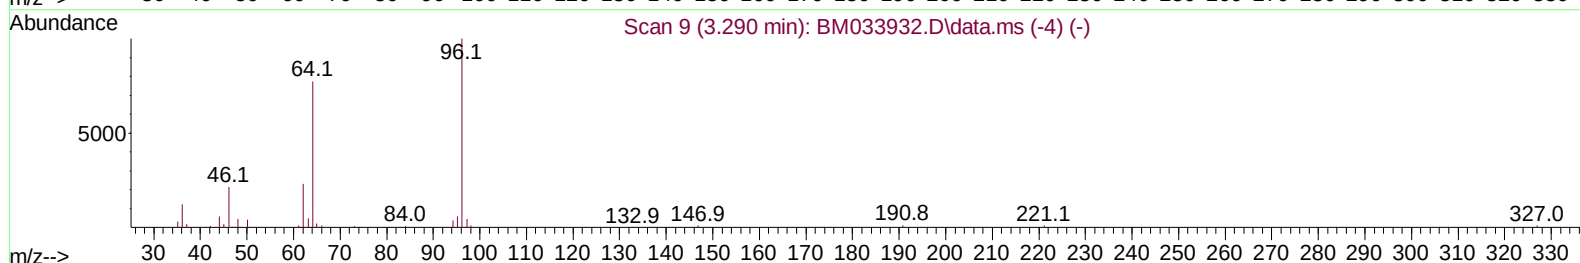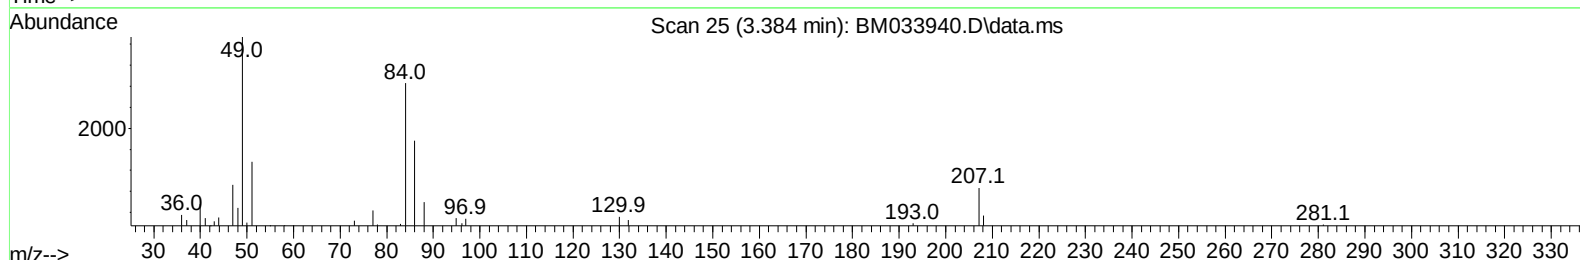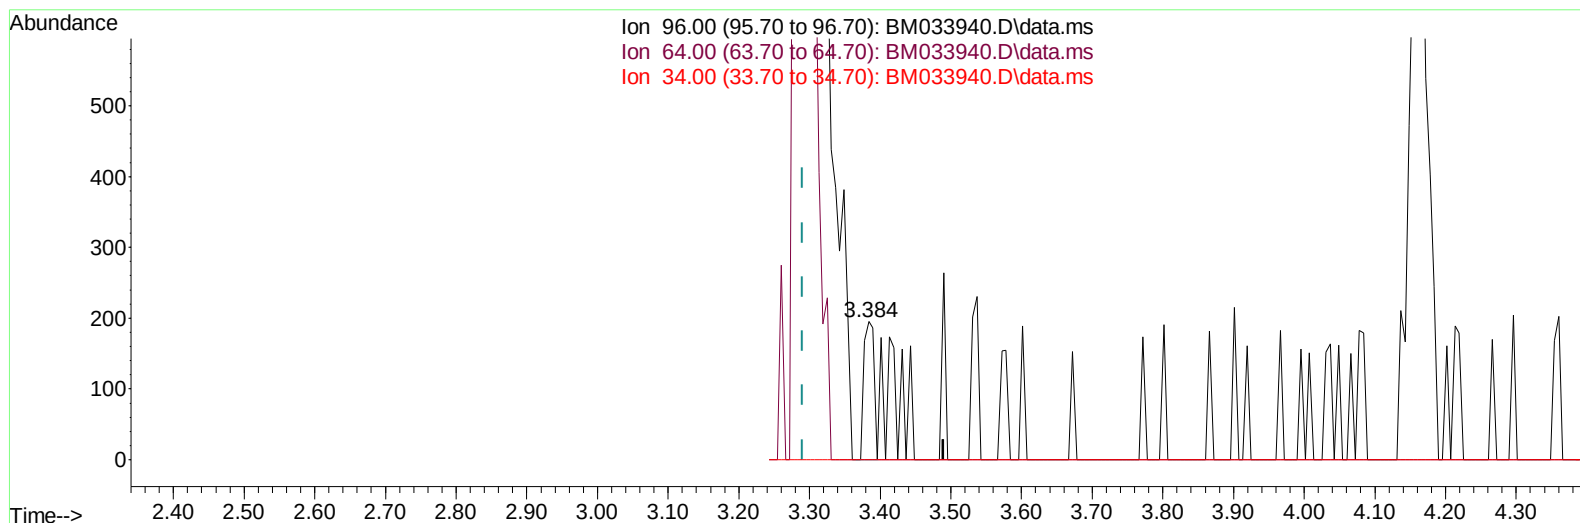

TIC: BM033940.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.384min (+ 0.094) 0.08 ng/uL

response 194

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033940.D
Acq On : 01 Feb 2022 15:34
Operator : CG/JU
Sample : N1273-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 01 23:59:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

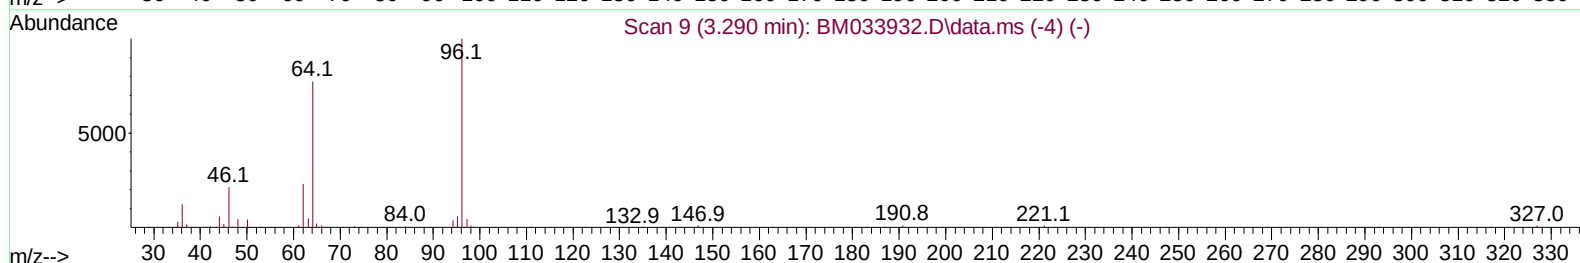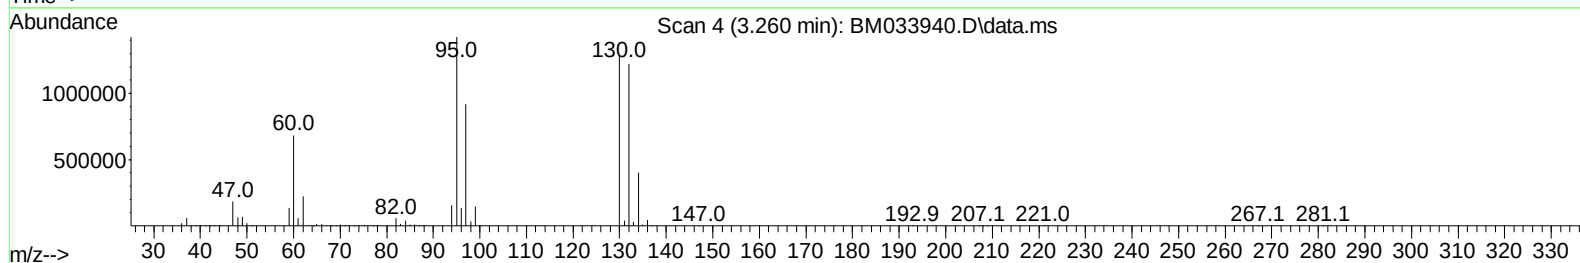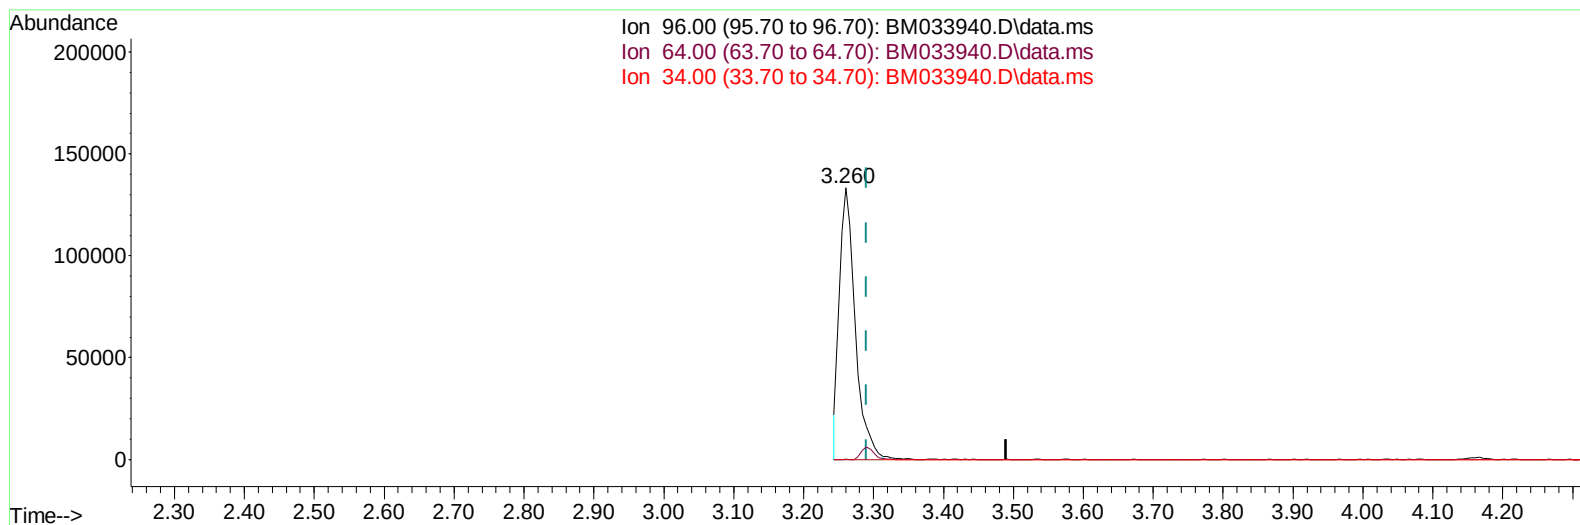

TIC: BM033940.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.260min (-0.030) 84.16 ng/uL m

response 211457

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	0.21#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033940.D
 Acq On : 01 Feb 2022 15:34
 Operator : CG/JU
 Sample : N1273-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL8

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:59:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

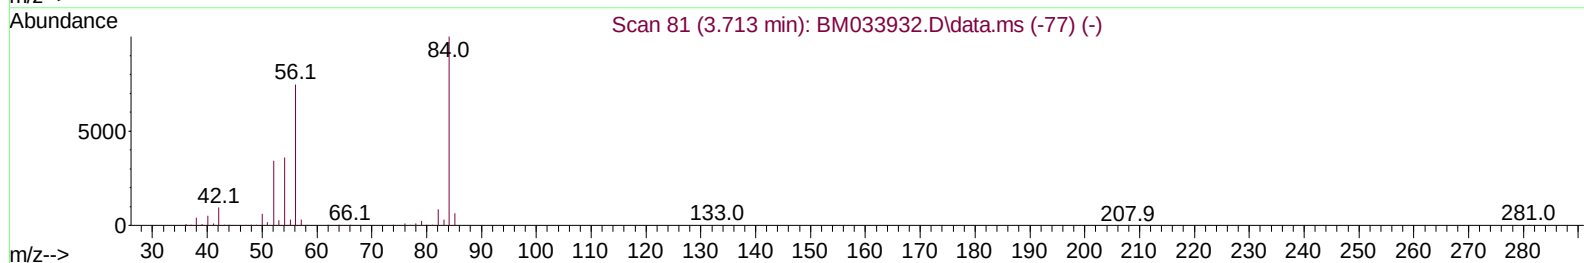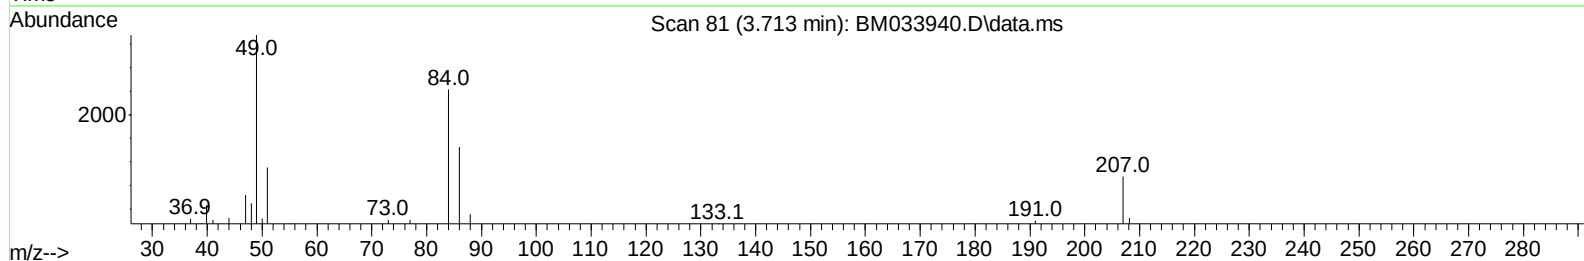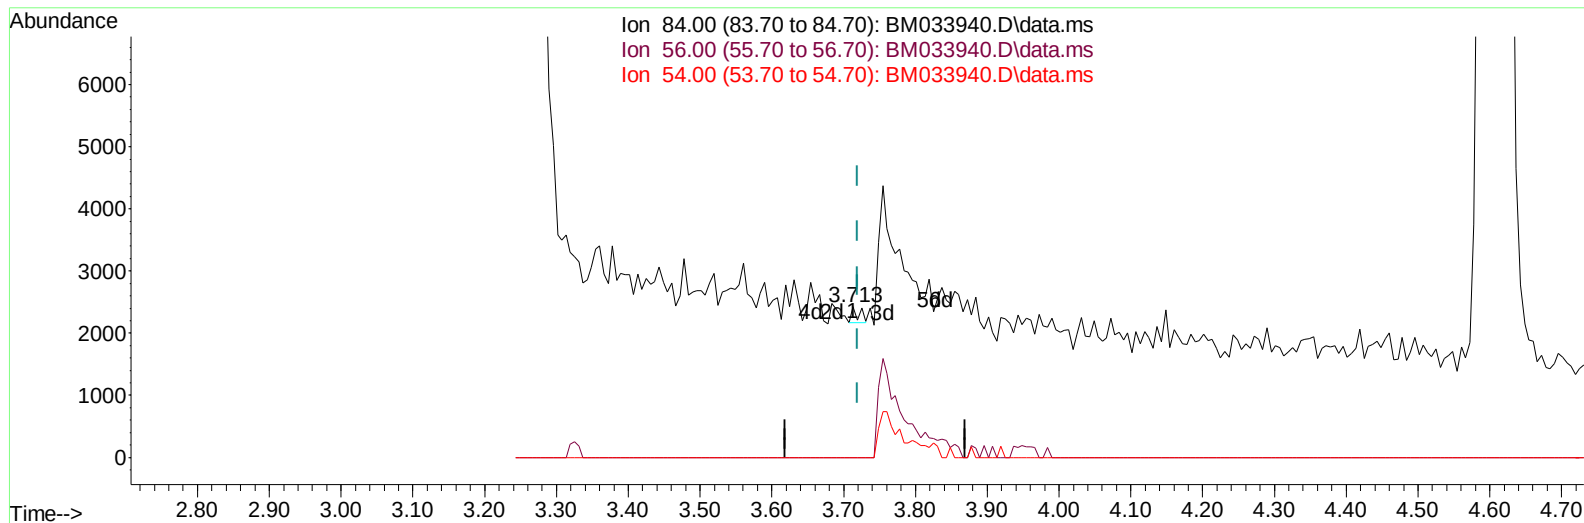

TIC: BM033940.D\data.ms

(4) Pyridine-d5 (S)

3.713min (-0.006) 0.03 ng/u1

response 198

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	80.70	0.00#
54.00	42.60	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033940.D
 Acq On : 01 Feb 2022 15:34
 Operator : CG/JU
 Sample : N1273-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL8

Manual IntegrationsAPPROVED

Quant Time: Feb 01 23:59:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

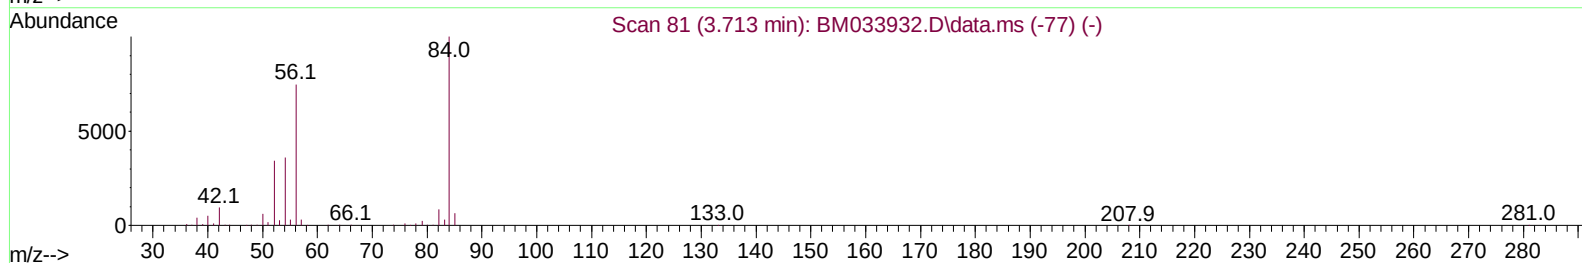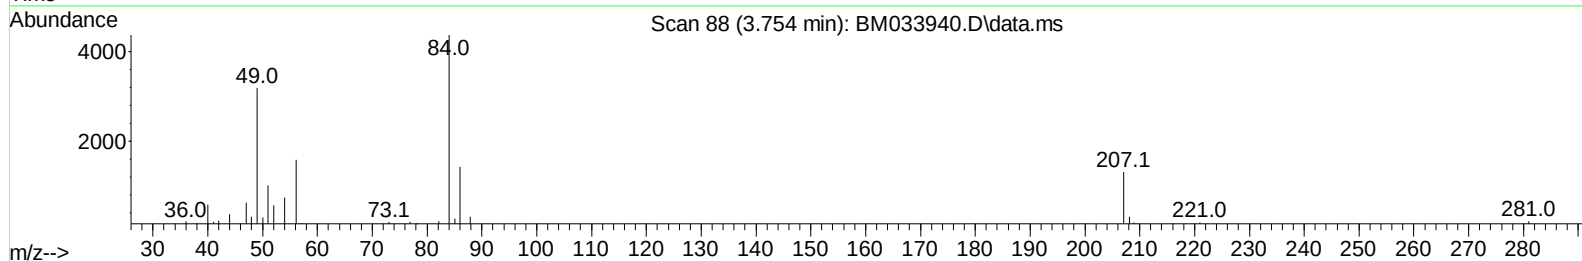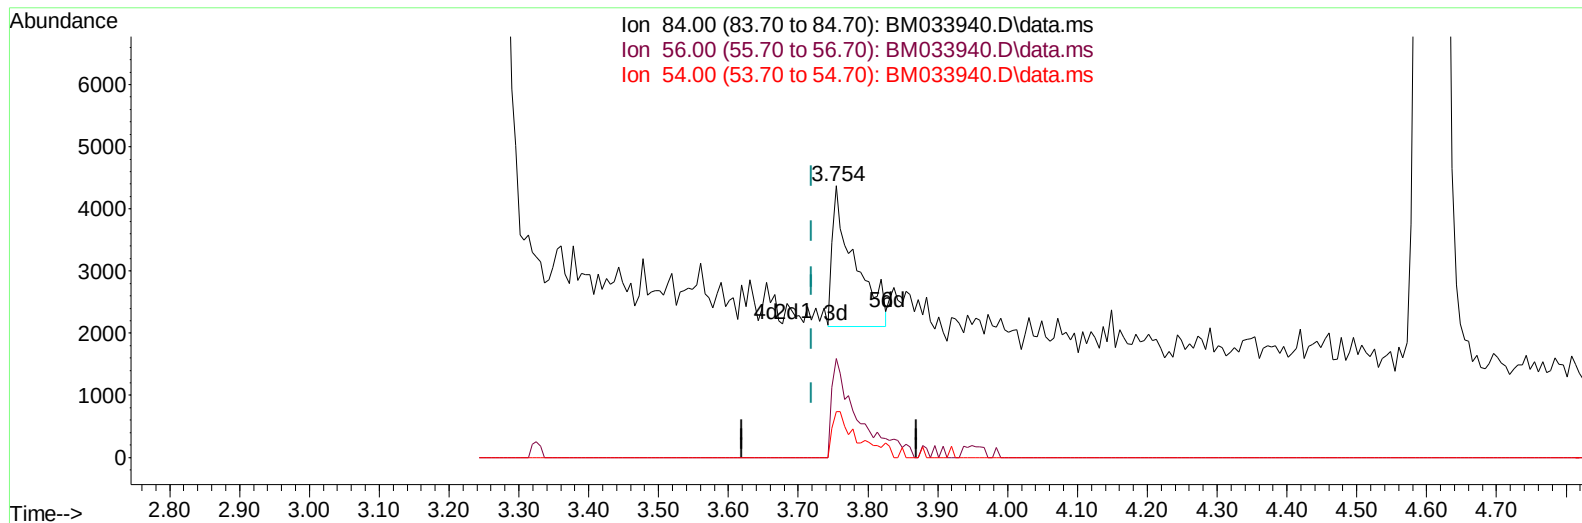

TIC: BM033940.D\data.ms

(4) Pyridine-d5 (S)

3.754min (+ 0.035) 0.71 ng/ul m

response 5010

Ion	Exp%	Act%
84.00	100.00	100.00
56.00	80.70	36.32#
54.00	42.60	16.94#
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033940.D
 Acq On : 01 Feb 2022 15:34
 Operator : CG/JU
 Sample : N1273-20
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 01 23:59:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	99091	20.000	ng/ul	0.00
20) Naphthalene-d8	10.742	136	429417	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.566	164	276537	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.301	188	533069	20.000	ng/ul	0.00
79) Chrysene-d12	21.465	240	387802	20.000	ng/ul	0.00
88) Perylene-d12	23.859	264	392447	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	211457m	84.161	ng/uL	-0.03
4) Pyridine-d5	3.754	84	5010m	0.714	ng/ul	0.04
7) Phenol-d5	7.084	99	50690	6.106	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	192521	38.040	ng/ul	0.00
11) 2-Chlorophenol-d4	7.454	132	176477	26.534	ng/ul	0.00
15) 4-Methylphenol-d8	8.636	113	106963	16.260	ng/ul	0.00
21) Nitrobenzene-d5	9.089	128	127381	36.969	ng/ul	0.00
24) 2-Nitrophenol-d4	9.819	143	132879	35.712	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	209135	31.059	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131	233500	25.112	ng/ul	0.00
46) Dimethylphthalate-d6	13.977	166	811336	39.262	ng/ul	0.00
49) Acenaphthylene-d8	14.260	160	968426	38.256	ng/ul	0.00
54) 4-Nitrophenol-d4	14.760	143	13448	3.809	ng/ul	0.00
60) Fluorene-d10	15.554	176	678025	39.295	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200	104291	31.163	ng/ul	0.00
73) Anthracene-d10	17.401	188	1034669	40.530	ng/ul	0.00
81) Pyrene-d10	19.683	212	1028221	44.910	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.700	264	839287	40.717	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.325	88	61036	22.262	ng/uL#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033940.D
Acq On : 01 Feb 2022 15:34
Operator : CG/JU
Sample : N1273-20
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL8

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 01 23:59:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

