




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033945.D
 Acq On : 01 Feb 2022 18:32
 Operator : CG/JU
 Sample : N1328-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HM2

Manual IntegrationsAPPROVED

Quant Time: Feb 02 00:01:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

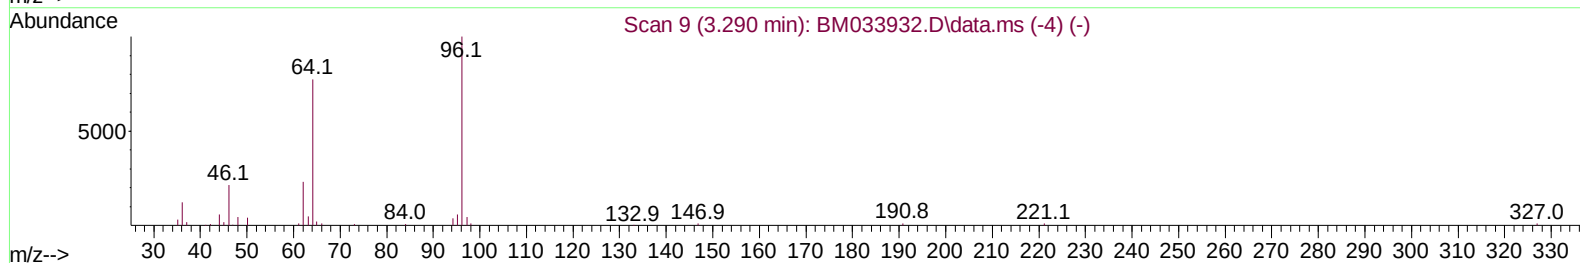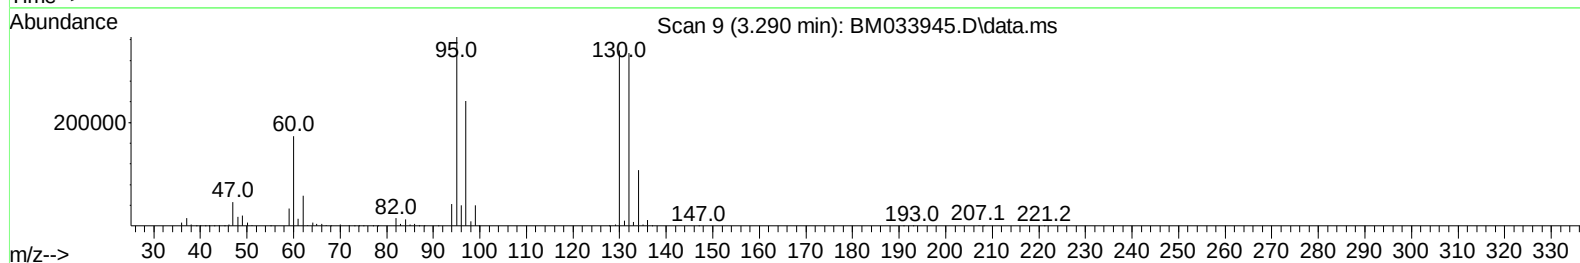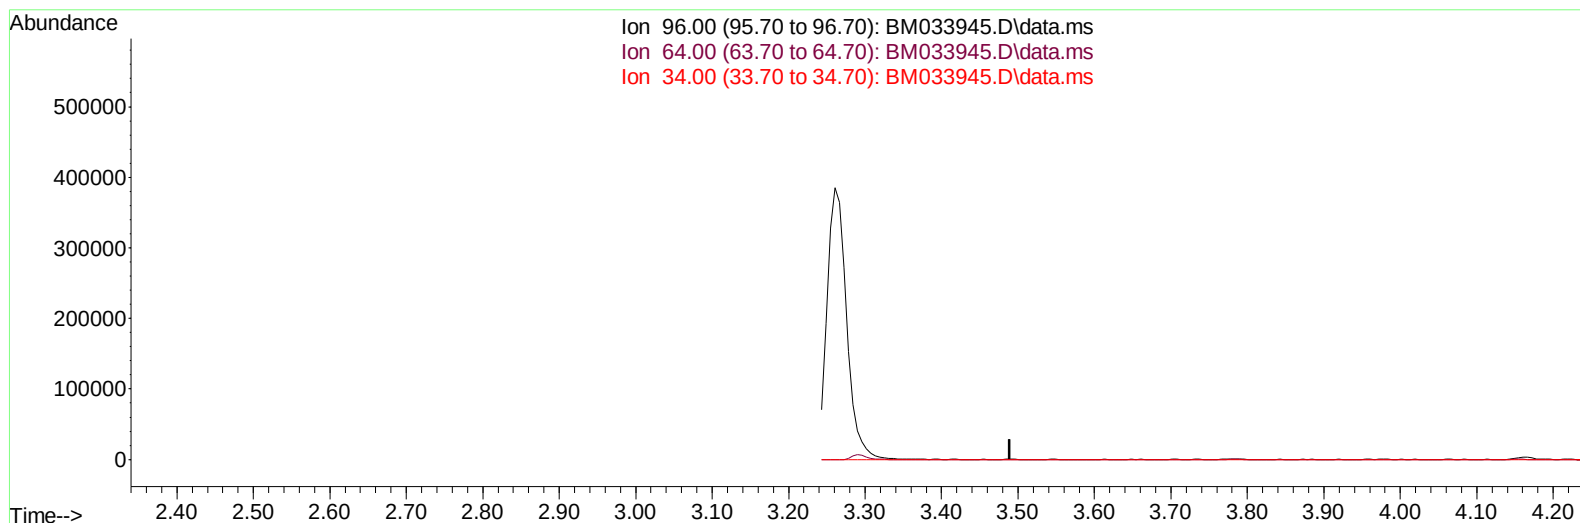

TIC: BM033945.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.290min (-3.290) 0.00 ng/uL

response 0

Ion	Exp%	Act%
96.00	100.00	0.00
64.00	74.20	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033945.D
 Acq On : 01 Feb 2022 18:32
 Operator : CG/JU
 Sample : N1328-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HM2

Manual IntegrationsAPPROVED

Quant Time: Feb 02 00:01:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

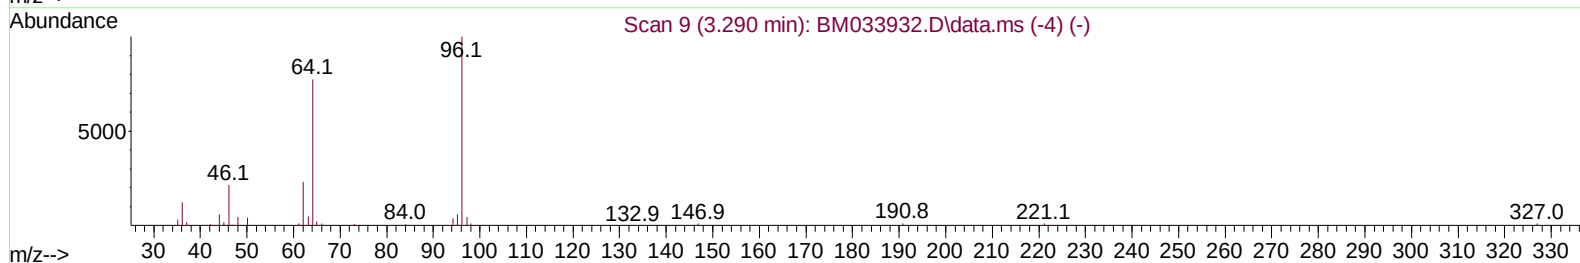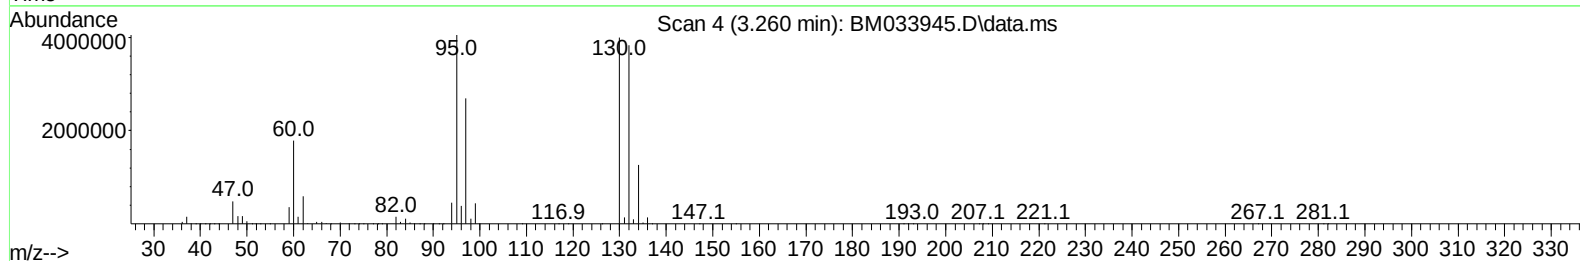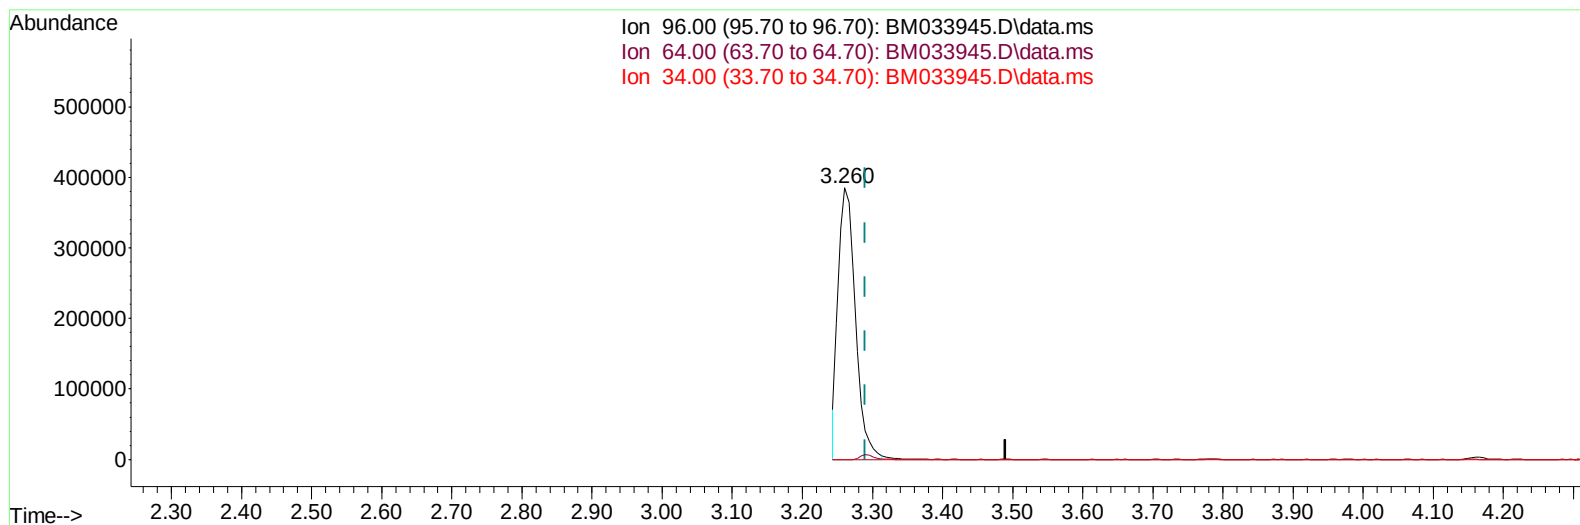

TIC: BM033945.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.260min (-0.030) 250.78 ng/uL m

response 658867

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033945.D
Acq On : 01 Feb 2022 18:32
Operator : CG/JU
Sample : N1328-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HM2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 02 00:01:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

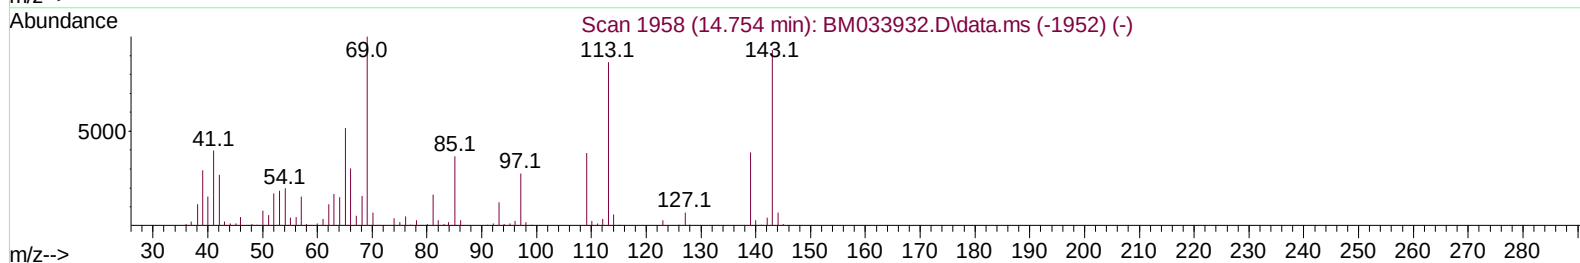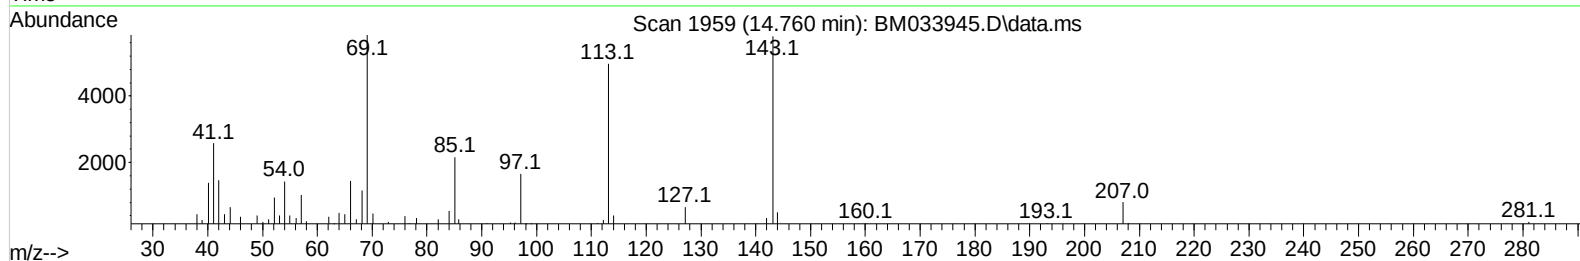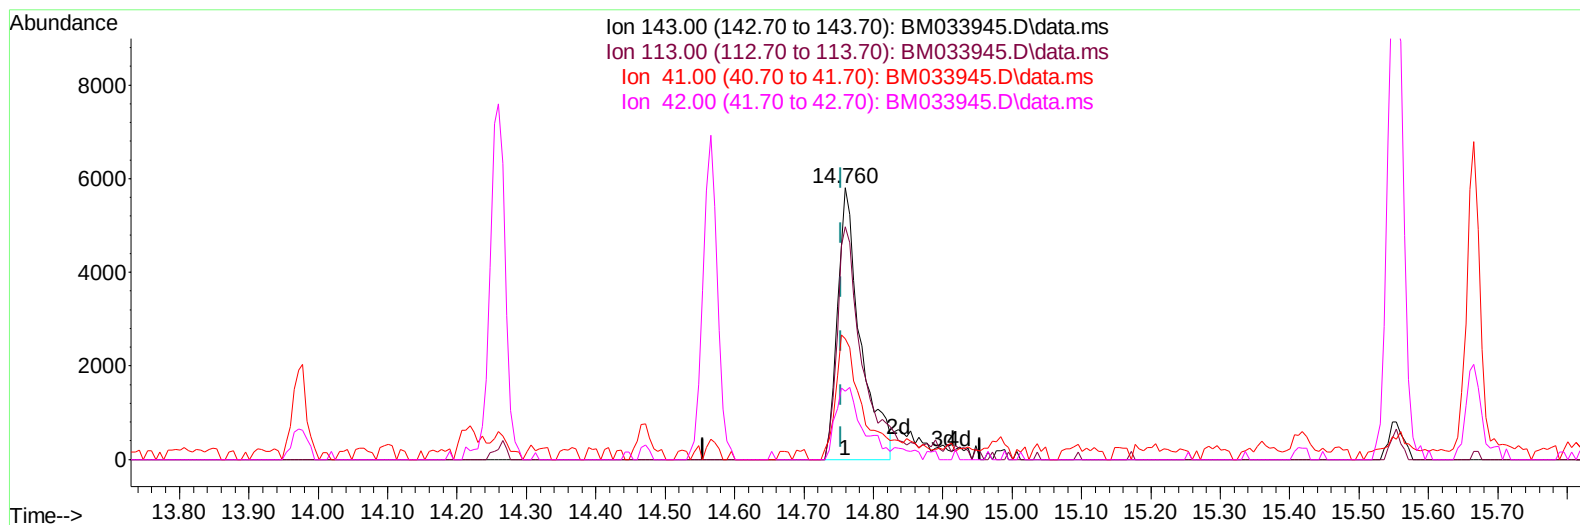

TIC: BM033945.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.760min (+ 0.006) 3.91 ng/ul m

response 13293

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	85.66
41.00	57.20	44.43#
42.00	39.50	25.15#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033945.D
 Acq On : 01 Feb 2022 18:32
 Operator : CG/JU
 Sample : N1328-03
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHM2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 02 00:01:39 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	103616	20.000	ng/ul	0.00
20) Naphthalene-d8	10.742	136	429870	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.566	164	266464	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.301	188	506102	20.000	ng/ul	0.00
79) Chrysene-d12	21.465	240	418110	20.000	ng/ul	0.00
88) Perylene-d12	23.859	264	425460	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	658867m	250.782	ng/uL	-0.03
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.084	99	53124	6.120	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	179186	33.859	ng/ul	0.00
11) 2-Chlorophenol-d4	7.454	132	174821	25.137	ng/ul	0.00
15) 4-Methylphenol-d8	8.637	113	104236	15.154	ng/ul	0.00
21) Nitrobenzene-d5	9.089	128	113306	32.849	ng/ul	0.00
24) 2-Nitrophenol-d4	9.813	143	118507	31.815	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	183939	27.288	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131	182262	19.581	ng/ul	0.00
46) Dimethylphthalate-d6	13.977	166	708940	35.604	ng/ul	0.00
49) Acenaphthylene-d8	14.260	160	825441	33.840	ng/ul	0.00
54) 4-Nitrophenol-d4	14.760	143	13293m	3.908	ng/ul	0.00
60) Fluorene-d10	15.554	176	589051	35.429	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.666	200	91223	28.711	ng/ul	0.00
73) Anthracene-d10	17.401	188	915516	37.773	ng/ul	0.00
81) Pyrene-d10	19.683	212	969222	39.265	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.700	264	856034	38.307	ng/ul	0.00
Target Compounds						
					Qvalue	
2) 1,4-Dioxane	3.325	88	728543	254.116	ng/ul#	86

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033945.D
Acq On : 01 Feb 2022 18:32
Operator : CG/JU
Sample : N1328-03
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HM2

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 02 00:01:39 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

