




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033955.D
Acq On : 02 Feb 2022 01:02
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q04

Manual IntegrationsAPPROVED

Quant Time: Feb 02 01:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

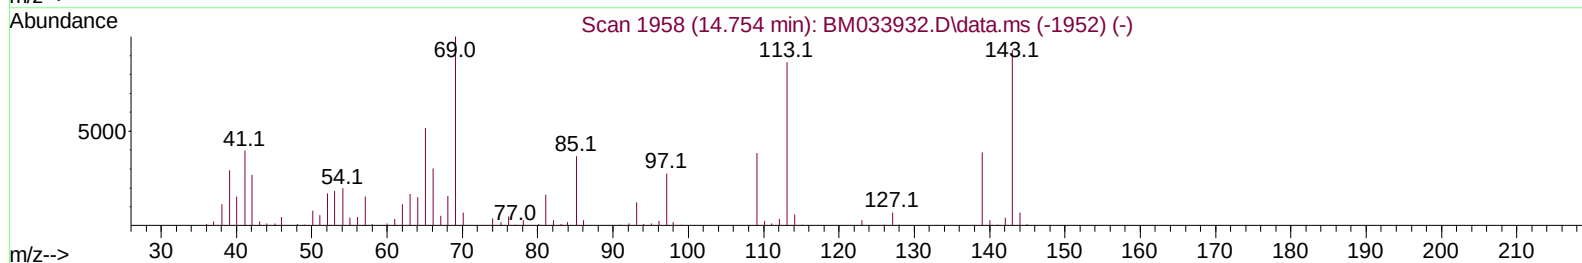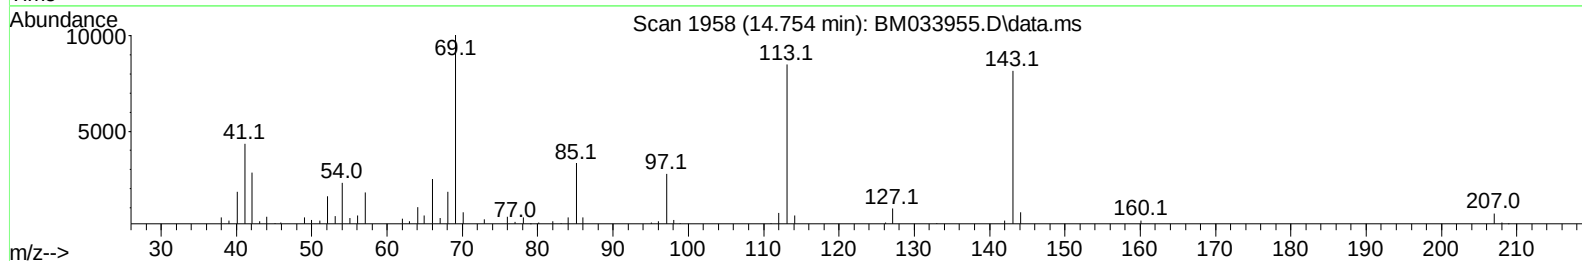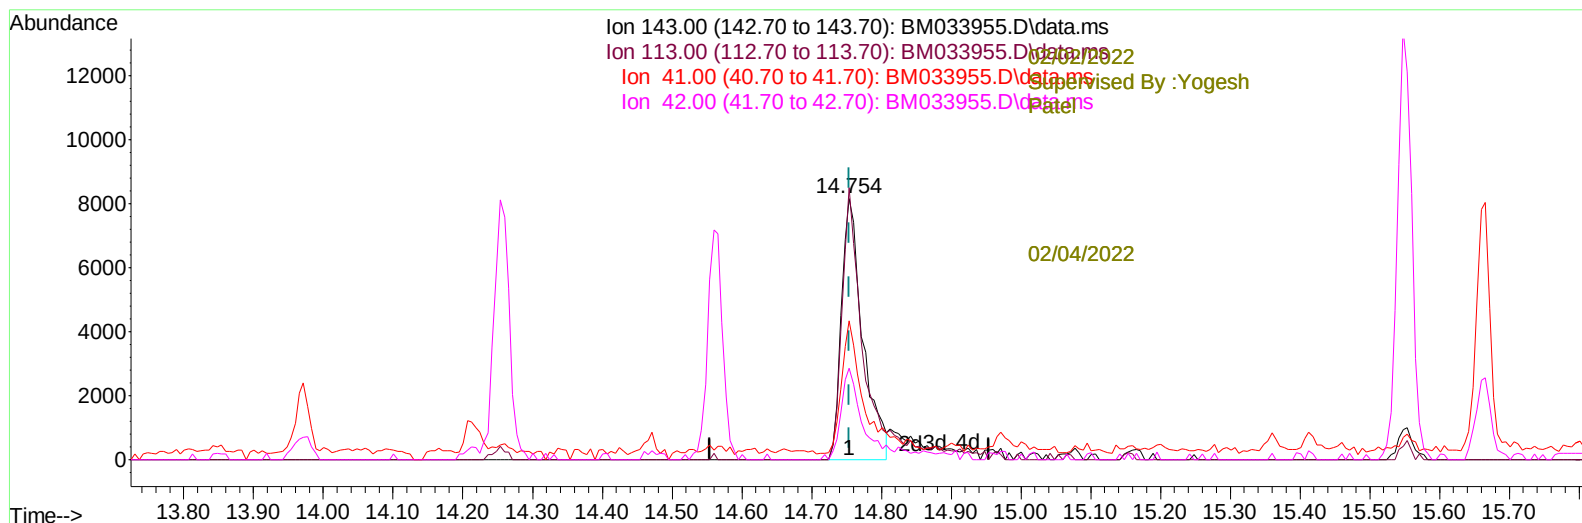

TIC: BM033955.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.754min (-0.000) 4.33 ng/u1

response 17336

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	104.04
41.00	57.20	53.19
42.00	39.50	34.86




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033955.D
Acq On : 02 Feb 2022 01:02
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q04

Manual IntegrationsAPPROVED

Quant Time: Feb 02 01:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut
Upadhyay

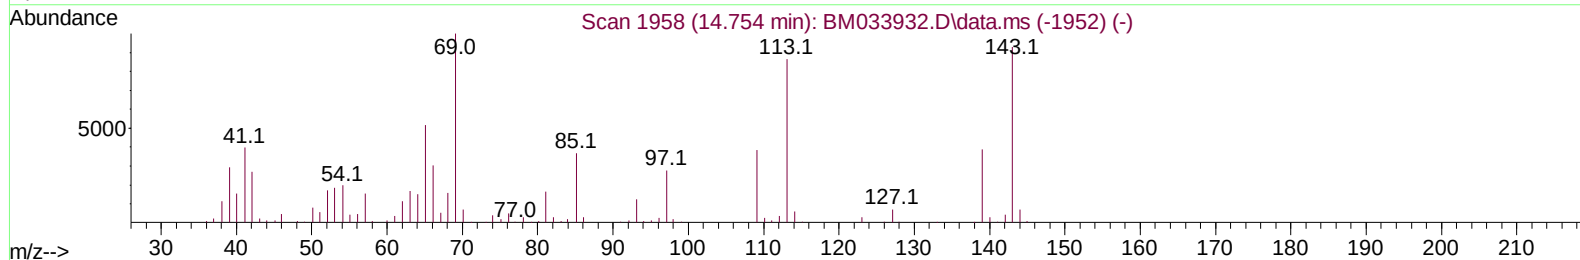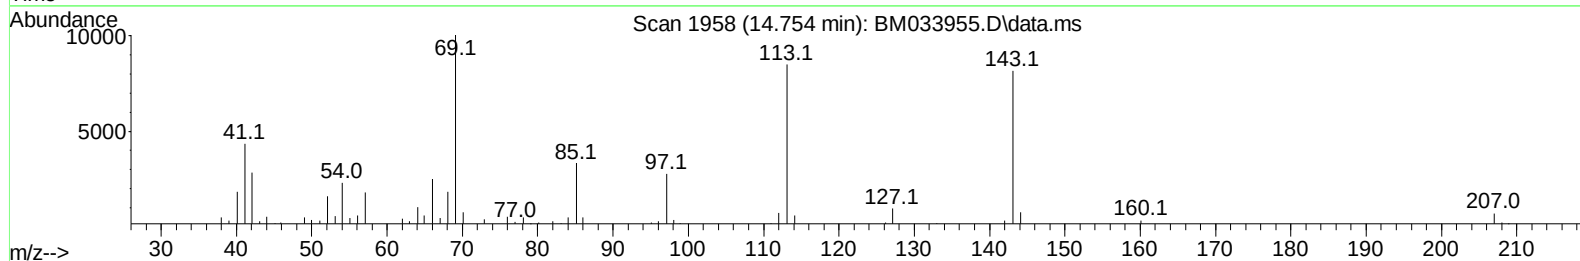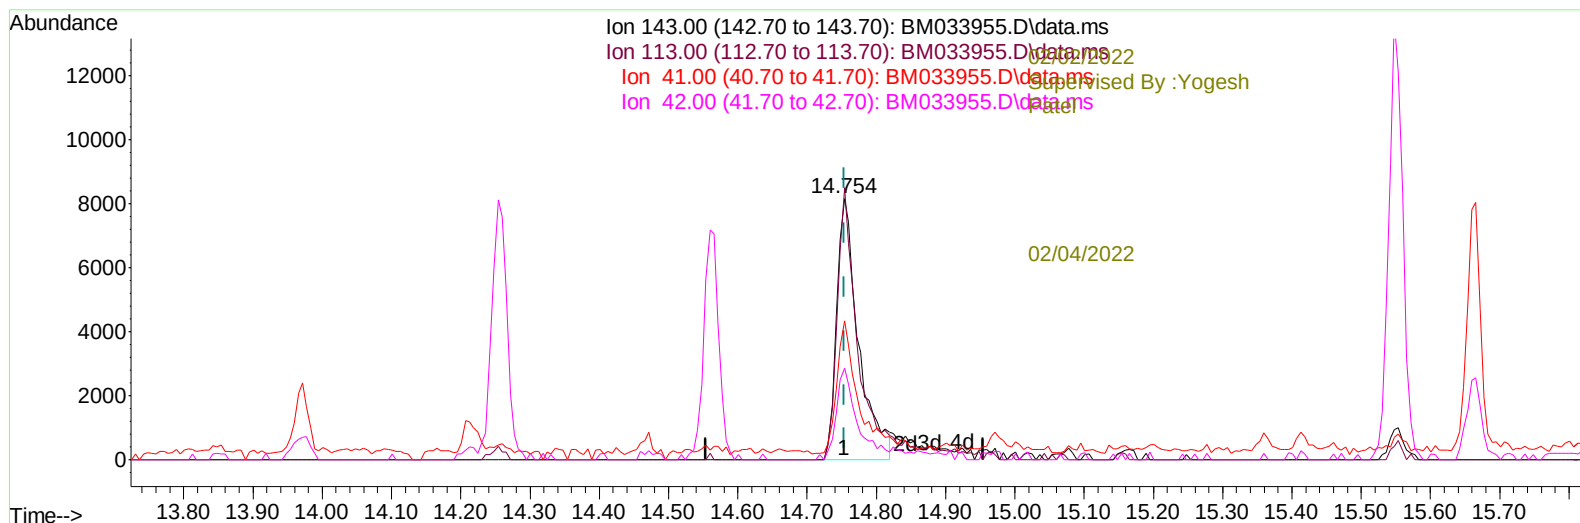

TIC: BM033955.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.754min (-0.000) 4.49 ng/ul m

response 17970

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	104.04
41.00	57.20	53.19
42.00	39.50	34.86

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033955.D
 Acq On : 02 Feb 2022 01:02
 Operator : CG/JU
 Sample : N1307-06
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q04

Manual IntegrationsAPPROVED

Quant Time: Feb 02 01:52:55 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut
 Upadhyay

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
-----02/02/2022							
Supervised By :Yogesh Patel							

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.925	152		122139	20.000	ng/ul	0.00
20) Naphthalene-d8	10.736	136		512464	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.566	164		313395	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.301	188		596103	20.000	ng/ul	0.00
79) Chrysene-d12	21.459	240		516602	20.000	ng/ul	0.00
88) Perylene-d12	23.847	264		517293	20.000	ng/ul	-0.01
-----01/04/2022							
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.290	96		12463	4.024	ng/uL	0.00
4) Pyridine-d5	3.731	84		21734	2.514	ng/ul	0.01
7) Phenol-d5	7.084	99		65855	6.436	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67		192979	30.935	ng/ul	0.00
11) 2-Chlorophenol-d4	7.454	132		198975	24.271	ng/ul	0.00
15) 4-Methylphenol-d8	8.631	113		123308	15.208	ng/ul	-0.01
21) Nitrobenzene-d5	9.089	128		126213	30.694	ng/ul	0.00
24) 2-Nitrophenol-d4	9.813	143		130748	29.444	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.354	165		205862	25.619	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131		157290	14.175	ng/ul	0.00
46) Dimethylphthalate-d6	13.971	166		829423	35.417	ng/ul	0.00
49) Acenaphthylene-d8	14.254	160		923837	32.202	ng/ul	0.00
54) 4-Nitrophenol-d4	14.754	143		17970m	4.491	ng/ul	0.00
60) Fluorene-d10	15.554	176		677358	34.639	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200		114196	30.515	ng/ul	0.00
73) Anthracene-d10	17.395	188		1078689	37.786	ng/ul	0.00
81) Pyrene-d10	19.683	212		1157144	37.940	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.694	264		1039287	38.251	ng/ul	-0.01

Target Compounds						Qvalue	
71) Pentachlorophenol	16.954	266		84079	17.800	ng/ul	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033955.D
Acq On : 02 Feb 2022 01:02
Operator : CG/JU
Sample : N1307-06
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q04

Manual IntegrationsAPPROVED

Reviewed By :Jagrut
Upadhyay

Quant Time: Feb 02 01:52:55 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

