




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033968.D
 Acq On : 02 Feb 2022 10:55
 Operator : CG/JU
 Sample : N1273-17DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 00:11:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2022
 Supervised By :Yogesh Patel 02/04/2022

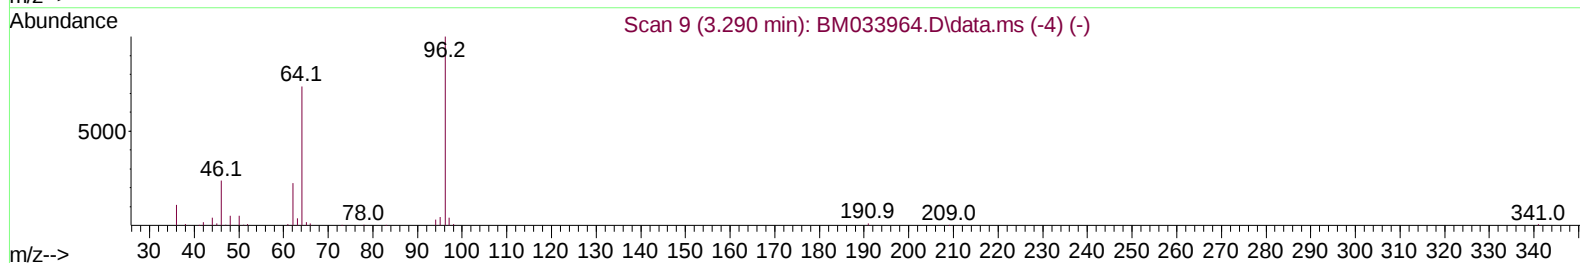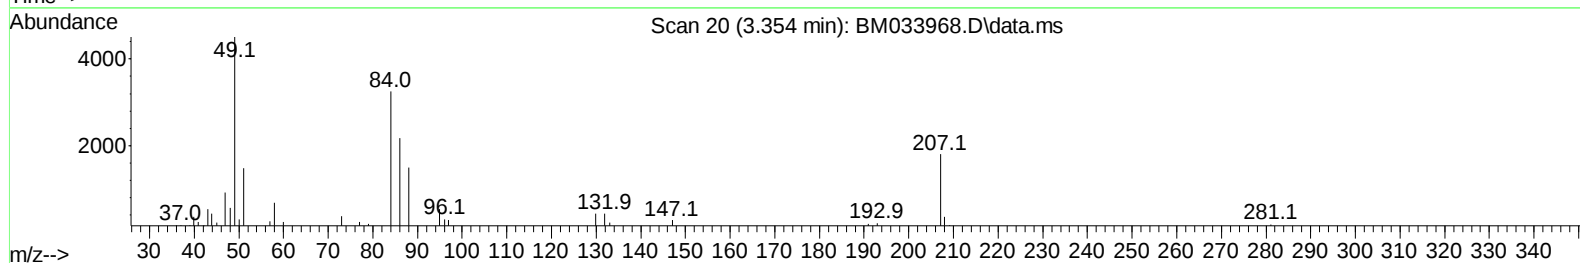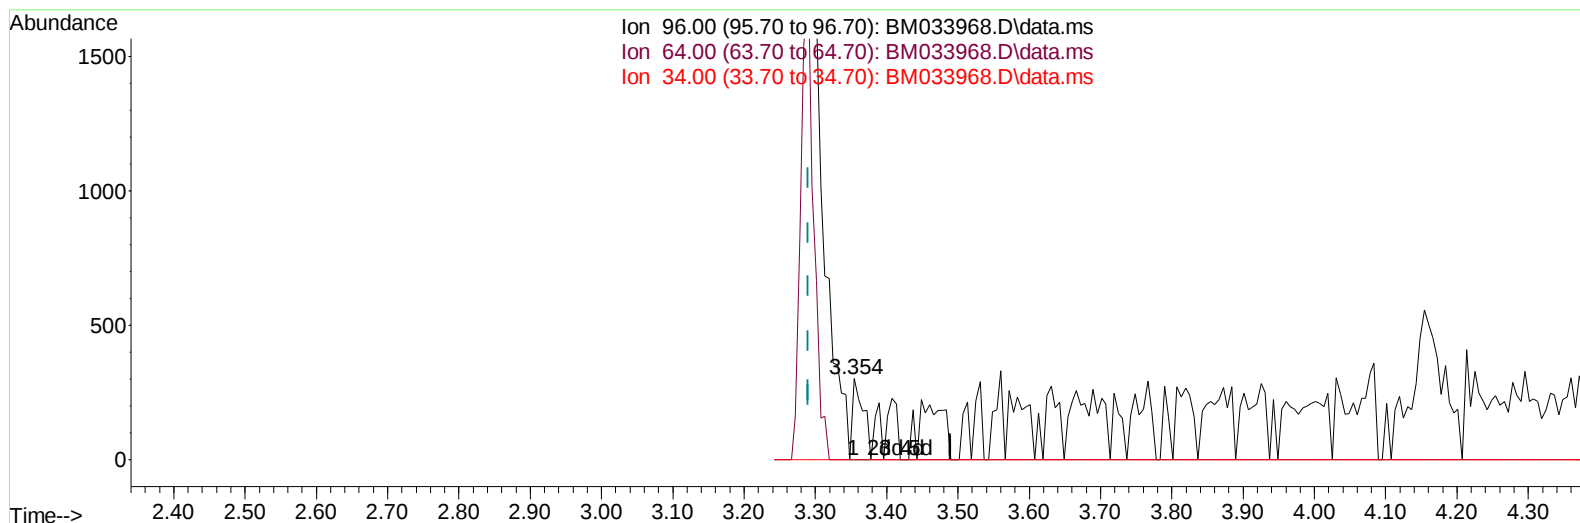

TIC: BM033968.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.354min (+ 0.064) 0.11 ng/uL

response 313

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033968.D
 Acq On : 02 Feb 2022 10:55
 Operator : CG/JU
 Sample : N1273-17DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 00:11:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2022
 Supervised By :Yogesh Patel 02/04/2022

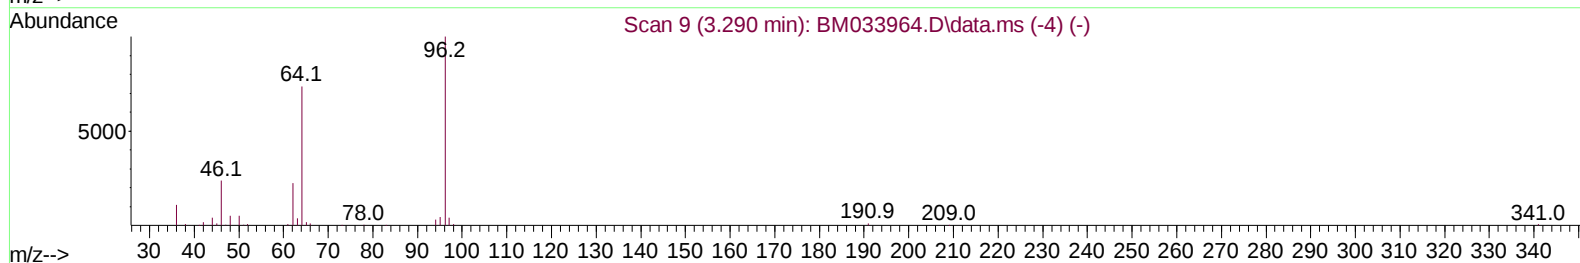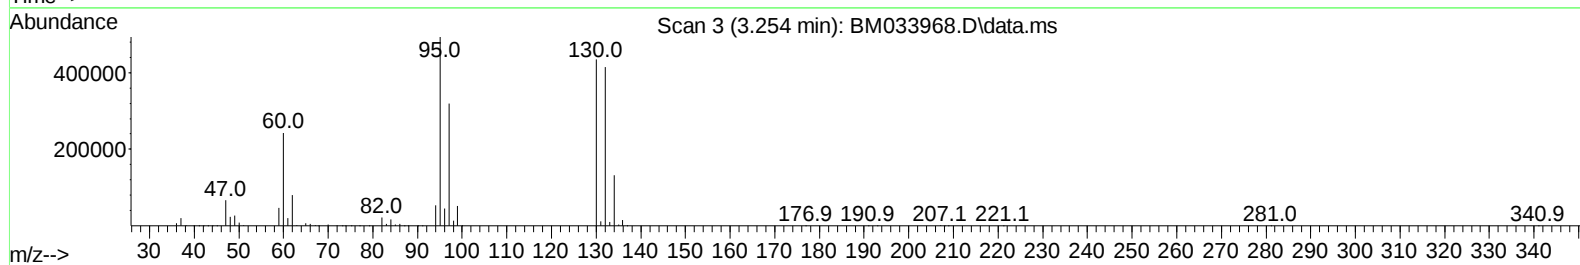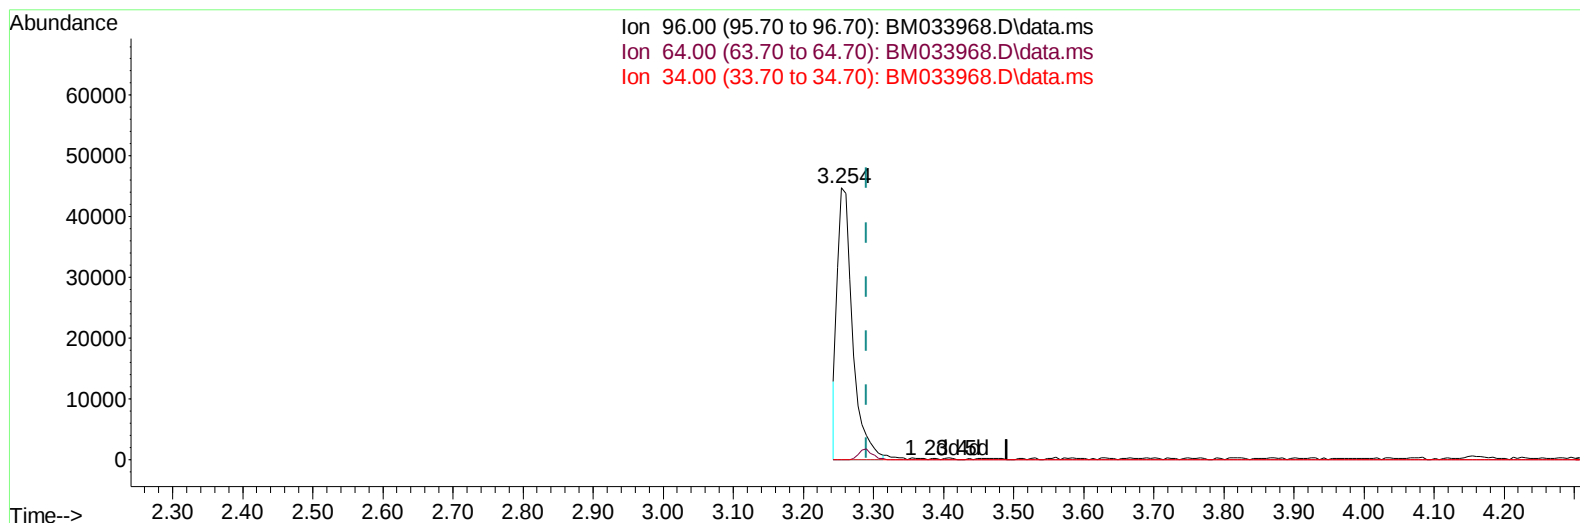

TIC: BM033968.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.254min (-0.036) 23.02 ng/uL m

response 67677

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	0.00#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033968.D
 Acq On : 02 Feb 2022 10:55
 Operator : CG/JU
 Sample : N1273-17DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 00:11:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2022
 Supervised By :Yogesh Patel 02/04/2022

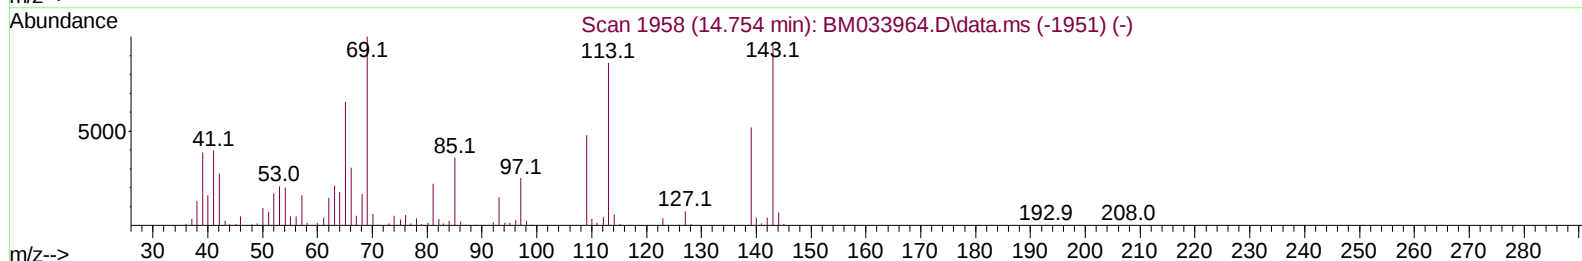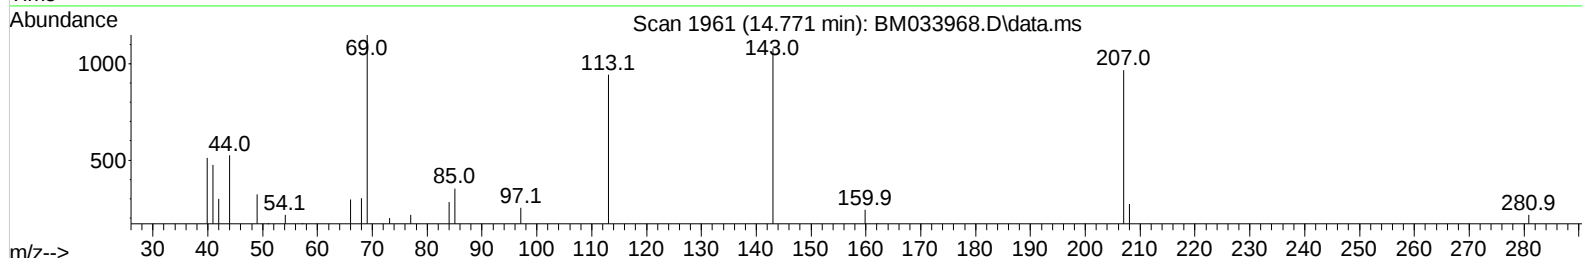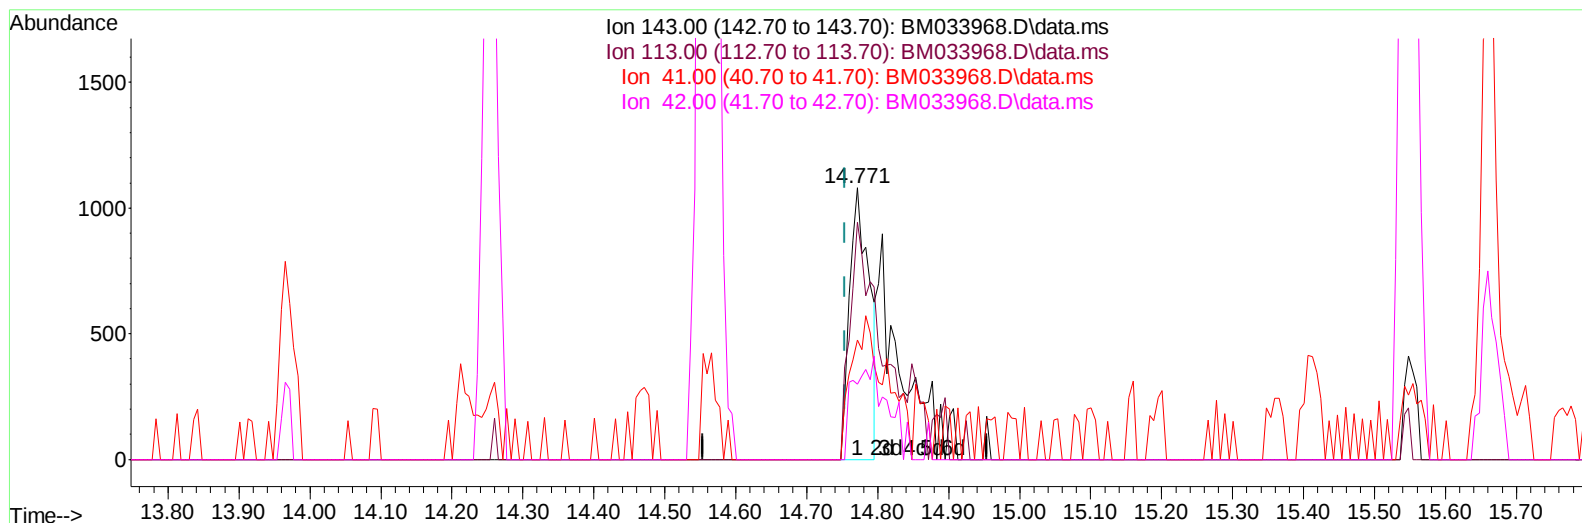

TIC: BM033968.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.771min (+ 0.018) 0.44 ng/ul

response 2054

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	87.31
41.00	57.20	43.98#
42.00	39.50	27.69#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033968.D
 Acq On : 02 Feb 2022 10:55
 Operator : CG/JU
 Sample : N1273-17DL 5X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0HL5DL

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 02/03/2022
 Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 03 00:11:45 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Dichlorobenzene-d4	7.925	152		115964	20.000	ng/ul	0.00
20) Naphthalene-d8	10.736	136		508896	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.560	164		361762	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.295	188		778583	20.000	ng/ul	-0.01
79) Chrysene-d12	21.459	240		615649	20.000	ng/ul	0.00
88) Perylene-d12	23.847	264		542014	20.000	ng/ul	-0.01
System Monitoring Compounds							
3) 1,4-Dioxane-d8	3.254	96		67677m	23.017	ng/uL	-0.04
4) Pyridine-d5	0.000	84		0d	0.000	ng/ul	
7) Phenol-d5	7.084	99		14033	1.444	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67		54069	9.129	ng/ul	0.00
11) 2-Chlorophenol-d4	7.454	132		50885	6.538	ng/ul	0.00
15) 4-Methylphenol-d8	8.631	113		27729	3.602	ng/ul	-0.01
21) Nitrobenzene-d5	9.089	128		32807	8.034	ng/ul	0.00
24) 2-Nitrophenol-d4	9.813	143		31954	7.246	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.354	165		52723	6.607	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131		11471	1.041	ng/ul	0.00
46) Dimethylphthalate-d6	13.971	166		262313	9.703	ng/ul	0.00
49) Acenaphthylene-d8	14.254	160		257850	7.786	ng/ul	0.00
54) 4-Nitrophenol-d4	14.771	143		3398m	0.736	ng/ul	0.02
60) Fluorene-d10	15.548	176		214555	9.505	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200		29272	5.989	ng/ul	0.00
73) Anthracene-d10	17.395	188		365762	9.810	ng/ul	0.00
81) Pyrene-d10	19.677	212		405184	11.148	ng/ul	-0.01
92) Benzo(a)pyrene-d12	23.694	264		284041	9.977	ng/ul	-0.01
Target Compounds							
						Qvalue	
2) 1,4-Dioxane	3.325	88		44306	13.808	ng/ul#	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033968.D
Acq On : 02 Feb 2022 10:55
Operator : CG/JU
Sample : N1273-17DL 5X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0HL5DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 00:11:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/03/2022
Supervised By :Yogesh Patel 02/04/2022

