




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033972.D
 Acq On : 02 Feb 2022 13:32
 Operator : CG/JU
 Sample : N1307-07DL 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q47DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 16:23:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2022
 Supervised By :Yogesh Patel 02/08/2022

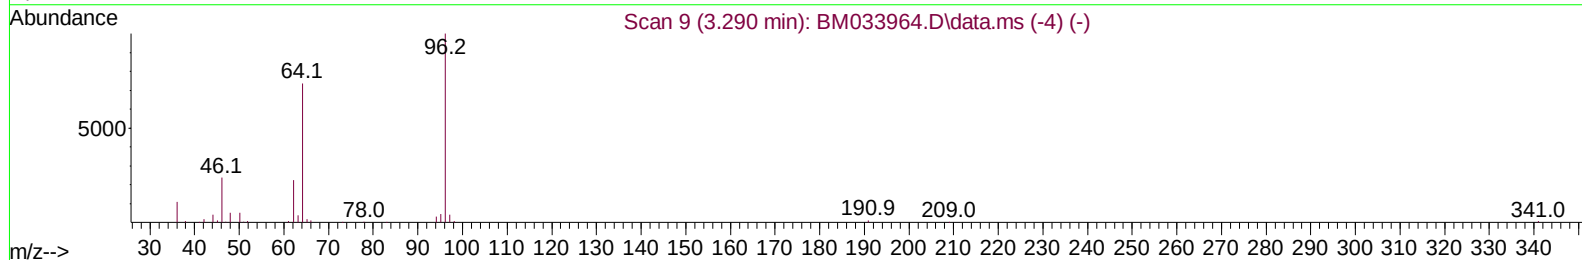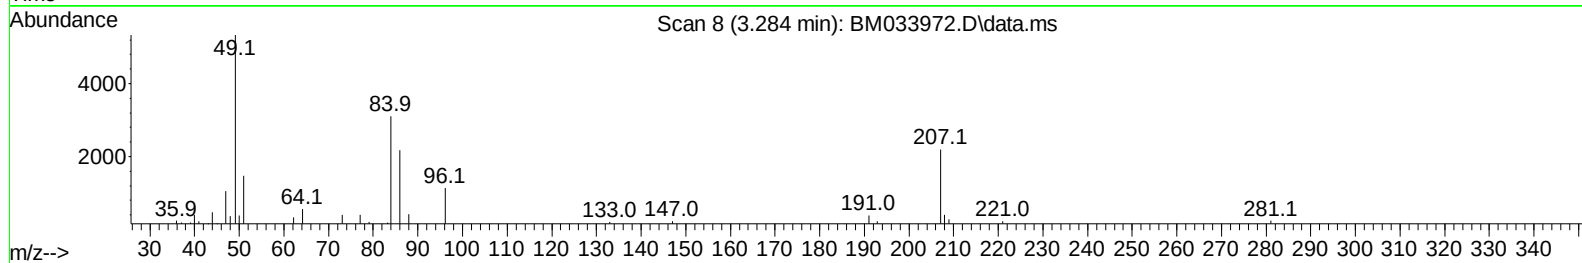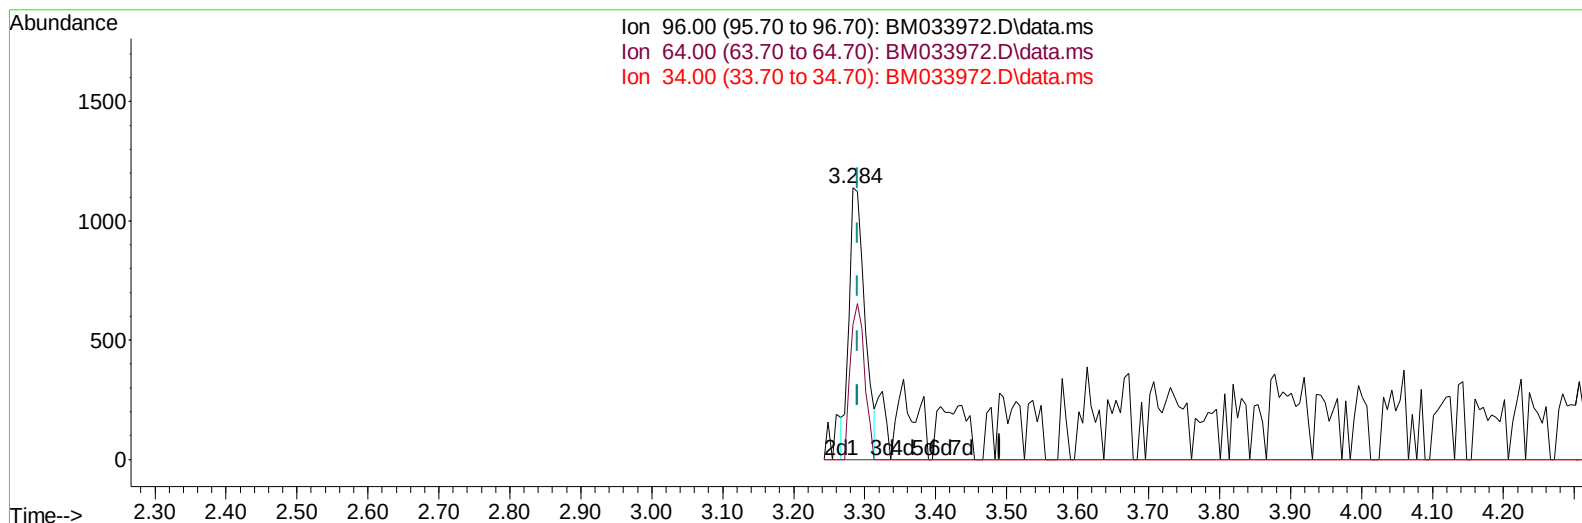

TIC: BM033972.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.284min (-0.006) 0.56 ng/uL

response 1738

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	49.65#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033972.D
 Acq On : 02 Feb 2022 13:32
 Operator : CG/JU
 Sample : N1307-07DL 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q47DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 16:23:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2022
 Supervised By :Yogesh Patel 02/08/2022

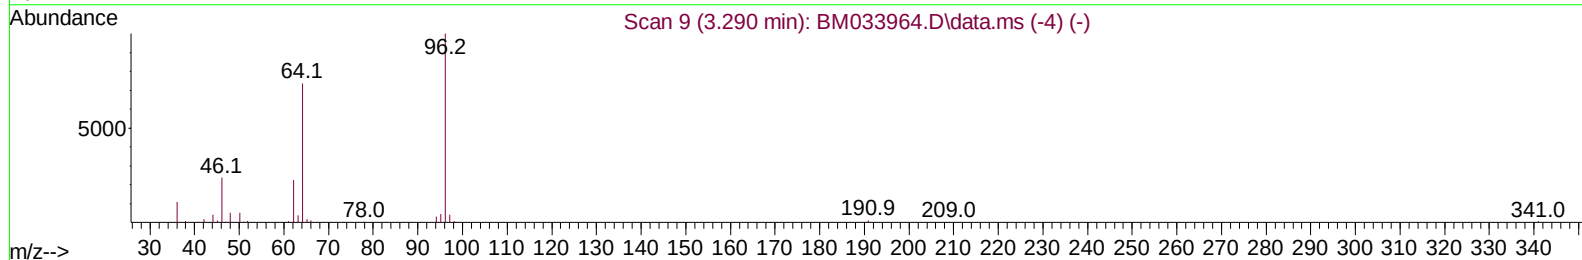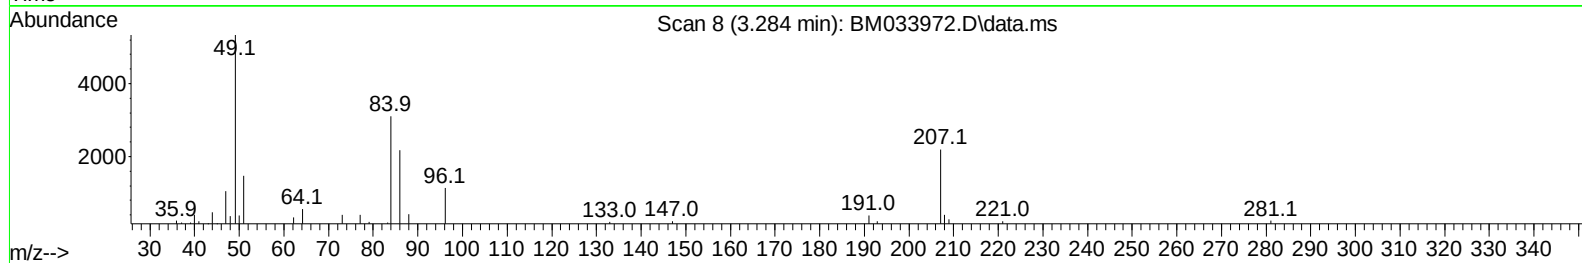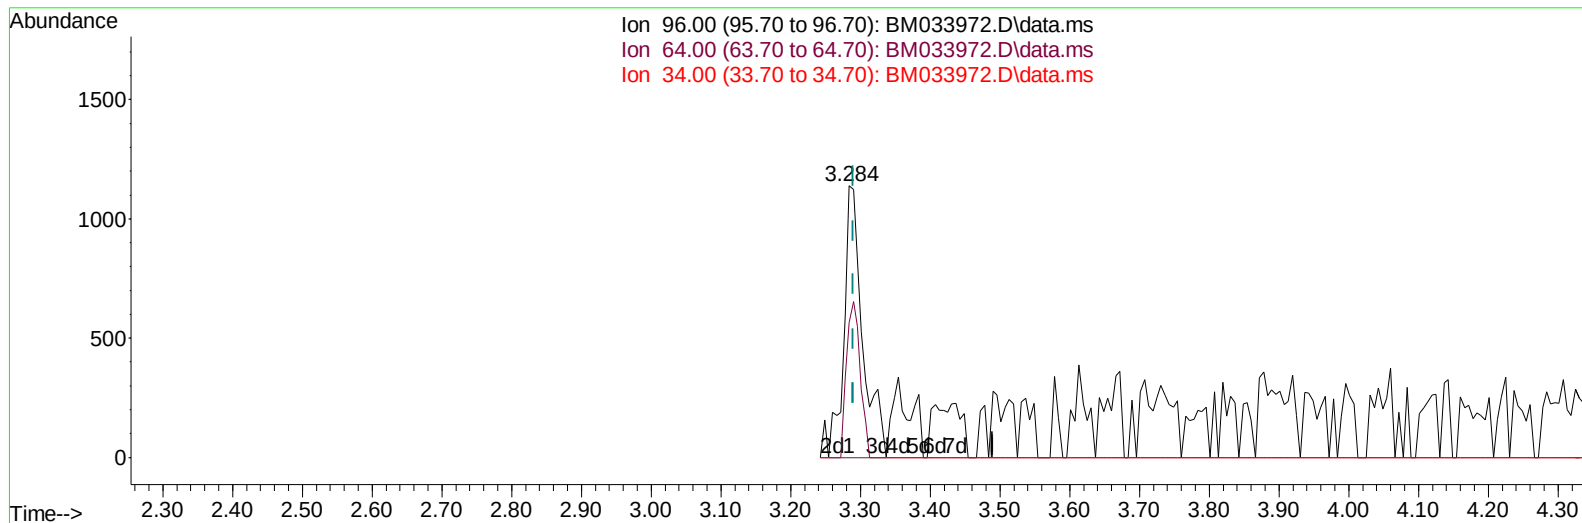

TIC: BM033972.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.284min (-0.006) 0.69 ng/uL m

response 2113

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	74.20	49.65#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033972.D
Acq On : 02 Feb 2022 13:32
Operator : CG/JU
Sample : N1307-07DL 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q47DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 16:23:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2022
Supervised By :Yogesh Patel 02/08/2022

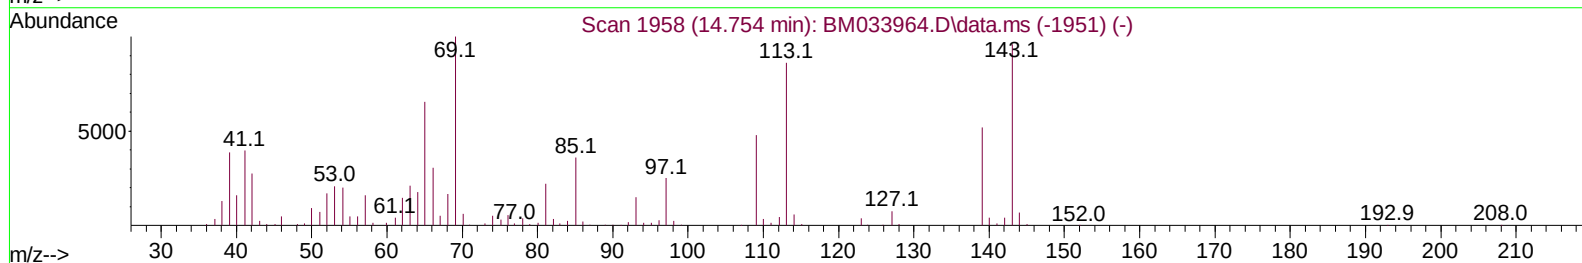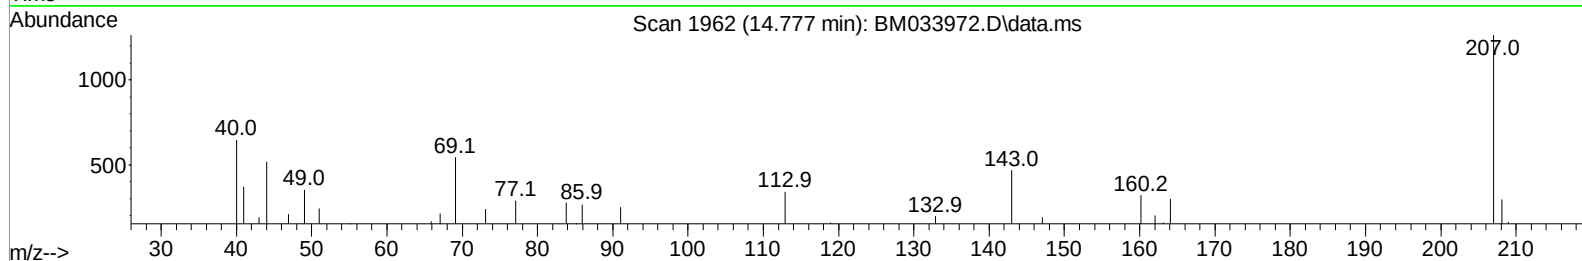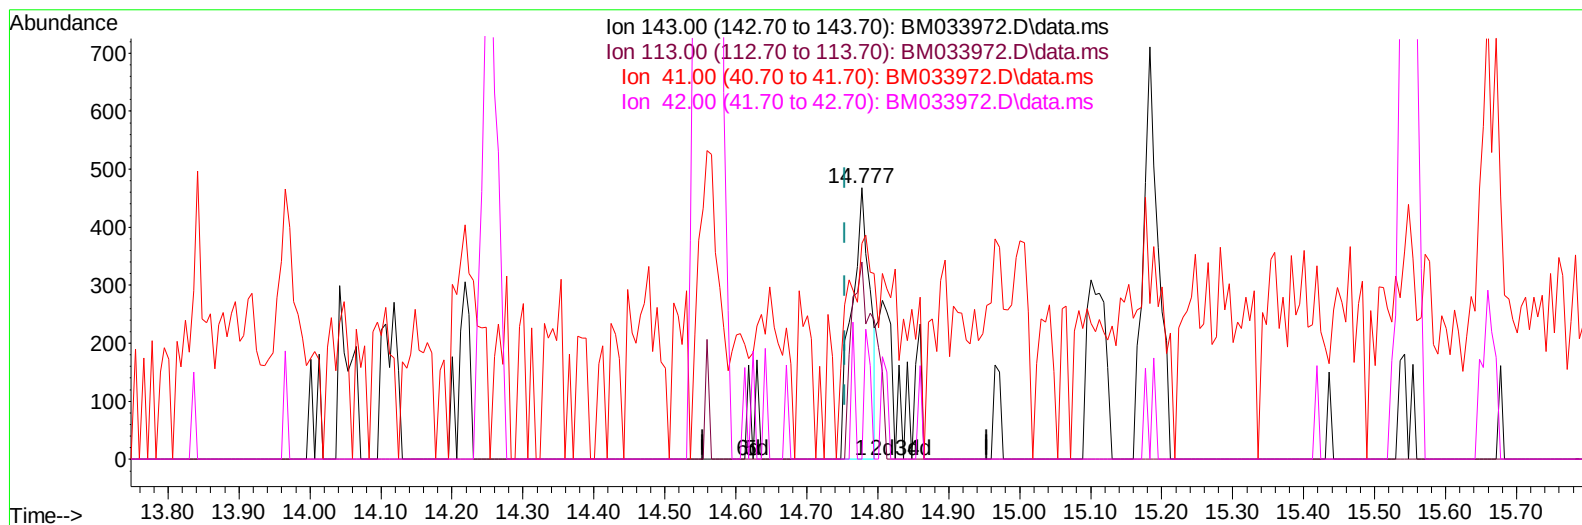

TIC: BM033972.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.777min (+ 0.023) 0.17 ng/ul

response 840

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	105.00	72.65#
41.00	57.20	79.49#
42.00	39.50	0.00#

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033972.D
 Acq On : 02 Feb 2022 13:32
 Operator : CG/JU
 Sample : N1307-07DL 10X
 Misc :
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q47DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 16:23:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2022
 Supervised By :Yogesh Patel 02/08/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	121535	20.000	ng/ul	0.00
20) Naphthalene-d8	10.736	136	536742	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.560	164	379026	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.301	188	786696	20.000	ng/ul	0.00
79) Chrysene-d12	21.459	240	600437	20.000	ng/ul	0.00
88) Perylene-d12	23.847	264	548506	20.000	ng/ul	-0.01
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.284	96	2113m	0.686	ng/uL	0.00
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	7.084	99	6118	0.601	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	18460	2.974	ng/ul	0.00
11) 2-Chlorophenol-d4	7.454	132	17059	2.091	ng/ul	0.00
15) 4-Methylphenol-d8	8.636	113	10783	1.336	ng/ul	0.00
21) Nitrobenzene-d5	9.089	128	10592	2.459	ng/ul	0.00
24) 2-Nitrophenol-d4	9.819	143	9529	2.049	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	17685	2.101	ng/ul	0.00
31) 4-Chloroaniline-d4	10.872	131	23194	1.996	ng/ul	0.00
46) Dimethylphthalate-d6	13.971	166	94694	3.343	ng/ul	0.00
49) Acenaphthylene-d8	14.254	160	96256	2.774	ng/ul	0.00
54) 4-Nitrophenol-d4	14.777	143	1193m	0.247	ng/ul	0.02
60) Fluorene-d10	15.548	176	78424	3.316	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200	8772	1.776	ng/ul	0.00
73) Anthracene-d10	17.395	188	120746	3.205	ng/ul	0.00
81) Pyrene-d10	19.683	212	126942	3.581	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.694	264	88991	3.089	ng/ul	-0.01
Target Compounds						
					Qvalue	
58) 2,3,4,6-Tetrachlorophenol	15.183	232	27980	4.271	ng/ul#	95
71) Pentachlorophenol	16.954	266	533794	85.630	ng/ul	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033972.D
Acq On : 02 Feb 2022 13:32
Operator : CG/JU
Sample : N1307-07DL 10X
Misc :
ALS Vial : 43 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0Q47DL

Manual IntegrationsAPPROVED

Quant Time: Feb 03 16:23:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 02/07/2022
Supervised By :Yogesh Patel 02/08/2022

