

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033938.D
 Acq On : 01 Feb 2022 14:22
 Operator : CG/JU
 Sample : N1273-13
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL1

Quant Time: Feb 01 23:59:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	97504	20.000	ng/u1	0.00
20) Naphthalene-d8	10.742	136	419303	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.566	164	272452	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.301	188	529998	20.000	ng/u1	0.00
79) Chrysene-d12	21.465	240	394788	20.000	ng/u1	0.00
88) Perylene-d12	23.853	264	400480	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	11392	4.608	ng/uL	0.00
4) Pyridine-d5	3.731	84	31737	4.599	ng/u1	0.01
7) Phenol-d5	7.084	99	56751	6.947	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	187565	37.663	ng/u1	0.00
11) 2-Chlorophenol-d4	7.454	132	181733	27.769	ng/u1	0.00
15) 4-Methylphenol-d8	8.637	113	111318	17.198	ng/u1	0.00
21) Nitrobenzene-d5	9.090	128	122302	36.351	ng/u1	0.00
24) 2-Nitrophenol-d4	9.819	143	128221	35.291	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	199578	30.355	ng/u1	0.00
31) 4-Chloroaniline-d4	10.872	131	209965	23.126	ng/u1	0.00
46) Dimethylphthalate-d6	13.977	166	785404	38.577	ng/u1	0.00
49) Acenaphthylene-d8	14.260	160	924171	37.055	ng/u1	0.00
54) 4-Nitrophenol-d4	14.754	143	14781	4.249	ng/u1	0.00
60) Fluorene-d10	15.554	176	654134	38.478	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.666	200	108002	32.459	ng/u1	0.00
73) Anthracene-d10	17.401	188	1045704	41.199	ng/u1	0.00
81) Pyrene-d10	19.683	212	1066625	45.763	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.700	264	872887	41.497	ng/u1	0.00


Target Compounds					Qvalue	
2) 1,4-Dioxane	3.325	88	8526	3.160	ng/uL#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033938.D
Acq On : 01 Feb 2022 14:22
Operator : CG/JU
Sample : N1273-13
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL1

Quant Time: Feb 01 23:59:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

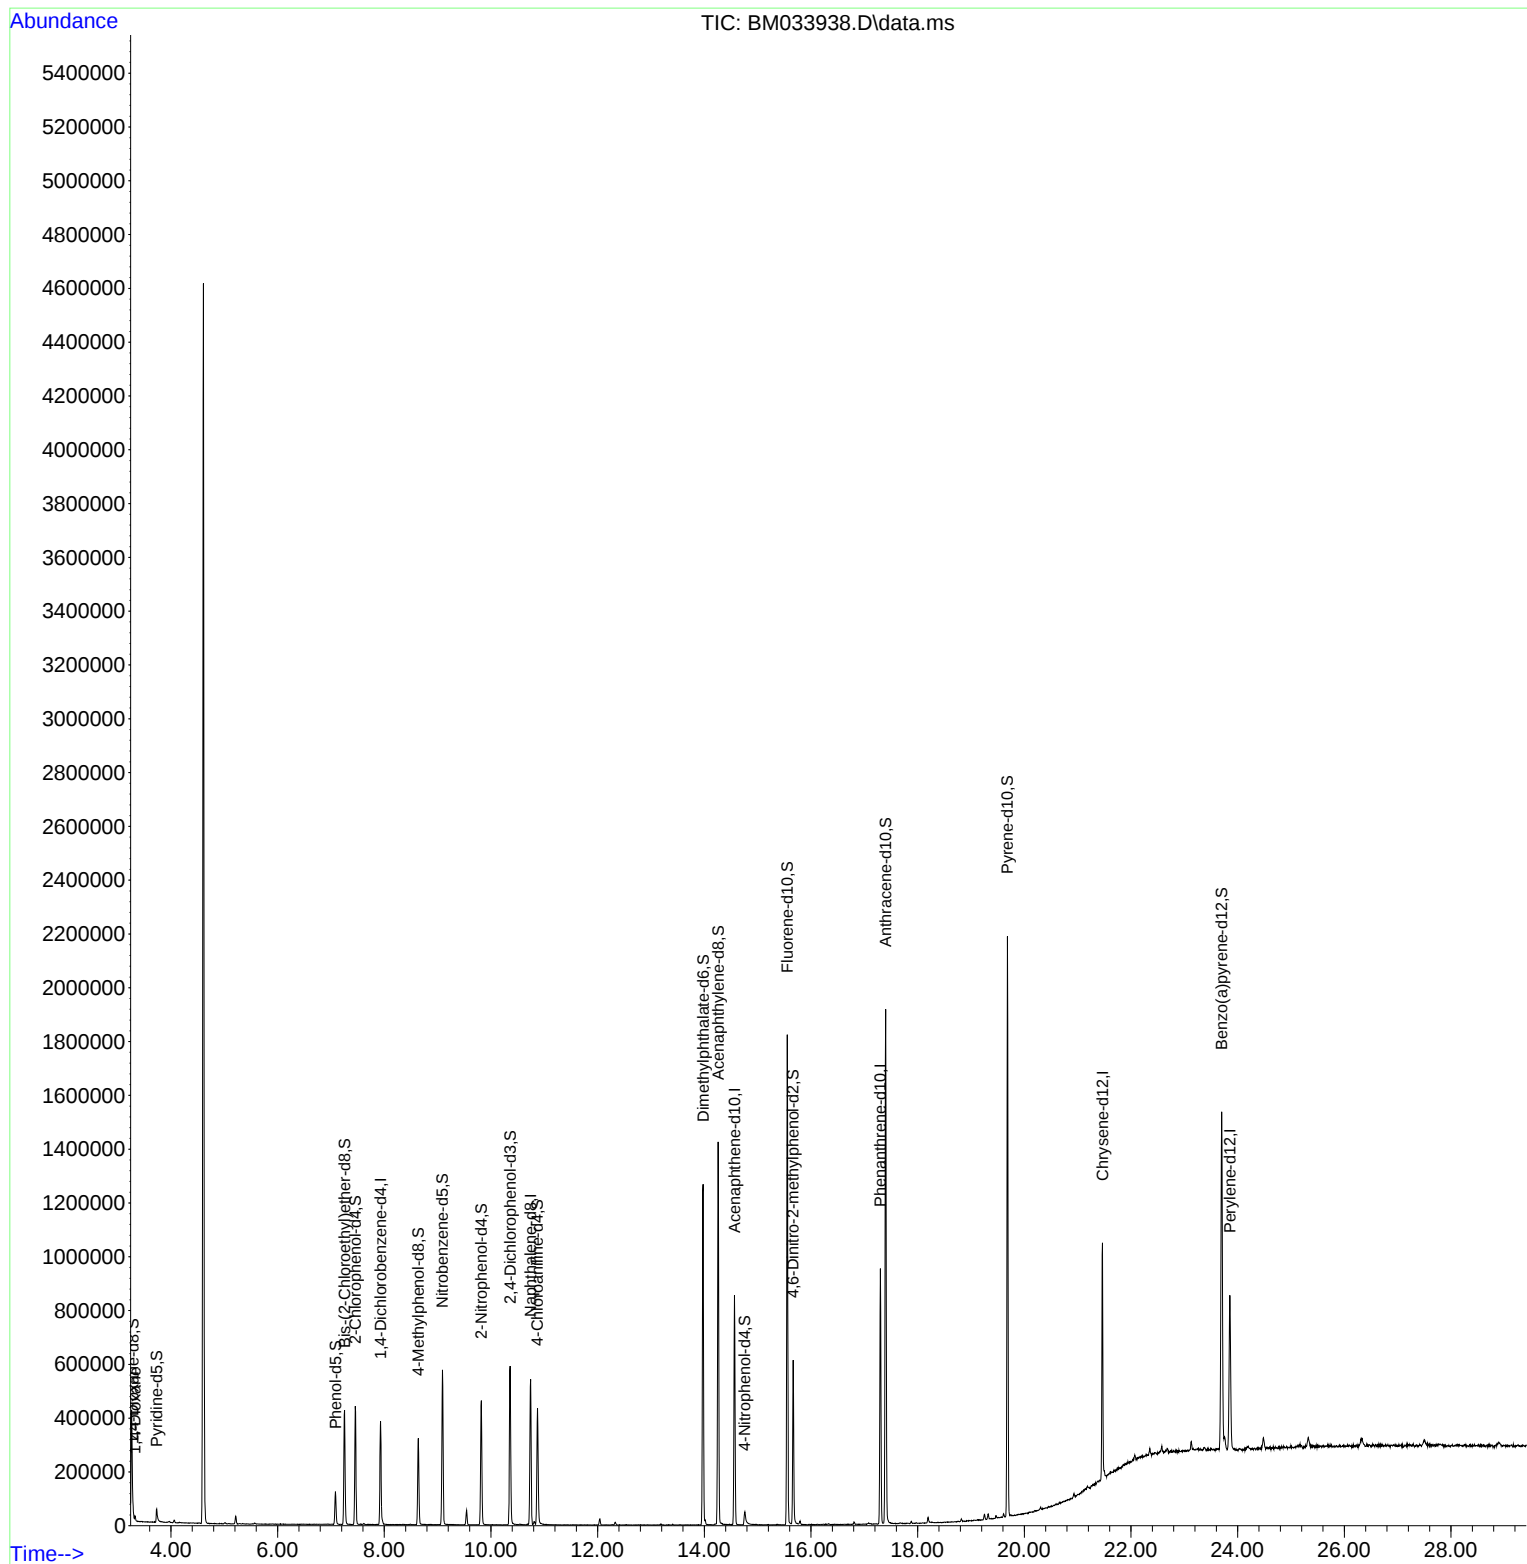

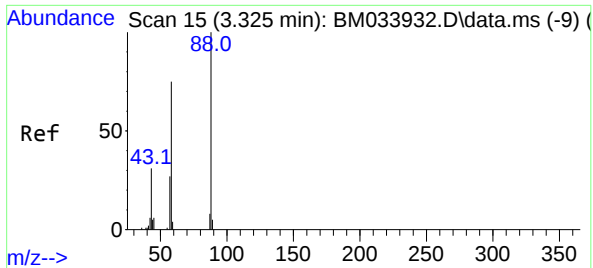

#2
 1,4-Dioxane
 Concen: 3.160 ng/uL
 RT: 3.325 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BM033938.D
 Acq: 01 Feb 2022 14:22

Instrument :
 BNA_M
 ClientSampleId :
 COHL1

Tgt Ion: 88 Resp: 8526

Ion	Ratio	Lower	Upper
88	100		
43	30.1	36.2	54.4#
58	79.6	68.5	102.7

