

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033941.D
 Acq On : 01 Feb 2022 16:09
 Operator : CG/JU
 Sample : N1273-18
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL6

Quant Time: Feb 01 23:59:59 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	97851	20.000	ng/u1	0.00
20) Naphthalene-d8	10.742	136	411101	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.566	164	257602	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.301	188	472489	20.000	ng/u1	0.00
79) Chrysene-d12	21.465	240	376235	20.000	ng/u1	0.00
88) Perylene-d12	23.859	264	399168	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	8983	3.621	ng/uL	0.00
4) Pyridine-d5	3.725	84	38093	5.501	ng/u1	0.00
7) Phenol-d5	7.084	99	49590	6.049	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.254	67	173673	34.750	ng/u1	0.00
11) 2-Chlorophenol-d4	7.454	132	168992	25.730	ng/u1	0.00
15) 4-Methylphenol-d8	8.637	113	98879	15.222	ng/u1	0.00
21) Nitrobenzene-d5	9.089	128	110502	33.499	ng/u1	0.00
24) 2-Nitrophenol-d4	9.819	143	115792	32.506	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	181311	28.127	ng/u1	0.00
31) 4-Chloroaniline-d4	10.872	131	241396	27.118	ng/u1	0.00
46) Dimethylphthalate-d6	13.977	166	707840	36.771	ng/u1	0.00
49) Acenaphthylene-d8	14.260	160	825385	35.002	ng/u1	0.00
54) 4-Nitrophenol-d4	14.760	143	11632	3.537	ng/u1	0.00
60) Fluorene-d10	15.554	176	591717	36.813	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.666	200	87416	29.470	ng/u1	0.00
73) Anthracene-d10	17.401	188	879185	38.855	ng/u1	0.00
81) Pyrene-d10	19.683	212	899009	40.474	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.706	264	811534	38.707	ng/u1	0.00


Target Compounds					Qvalue
2) 1,4-Dioxane	3.325	88	69788	25.776 ng/uL#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033941.D
Acq On : 01 Feb 2022 16:09
Operator : CG/JU
Sample : N1273-18
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
COHL6

Quant Time: Feb 01 23:59:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

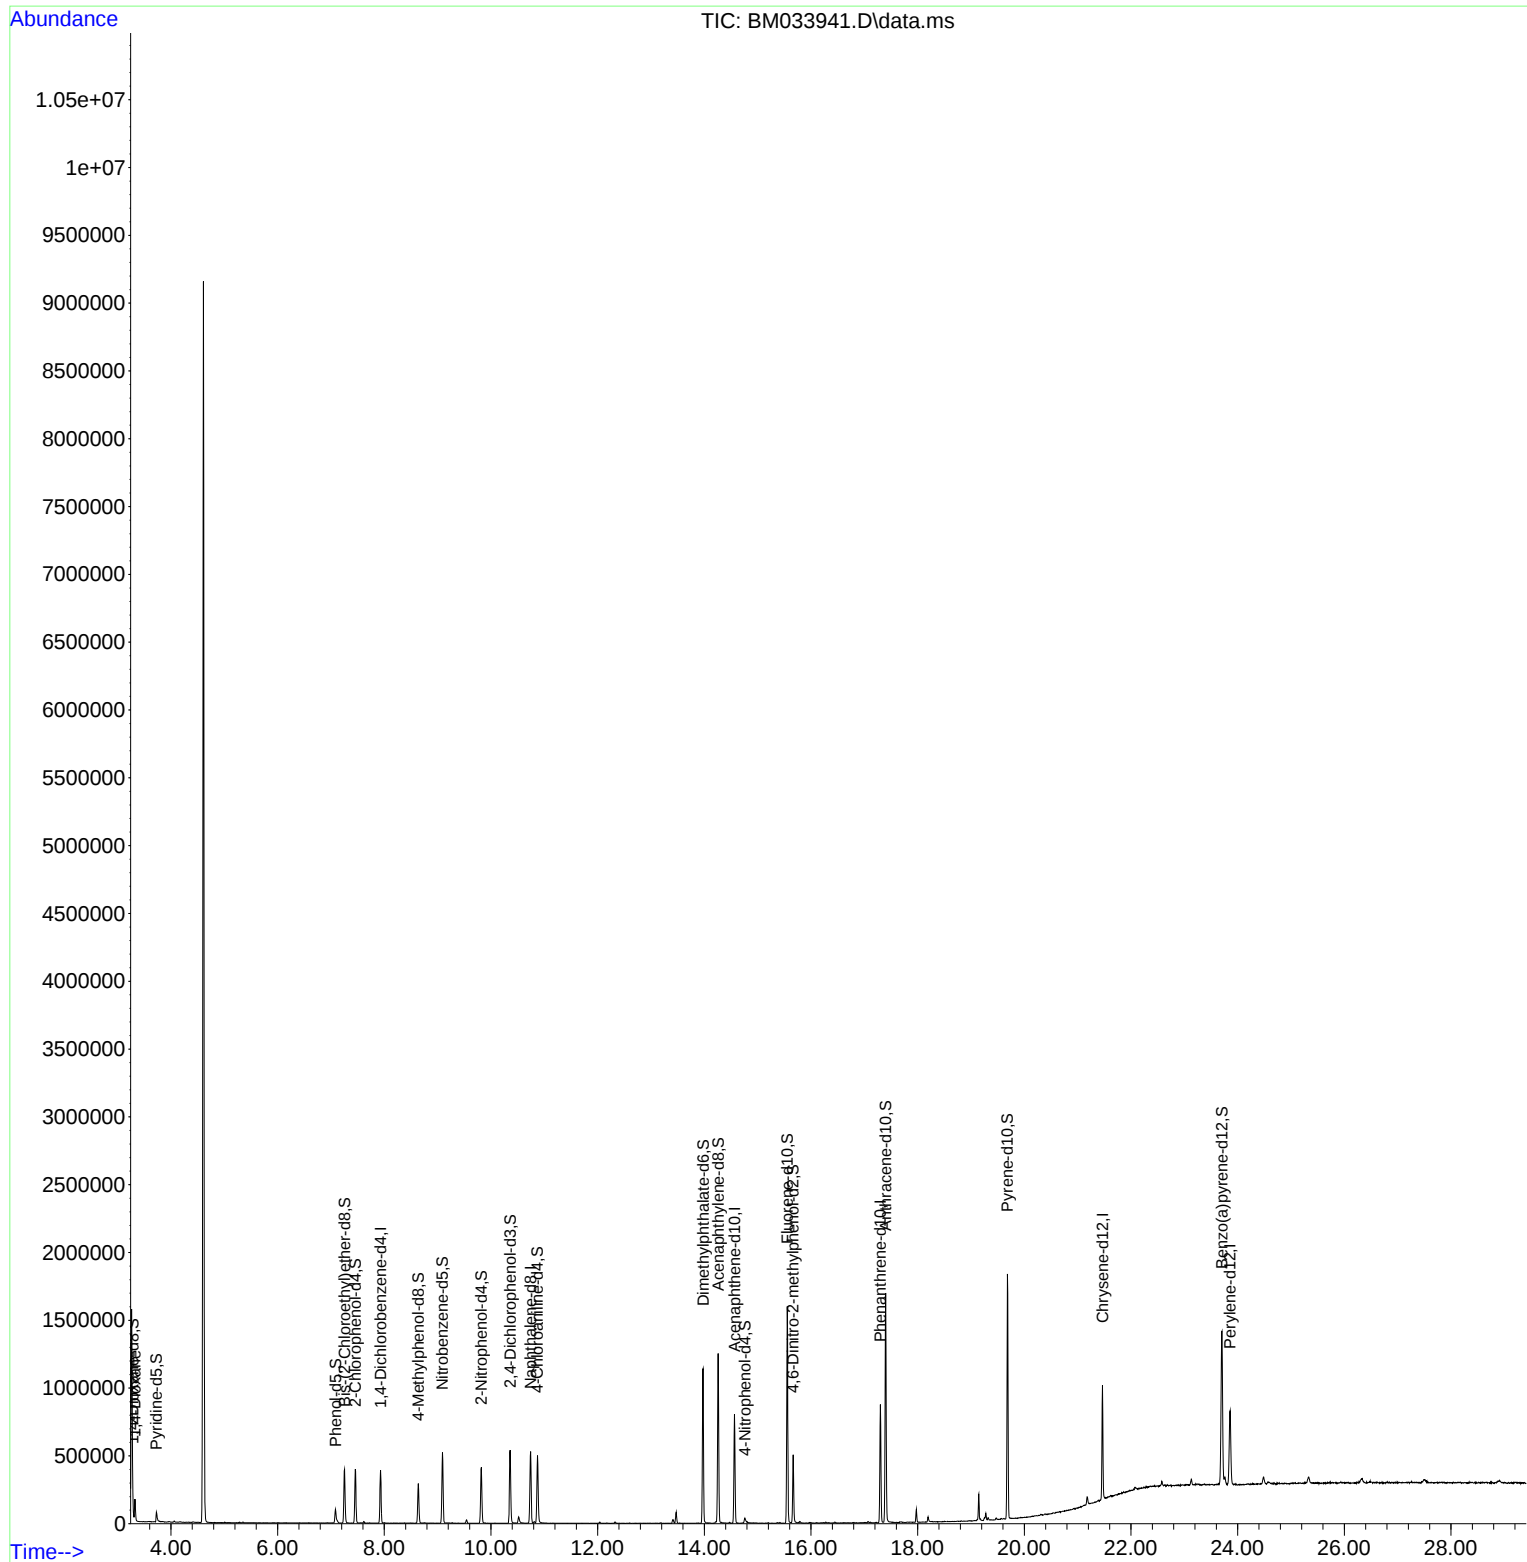

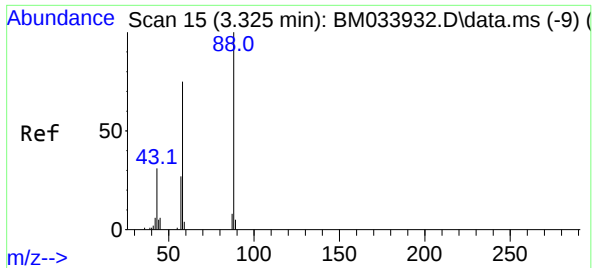

1,4-Dioxane

Concen: 25.776 ng/uL

RT: 3.325 min Scan# 11

Delta R.T. 0.000 min

Lab File: BM033941.D

Acq: 01 Feb 2022 16:09

Instrument :

BNA_M

ClientSampleId :

COHL6

Tgt Ion: 88 Resp: 69788

Ion Ratio Lower Upper

88 100

43 33.2 36.2 54.4#

58 81.0 68.5 102.7

