

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033944.D
 Acq On : 01 Feb 2022 17:56
 Operator : CG/JU
 Sample : N1273-21
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 COHL9

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 02 00:01:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.931	152	98360	20.000	ng/u1	0.00
20) Naphthalene-d8	10.742	136	425415	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.566	164	274513	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.301	188	532729	20.000	ng/u1	0.00
79) Chrysene-d12	21.465	240	412861	20.000	ng/u1	0.00
88) Perylene-d12	23.853	264	403692	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.260	96	84102m	33.722	ng/uL	-0.03
4) Pyridine-d5	3.725	84	49906	7.169	ng/u1	0.00
7) Phenol-d5	7.084	99	47734	5.793	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.248	67	186026	37.029	ng/u1	0.00
11) 2-Chlorophenol-d4	7.454	132	161149	24.409	ng/u1	0.00
15) 4-Methylphenol-d8	8.636	113	99717	15.271	ng/u1	0.00
21) Nitrobenzene-d5	9.089	128	120635	35.340	ng/u1	0.00
24) 2-Nitrophenol-d4	9.819	143	115804	31.415	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.360	165	184097	27.598	ng/u1	0.00
31) 4-Chloroaniline-d4	10.872	131	257324	27.935	ng/u1	0.00
46) Dimethylphthalate-d6	13.977	166	798824	38.941	ng/u1	0.00
49) Acenaphthylene-d8	14.260	160	925569	36.832	ng/u1	0.00
54) 4-Nitrophenol-d4	14.754	143	14366	4.099	ng/u1	0.00
60) Fluorene-d10	15.554	176	659160	38.483	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.665	200	95363	28.514	ng/u1	0.00
73) Anthracene-d10	17.401	188	1027195	40.263	ng/u1	0.00
81) Pyrene-d10	19.683	212	1061856	43.564	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.700	264	877037	41.363	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.325	88	307114	112.846	ng/uL#	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033944.D
Acq On : 01 Feb 2022 17:56
Operator : CG/JU
Sample : N1273-21
Misc :
ALS Vial : 14 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0HL9

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022


Quant Time: Feb 02 00:01:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

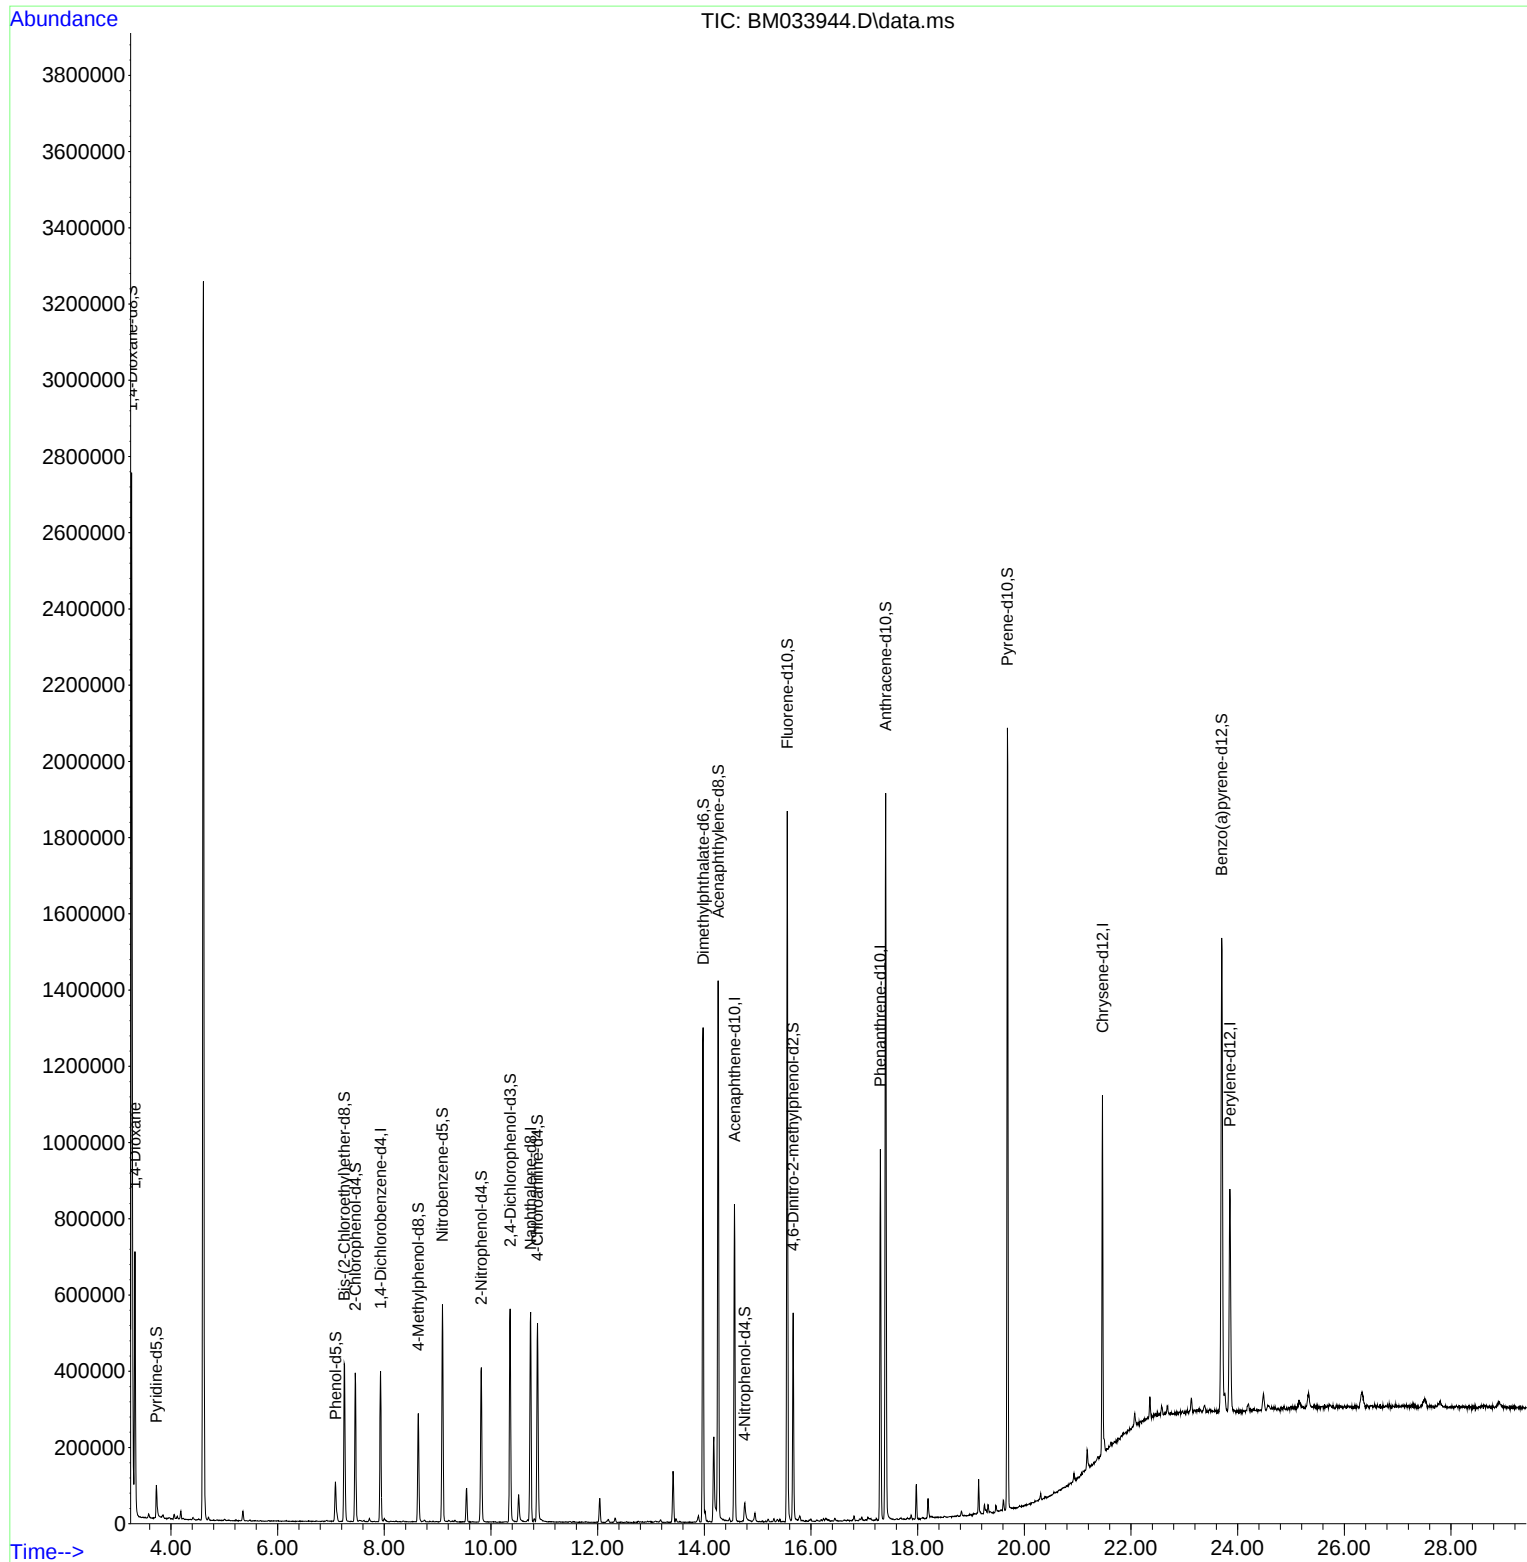

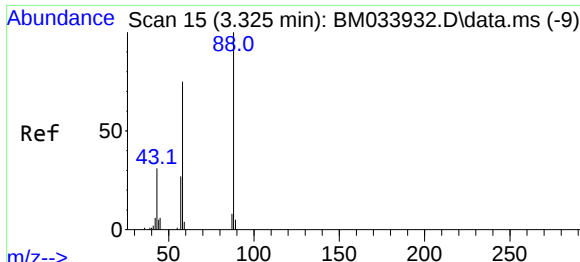

1,4-Dioxane
 Concen: 112.846 ng/uL
 RT: 3.325 min Scan# 11
 Delta R.T. 0.000 min
 Lab File: BM033944.D
 Acq: 01 Feb 2022 17:56

Instrument :
 BNA_M
 ClientSampleId :
 COHL9

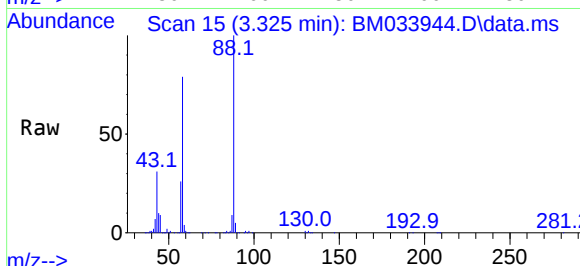

Tgt Ion: 88 Resp: 307114

Ion	Ratio	Lower	Upper
88	100		
43	31.1	36.2	54.4
58	78.8	68.5	102.7

Manual Integrations
APPROVED
 Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

