

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
 Data File : BM033952.D
 Acq On : 01 Feb 2022 23:16
 Operator : CG/JU
 Sample : N1307-04
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0Q33

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
 Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 02 01:52:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Feb 01 02:16:28 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.925	152	112528	20.000	ng/u1	0.00
20) Naphthalene-d8	10.737	136	474106	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.566	164	288829	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.301	188	538608	20.000	ng/u1	0.00
79) Chrysene-d12	21.460	240	458068	20.000	ng/u1	0.00
88) Perylene-d12	23.853	264	464652	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.290	96	13462	4.718	ng/uL	0.00
4) Pyridine-d5	3.720	84	70982	8.913	ng/u1	0.00
7) Phenol-d5	7.084	99	62638	6.644	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.249	67	184329	32.072	ng/u1	0.00
11) 2-Chlorophenol-d4	7.455	132	188031	24.895	ng/u1	0.00
15) 4-Methylphenol-d8	8.631	113	118972	15.926	ng/u1	-0.01
21) Nitrobenzene-d5	9.090	128	119726	31.472	ng/u1	0.00
24) 2-Nitrophenol-d4	9.813	143	122020	29.702	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.354	165	196719	26.461	ng/u1	0.00
31) 4-Chloroaniline-d4	10.872	131	265678m	25.879	ng/u1	0.00
46) Dimethylphthalate-d6	13.972	166	732549	33.941	ng/u1	0.00
49) Acenaphthylene-d8	14.260	160	850305	32.160	ng/u1	0.00
54) 4-Nitrophenol-d4	14.760	143	14483	3.928	ng/u1	0.00
60) Fluorene-d10	15.554	176	597752	33.168	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.666	200	86685	25.636	ng/u1	0.00
73) Anthracene-d10	17.395	188	897467	34.794	ng/u1	0.00
81) Pyrene-d10	19.683	212	957901	35.421	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.695	264	858561	35.179	ng/u1	-0.01
Target Compounds						
59) Diethylphthalate	15.378	149	50738	2.298	ng/u1	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM020122\
Data File : BM033952.D
Acq On : 01 Feb 2022 23:16
Operator : CG/JU
Sample : N1307-04
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
C0Q33

Manual Integrations
APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022
Supervised By :Yogesh Patel 02/04/2022

Quant Time: Feb 02 01:52:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM013122.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Feb 01 02:16:28 2022
Response via : Initial Calibration

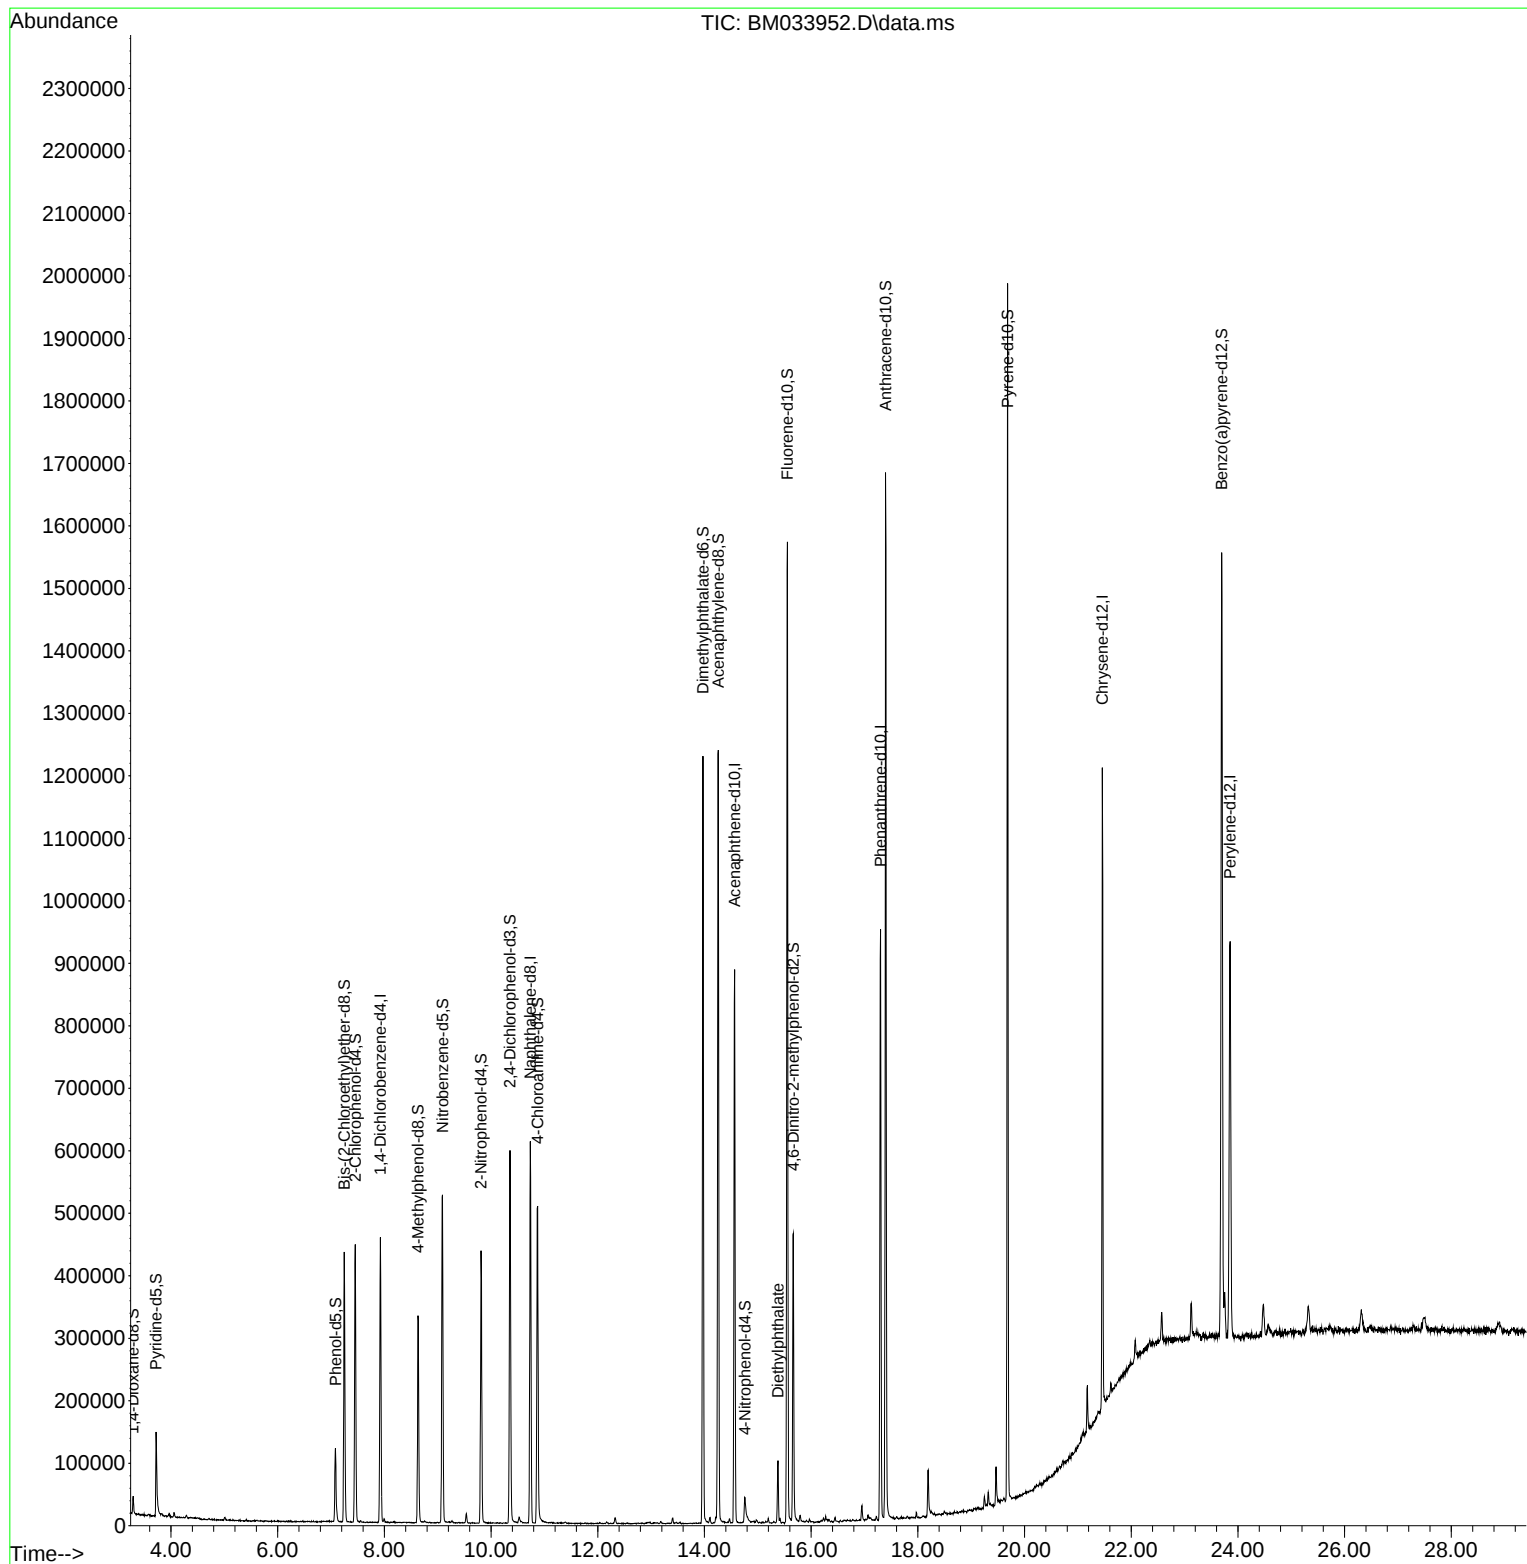

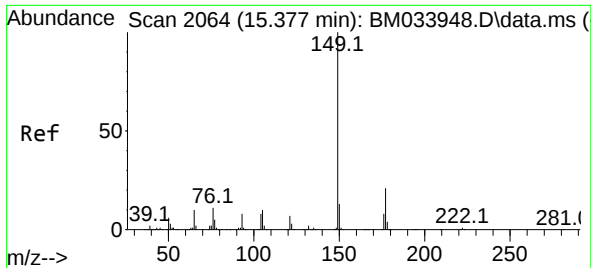

#59

Diethylphthalate

Concen: 2.298 ng/ul

RT: 15.378 min Scan# 20

Delta R.T. -0.006 min

Lab File: BM033952.D


Acq: 01 Feb 2022 23:16

Instrument :

BNA_M

ClientSampleId :

C0Q33

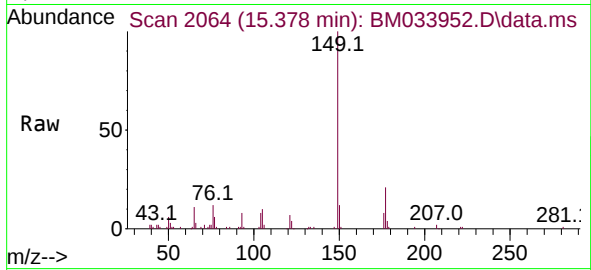

Tgt Ion:149 Resp: 50738

Ion Ratio Lower Upper

149 100

177 21.2 17.1 25.7

150 11.8 9.9 14.9

Manual Integrations

APPROVED

Reviewed By :Jagrut Upadhyay 02/02/2022

Supervised By :Yogesh Patel 02/04/2022

